

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122822\
 Data File : BF131856.D
 Acq On : 28 Dec 2022 12:01
 Operator : CG\JU
 Sample : PB149912BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB149912BL

Quant Time: Dec 29 00:51:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 05:13:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.822	152	79203	20.000	ng	-0.01
21) Naphthalene-d8	8.116	136	295706	20.000	ng	-0.01
39) Acenaphthene-d10	9.881	164	171896	20.000	ng	-0.01
64) Phenanthrene-d10	11.375	188	327788	20.000	ng	-0.01
76) Chrysene-d12	14.027	240	264554	20.000	ng	-0.01
86) Perylene-d12	15.515	264	211951	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.446	112	660693	138.241	ng	0.00
7) Phenol-d6	6.463	99	864980	137.756	ng	0.00
23) Nitrobenzene-d5	7.393	82	595533	80.408	ng	-0.02
42) 2,4,6-Tribromophenol	10.675	330	230959	123.662	ng	-0.01
45) 2-Fluorobiphenyl	9.198	172	1003314	79.948	ng	-0.01
79) Terphenyl-d14	12.975	244	1218445	77.906	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122822\
Data File : BF131856.D
Acq On : 28 Dec 2022 12:01
Operator : CG\JU
Sample : PB149912BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB149912BL

Quant Time: Dec 29 00:51:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 05:13:34 2022
Response via : Initial Calibration




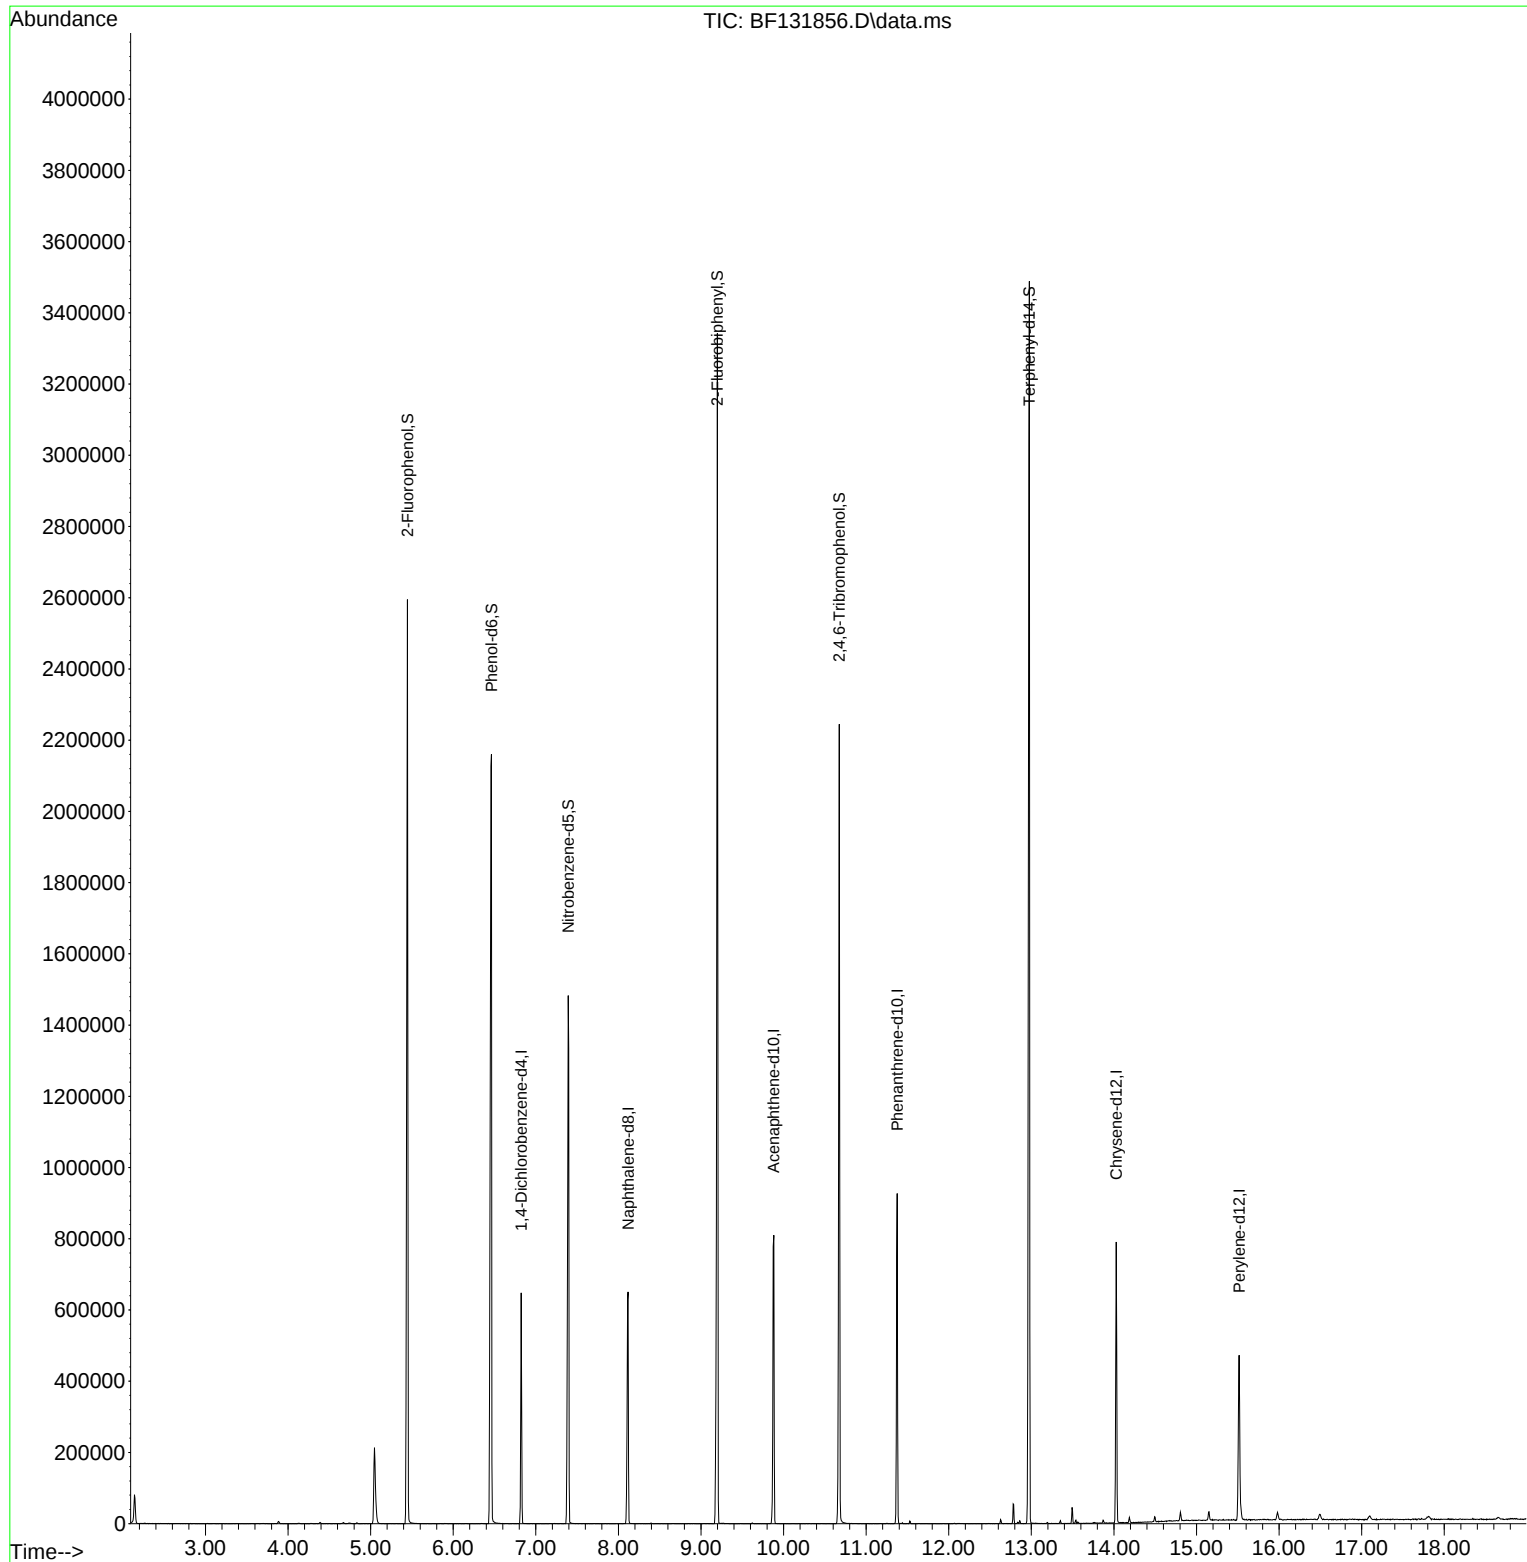


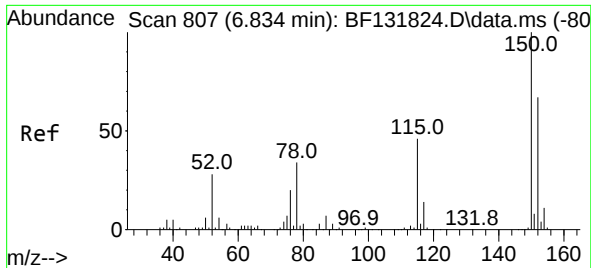

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.822 min Scan# 807
Delta R.T. -0.012 min
Lab File: BF131856.D
Acq: 28 Dec 2022 12:01




Instrument :
BNA_F
ClientSampleId :
PB149912BL


Tgt Ion:152 Resp: 79203
Ion Ratio Lower Upper
152 100
150 146.5 120.0 180.0
115 67.3 55.1 82.7

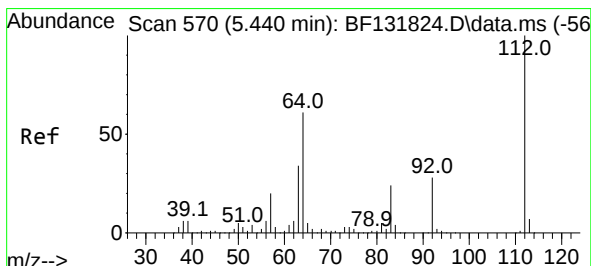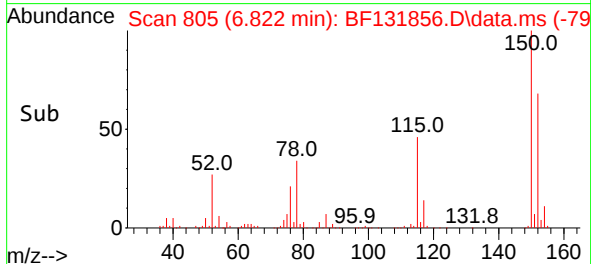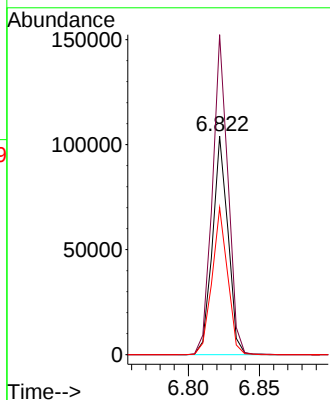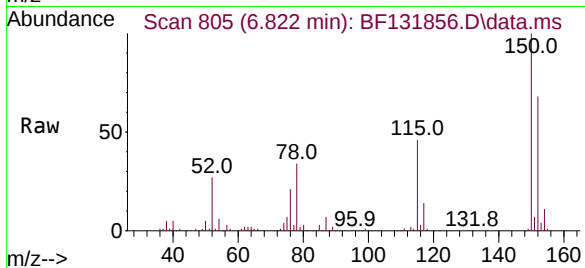

#5
2-Fluorophenol
Concen: 138.241 ng
RT: 5.446 min Scan# 571
Delta R.T. 0.006 min
Lab File: BF131856.D
Acq: 28 Dec 2022 12:01


Tgt Ion:112 Resp: 660693
Ion Ratio Lower Upper
112 100
64 63.9 49.2 73.8
63 35.5 27.5 41.3

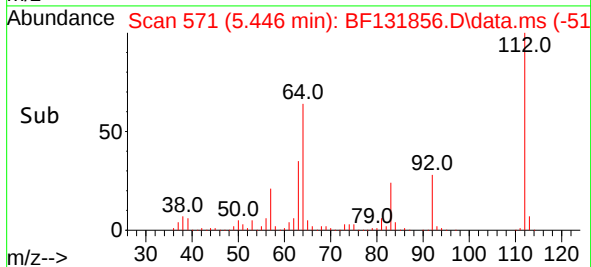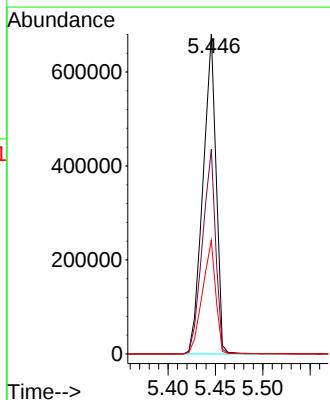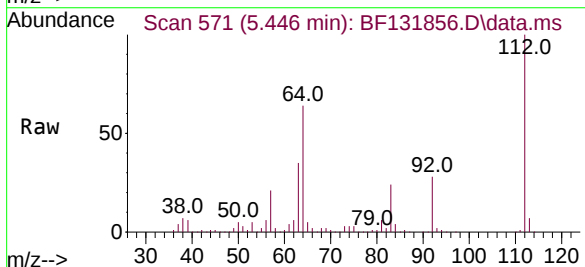



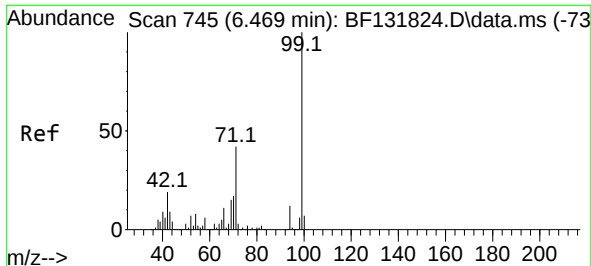


#7
Phenol-d6
Concen: 137.756 ng
RT: 6.463 min Scan# 745
Delta R.T. -0.006 min
Lab File: BF131856.D
Acq: 28 Dec 2022 12:01

Instrument :
BNA_F
ClientSampleId :
PB149912BL



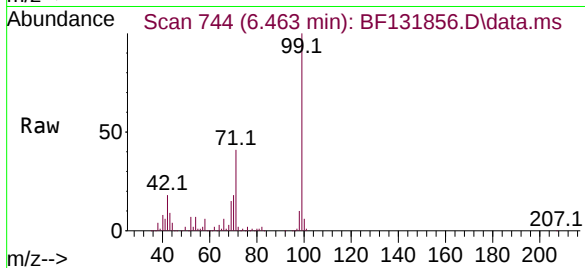



Tgt Ion: 99 Resp: 864980
Ion Ratio Lower Upper
99 100
42 18.0 15.3 22.9
71 41.3 33.5 50.3

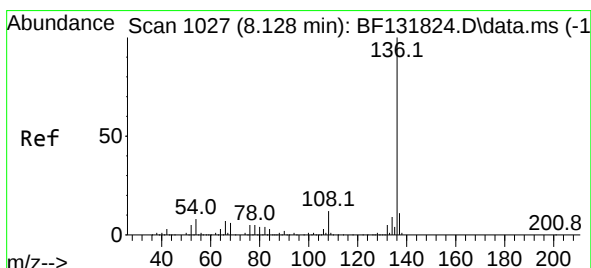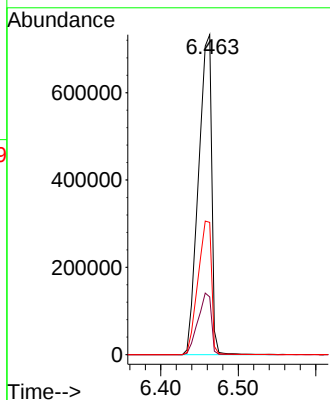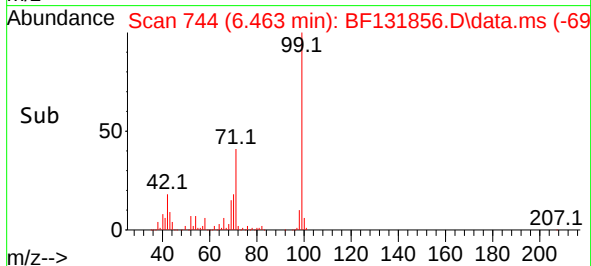

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.116 min Scan# 1025
Delta R.T. -0.012 min
Lab File: BF131856.D
Acq: 28 Dec 2022 12:01

Tgt Ion: 136 Resp: 295706
Ion Ratio Lower Upper
136 100
137 10.7 8.6 12.8
54 7.6 6.7 10.1
68 5.5 4.8 7.2


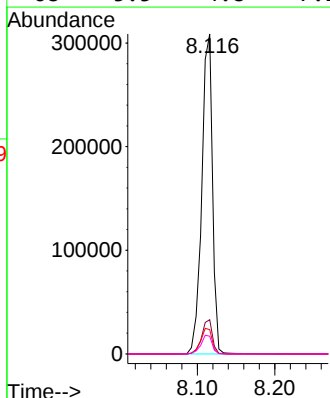
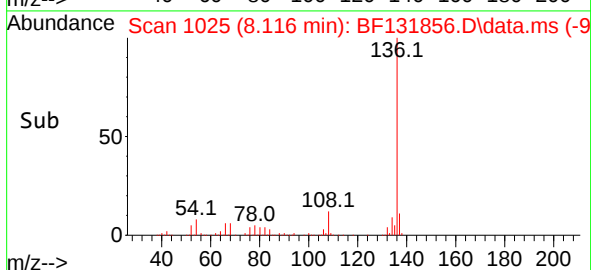
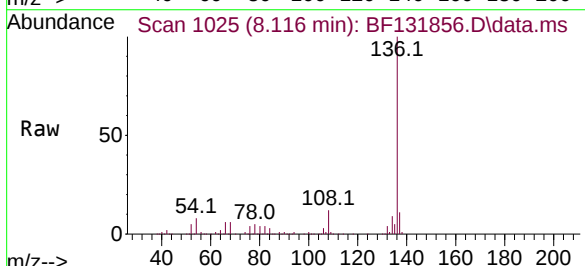


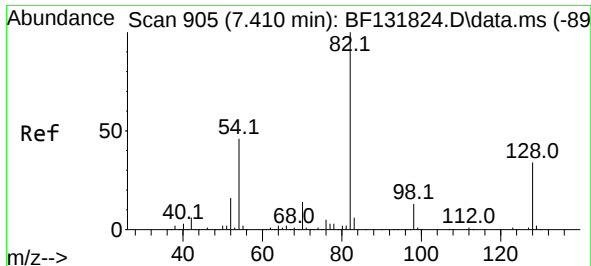

#23
Nitrobenzene-d5
Concen: 80.408 ng
RT: 7.393 min Scan# 905
Delta R.T. -0.018 min
Lab File: BF131856.D
Acq: 28 Dec 2022 12:01




Instrument :
BNA_F
ClientSampleId :
PB149912BL


Tgt Ion: 82 Resp: 595533
Ion Ratio Lower Upper
82 100
128 33.8 27.1 40.7
54 48.5 37.0 55.6

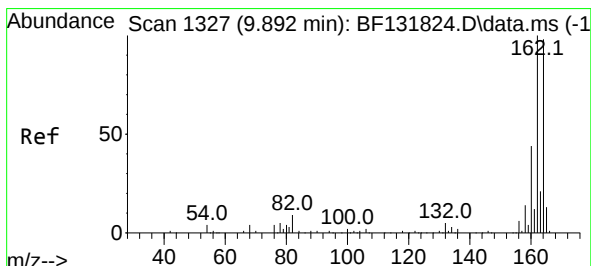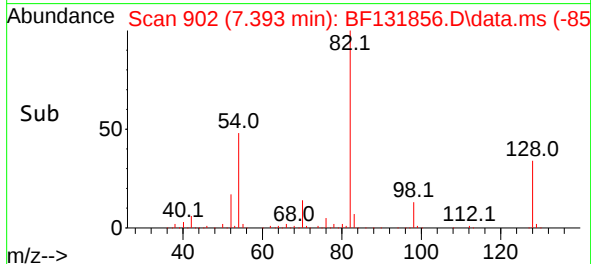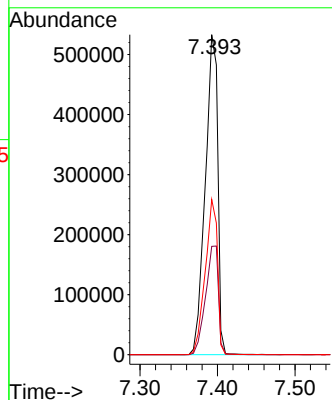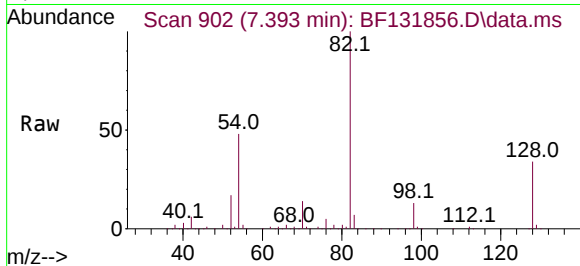

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.881 min Scan# 1325
Delta R.T. -0.012 min
Lab File: BF131856.D
Acq: 28 Dec 2022 12:01

Tgt Ion:164 Resp: 171896
Ion Ratio Lower Upper
164 100
162 106.2 81.8 122.6
160 44.9 35.7 53.5

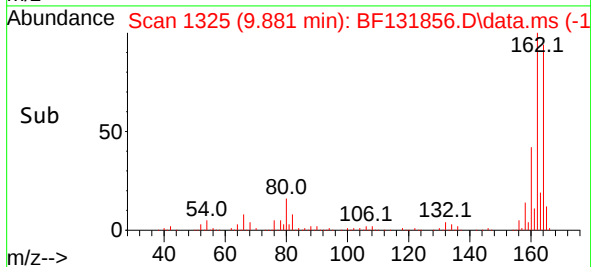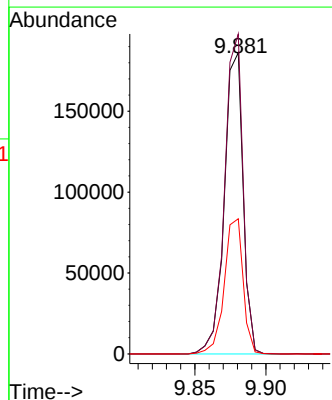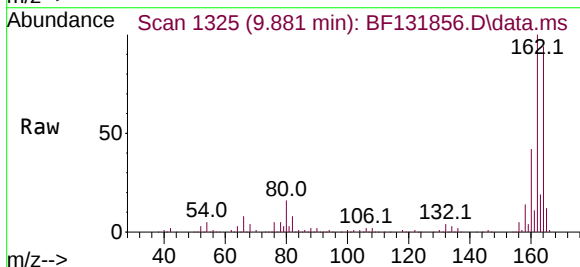

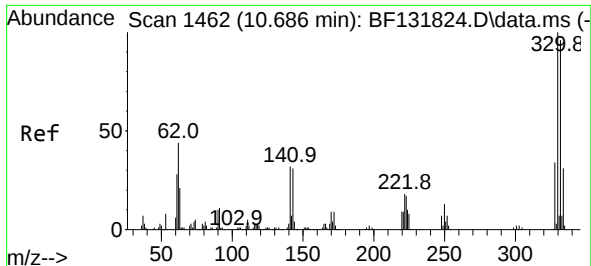

#42

2,4,6-Tribromophenol

Concen: 123.662 ng

RT: 10.675 min Scan# 1460

Delta R.T. -0.012 min

Lab File: BF131856.D


Acq: 28 Dec 2022 12:01

Instrument :

BNA_F

ClientSampleId :

PB149912BL

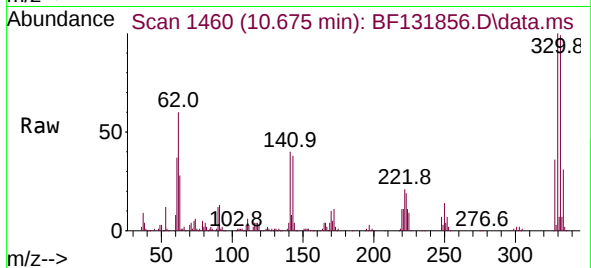




Tgt Ion:330 Resp: 230959

Ion Ratio Lower Upper

330 100

332 98.7 77.0 115.4

141 39.2 31.0 46.4

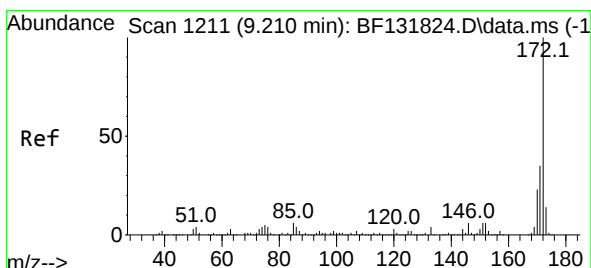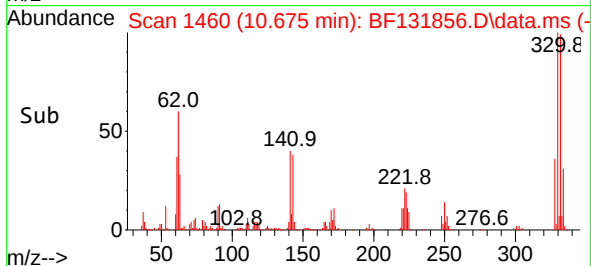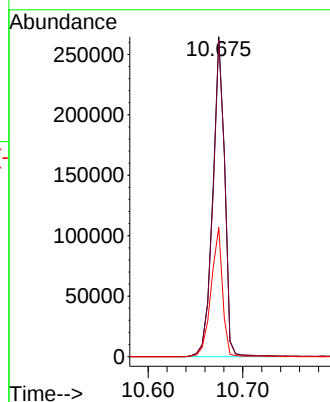

#45

2-Fluorobiphenyl

Concen: 79.948 ng

RT: 9.198 min Scan# 1209

Delta R.T. -0.012 min

Lab File: BF131856.D

Acq: 28 Dec 2022 12:01




Tgt Ion:172 Resp: 1003314


Ion Ratio Lower Upper

172 100

171 34.7 27.9 41.9

170 23.4 18.7 28.1


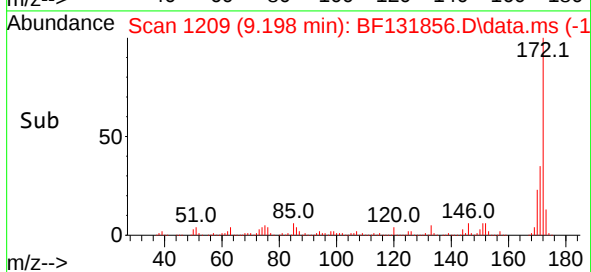
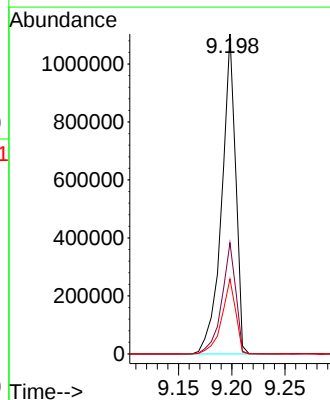
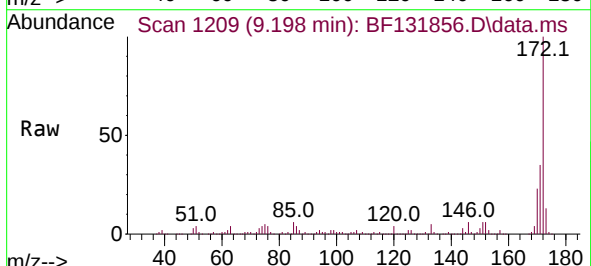


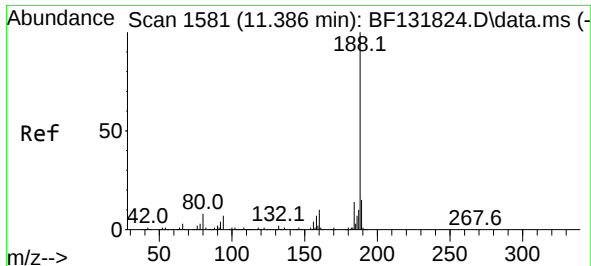

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.375 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF131856.D
Acq: 28 Dec 2022 12:01




Instrument :
BNA_F
ClientSampleId :
PB149912BL


Tgt Ion:188 Resp: 327788
Ion Ratio Lower Upper
188 100
94 7.4 5.8 8.6
80 8.7 6.7 10.1

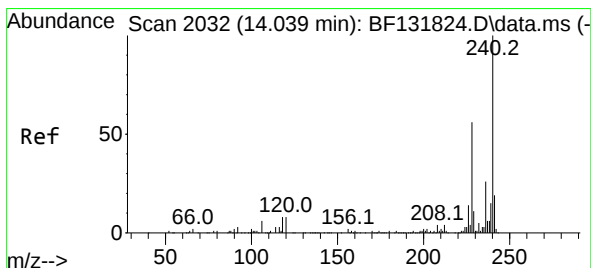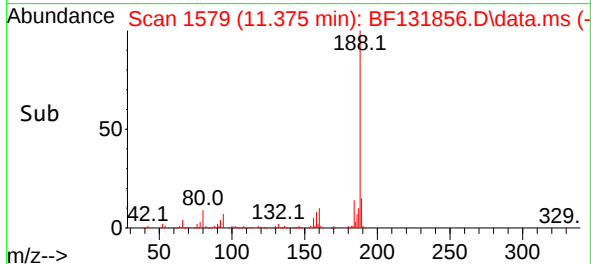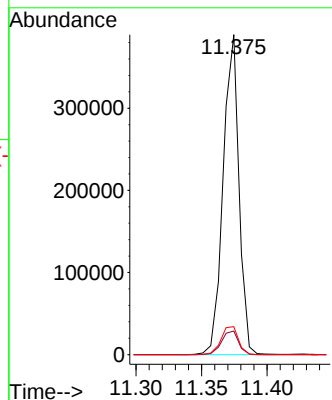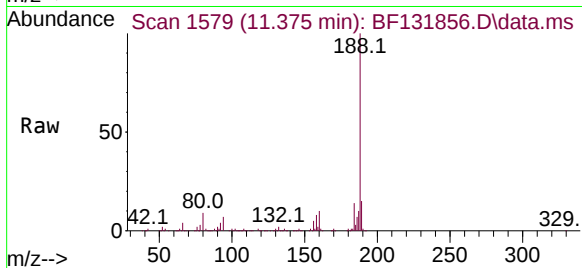

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.027 min Scan# 2030
Delta R.T. -0.012 min
Lab File: BF131856.D
Acq: 28 Dec 2022 12:01


Tgt Ion:240 Resp: 264554
Ion Ratio Lower Upper
240 100
120 8.2 6.7 10.1
236 25.9 20.6 31.0

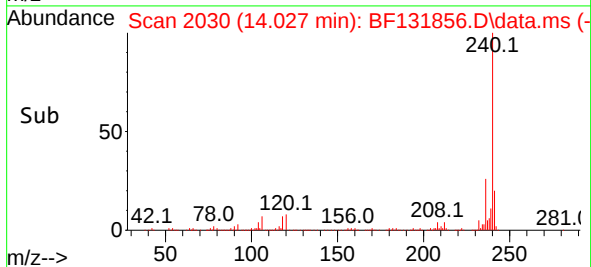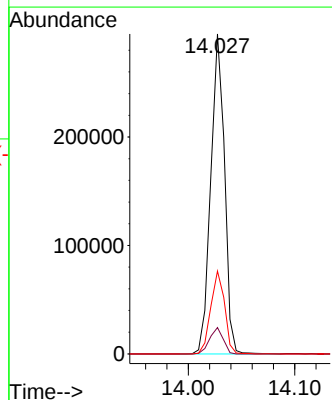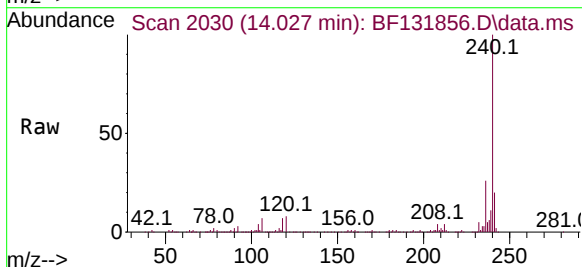



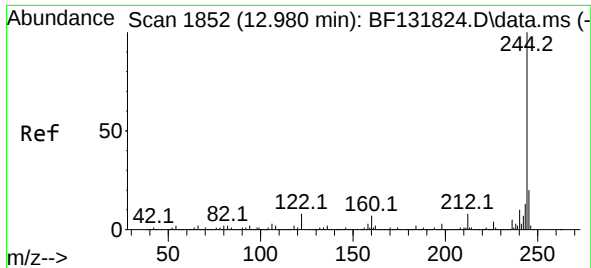


#79
 Terphenyl-d14
 Concen: 77.906 ng
 RT: 12.975 min Scan# 1851
 Delta R.T. -0.006 min
 Lab File: BF131856.D
 Acq: 28 Dec 2022 12:01

Instrument :
 BNA_F
 ClientSampleId :
 PB149912BL

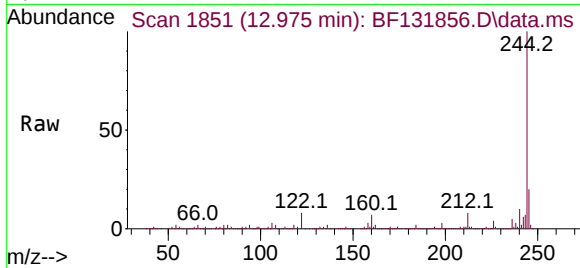

Tgt Ion:244 Resp: 1218445
 Ion Ratio Lower Upper
 244 100
 212 7.8 6.3 9.5
 122 8.0 6.4 9.6

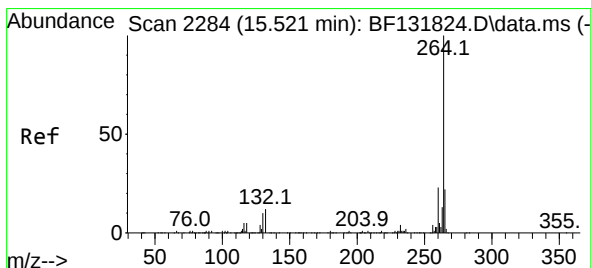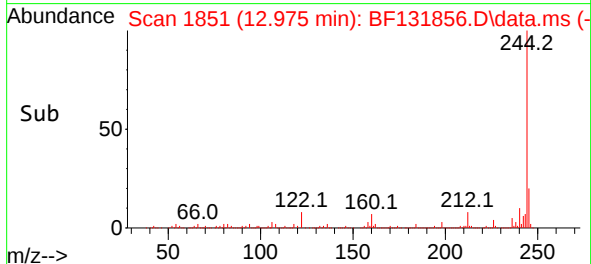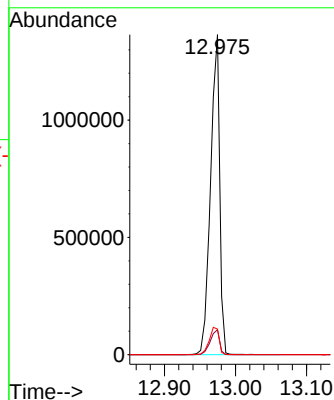

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.515 min Scan# 2283
 Delta R.T. -0.006 min
 Lab File: BF131856.D
 Acq: 28 Dec 2022 12:01

Tgt Ion:264 Resp: 211951
 Ion Ratio Lower Upper
 264 100
 260 23.7 18.6 28.0
 265 22.2 17.4 26.0

