


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122822\
 Data File : BF131853.D
 Acq On : 28 Dec 2022 10:21
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 26 05:13:34 2022

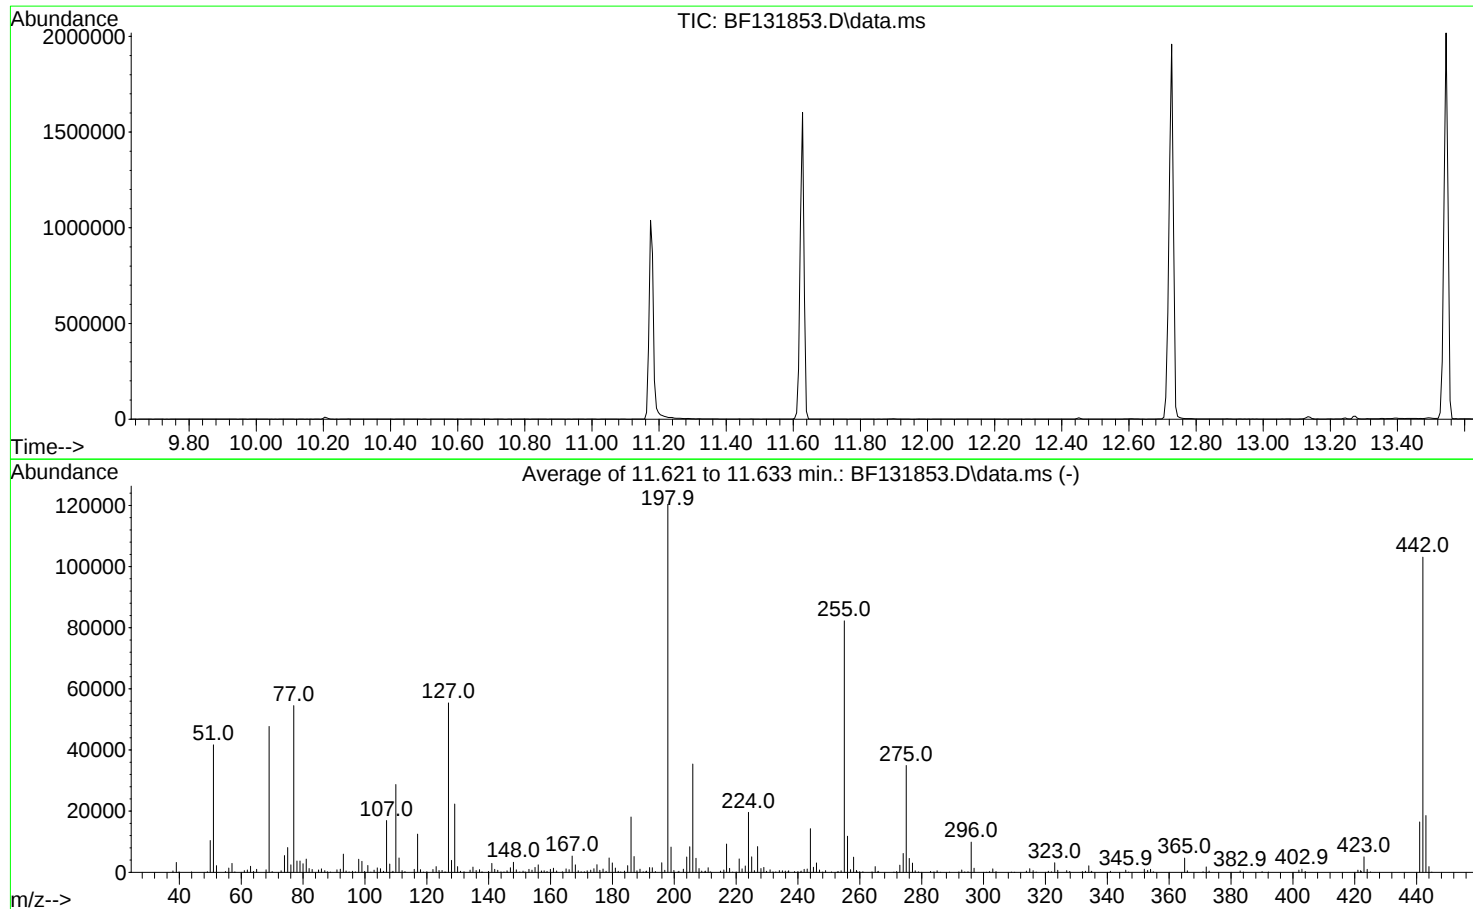




AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	41693	PASS
68	69	0.00	2	1.7	804	PASS
69	198	0.00	100	39.6	47688	PASS
70	69	0.00	2	0.5	221	PASS
127	198	10	80	46.0	55397	PASS
197	198	0.00	2	0.6	665	PASS
198	198	100	100	100.0	120336	PASS
199	198	5	9	6.8	8240	PASS
275	198	10	60	29.0	34925	PASS
365	198	1	100	3.8	4618	PASS
441	198	0.01	100	13.7	16464	PASS
442	442	50	100	100.0	103085	PASS
443	442	15	24	18.0	18561	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122822\
Data File : BF131853.D
Acq On : 28 Dec 2022 10:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 29 08:34:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 05:13:34 2022
Response via : Initial Calibration

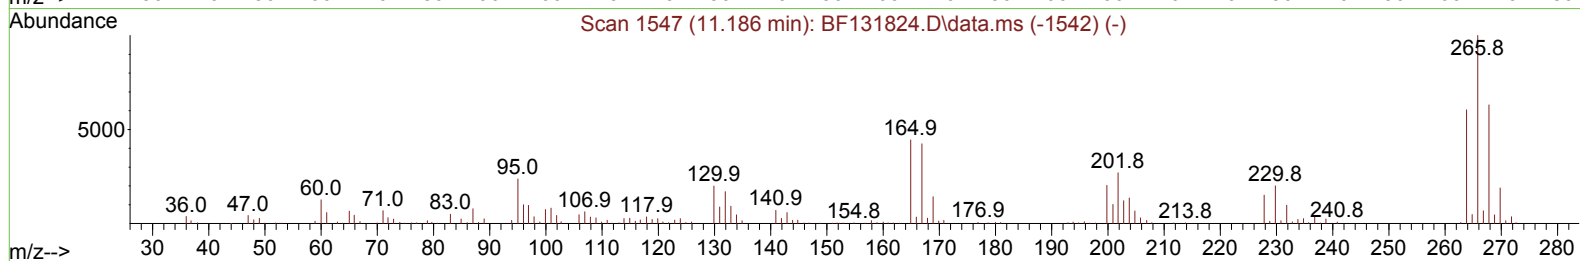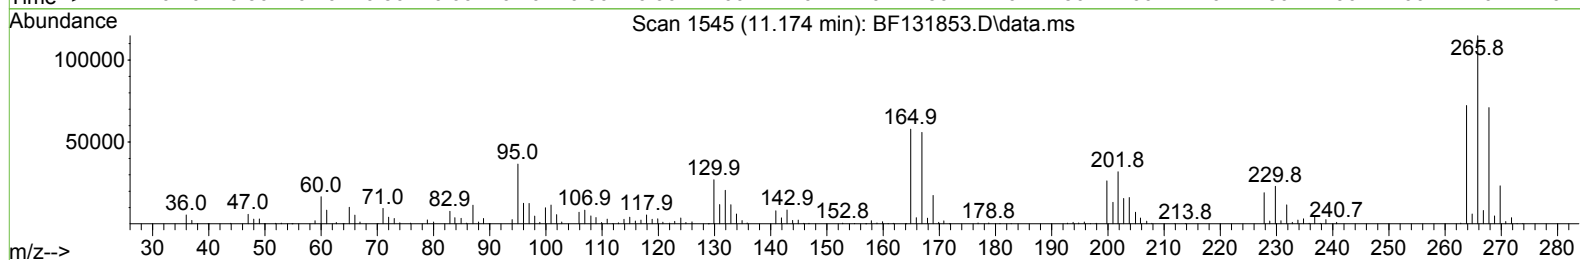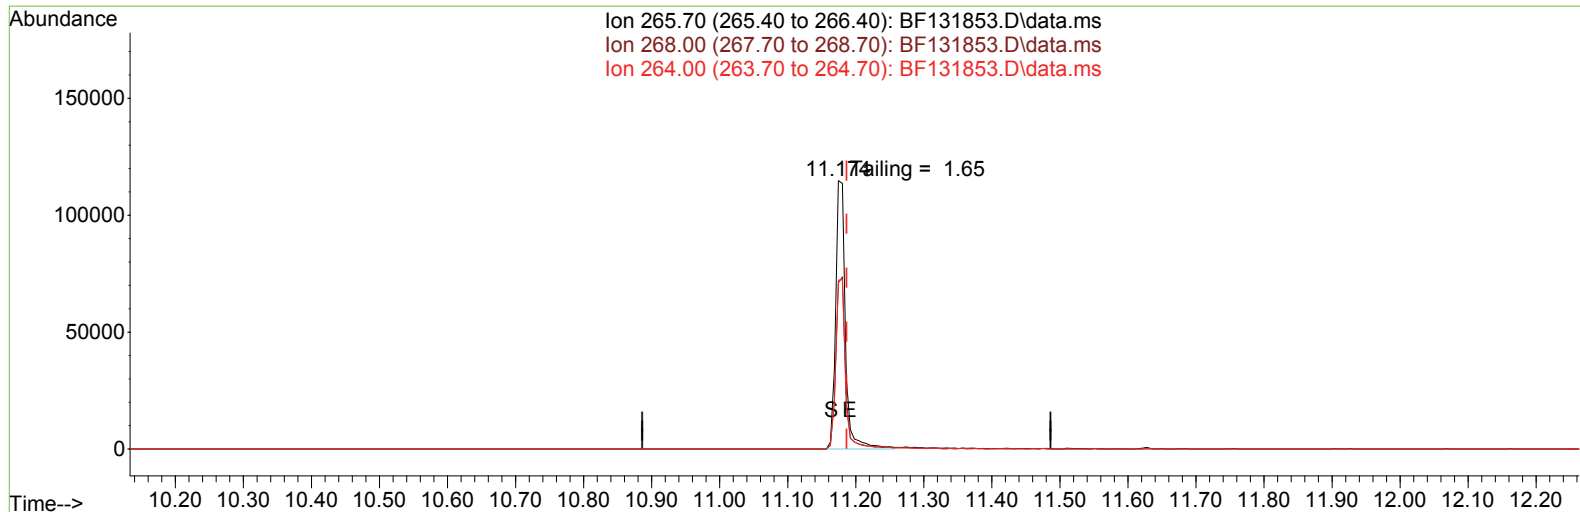

TIC: BF131853.D\data.ms

(70) Pentachlorophenol (C)

11.174min (-0.012) 33559.61 ng




response 114805

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	61.88
264.00	60.40	62.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122822\
Data File : BF131853.D
Acq On : 28 Dec 2022 10:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 29 08:34:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 05:13:34 2022
Response via : Initial Calibration

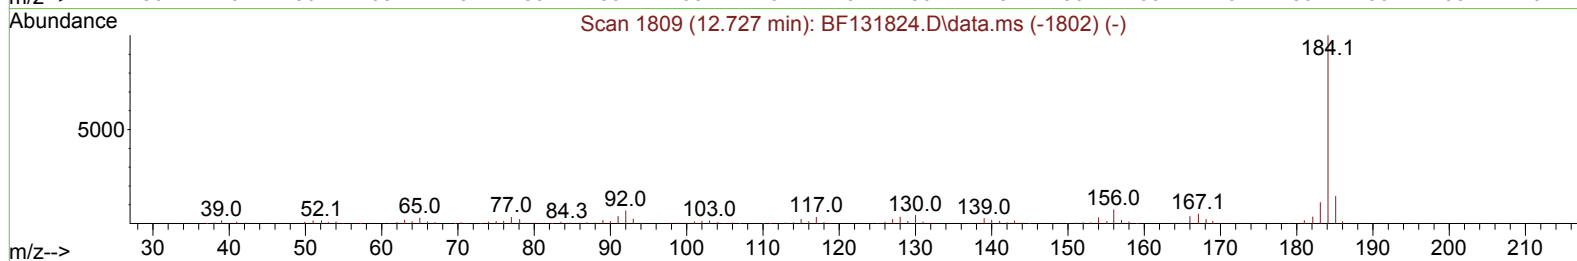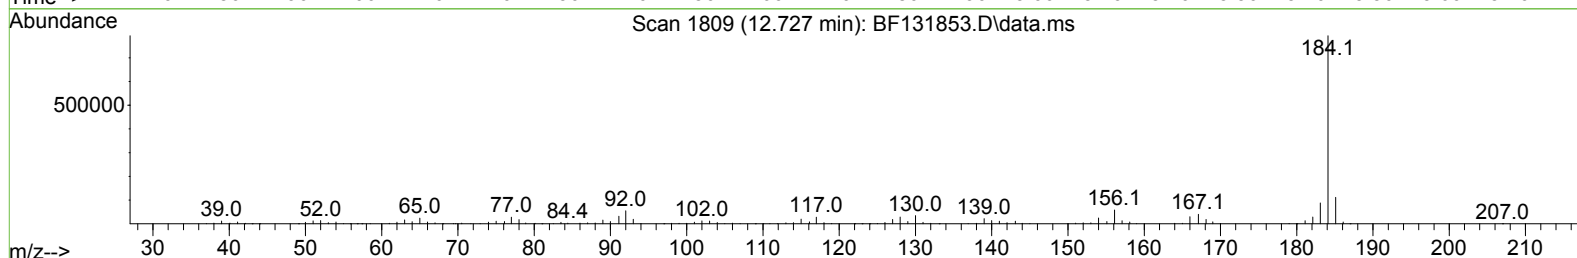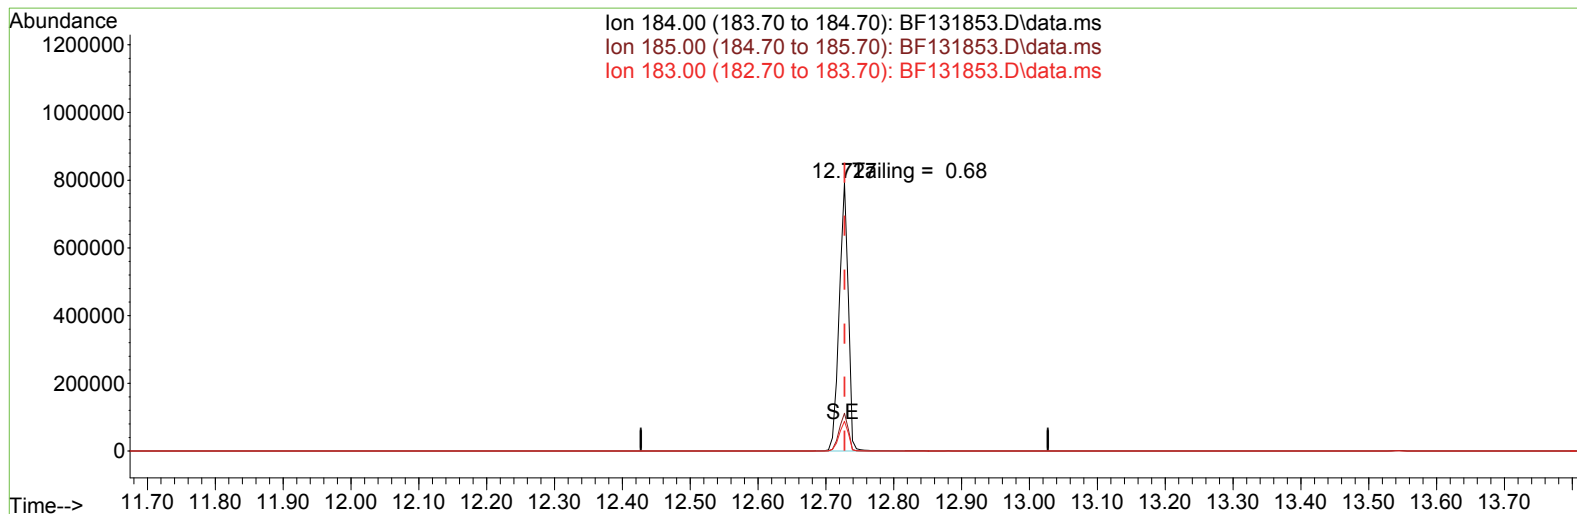

TIC: BF131853.D\data.ms

(77) Benzidine

12.727min (-0.000) 0.00 ng

response 732244

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.10
183.00	11.20	11.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/28/2022	BNA_F	<u>BF131853.D</u>
Compound Name	Response	Retention Time
DDT	329074	13.545
DDD	4222	13.274
DDE	82	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4304	333378	1.29

Instrument :
BNA_F
ClientSampleId :
DFTPP