

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122823\
 Data File : BF136786.D
 Acq On : 28 Dec 2023 10:37
 Operator : CG\JU
 Sample : PB157800BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157800BL

Quant Time: Dec 28 11:02:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.781	152	74445	20.000	ng	-0.01
21) Naphthalene-d8	8.057	136	284163	20.000	ng	-0.01
39) Acenaphthene-d10	9.816	164	147860	20.000	ng	-0.01
64) Phenanthrene-d10	11.310	188	290916	20.000	ng	0.00
76) Chrysene-d12	13.962	240	171769	20.000	ng	0.00
86) Perylene-d12	15.451	264	146547	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.439	112	629612	131.960	ng	0.01
7) Phenol-d6	6.434	99	782633	126.591	ng	0.00
23) Nitrobenzene-d5	7.345	82	486580	87.622	ng	-0.01
42) 2,4,6-Tribromophenol	10.616	330	224399	128.863	ng	0.00
45) 2-Fluorobiphenyl	9.139	172	972757	88.485	ng	-0.01
79) Terphenyl-d14	12.910	244	1023041	83.232	ng	0.00
Target Compounds						Qvalue
19) n-Nitroso-di-n-propyla...	7.345	70	64296	17.156	ng	# 72
25) Isophorone	7.345	82	484510	47.949	ng	# 65
50) Dimethylphthalate	9.816	163	28463	2.635	ng	# 1
51) 2,6-Dinitrotoluene	9.816	165	18621	7.597	ng	# 30
57) 2,4-Dinitrotoluene	9.816	165	18621	5.852	ng	# 21
67) 4-Bromophenyl-phenylether	10.616	248	13070	4.045	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122823\
Data File : BF136786.D
Acq On : 28 Dec 2023 10:37
Operator : CG\JU
Sample : PB157800BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157800BL

Quant Time: Dec 28 11:02:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration



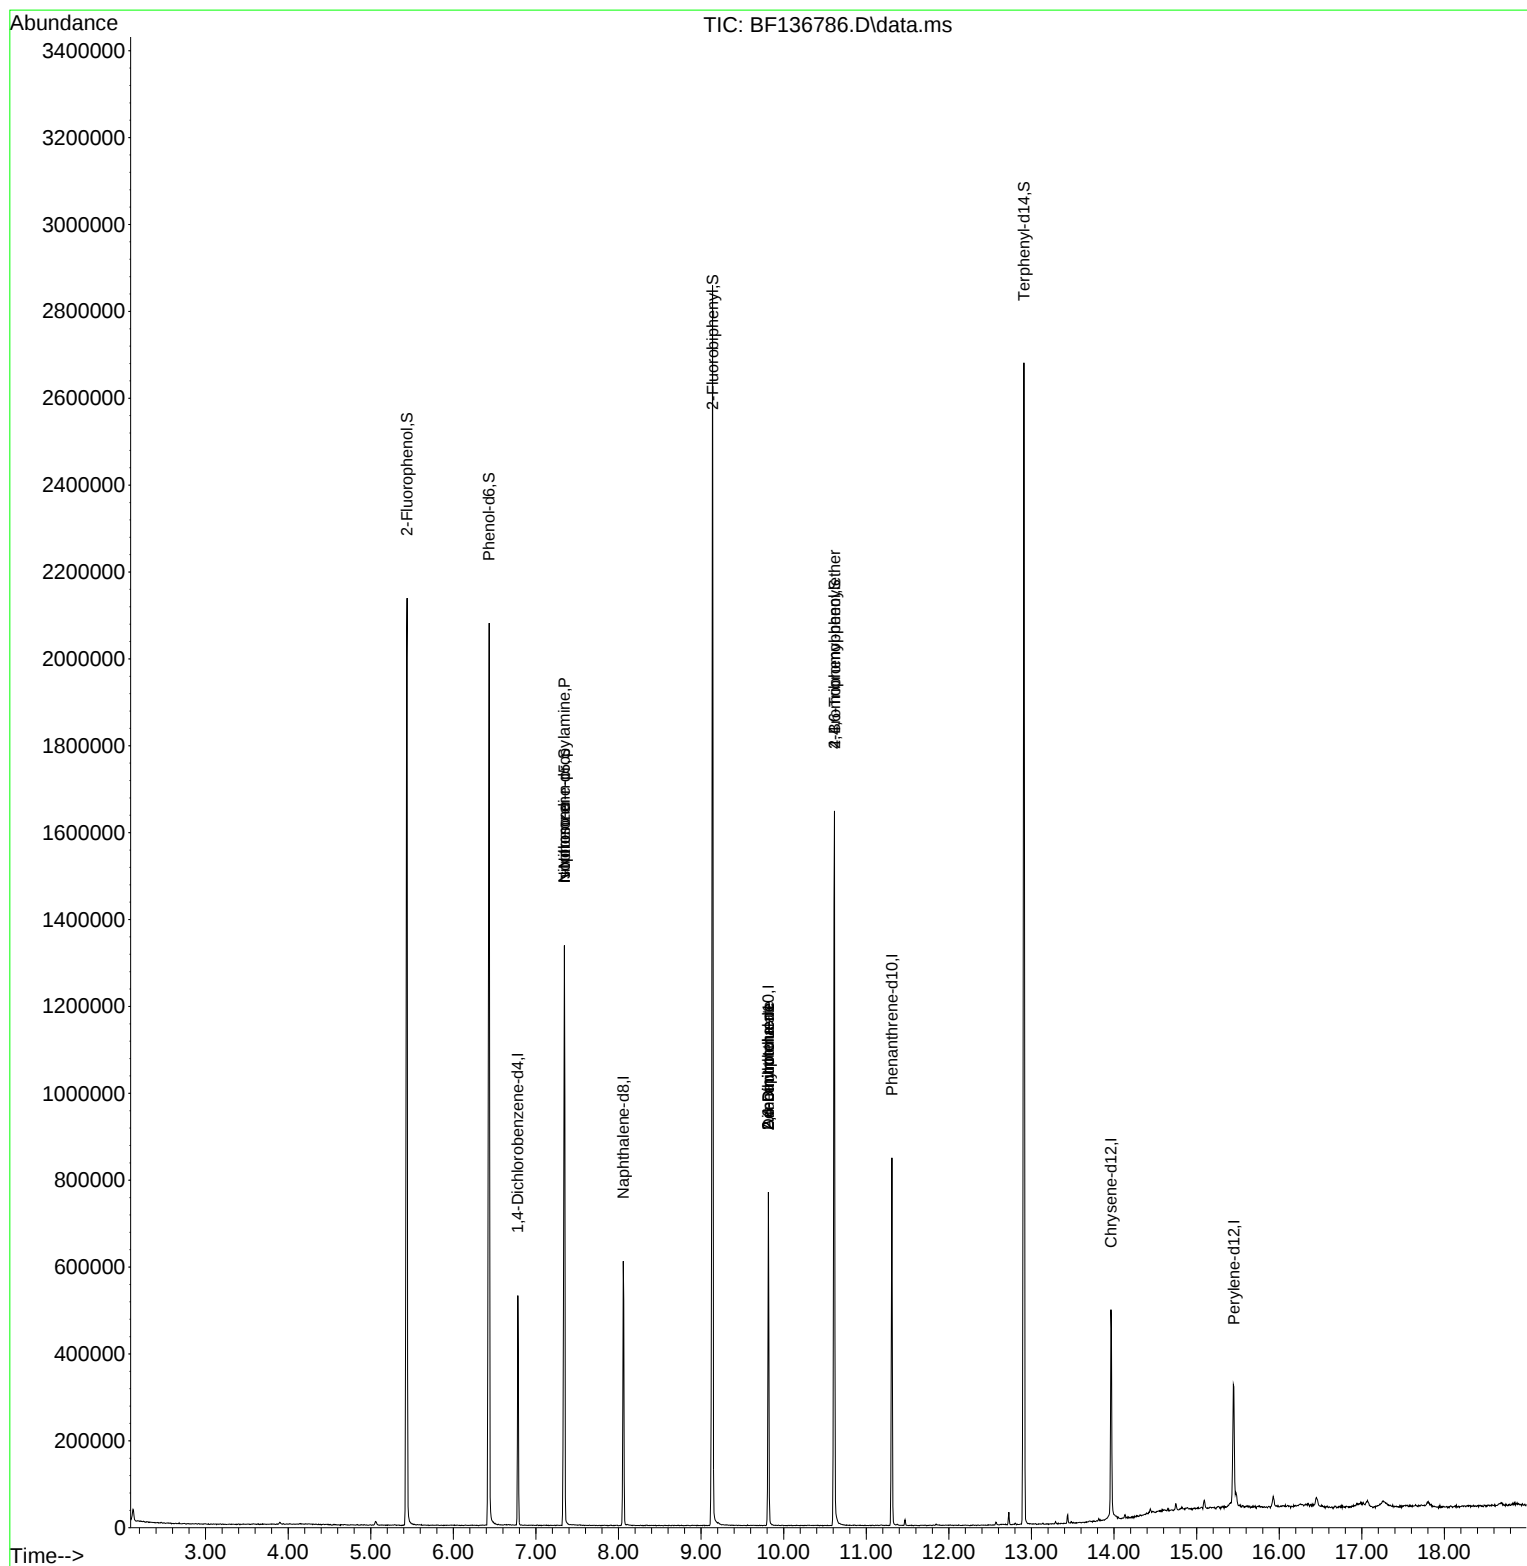




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.781 min Scan# 71
Delta R.T. -0.011 min
Lab File: BF136786.D
Acq: 28 Dec 2023 10:37




Instrument :
BNA_F
ClientSampleId :
PB157800BL


Tgt Ion:152 Resp: 74445
Ion Ratio Lower Upper
152 100
150 161.2 127.0 190.6
115 61.6 49.0 73.4

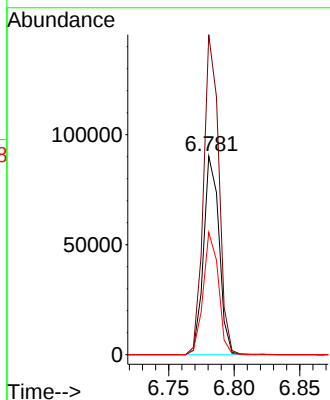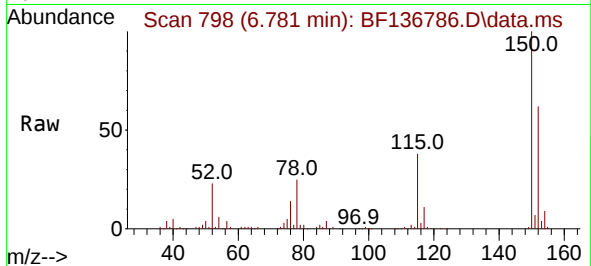

#5
2-Fluorophenol
Concen: 131.960 ng
RT: 5.439 min Scan# 570
Delta R.T. 0.012 min
Lab File: BF136786.D
Acq: 28 Dec 2023 10:37

Tgt Ion:112 Resp: 629612
Ion Ratio Lower Upper
112 100
64 58.6 51.1 76.7
63 30.0 26.1 39.1


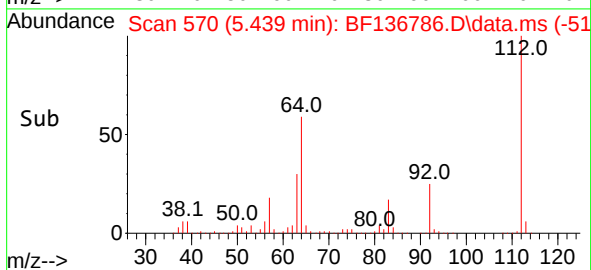
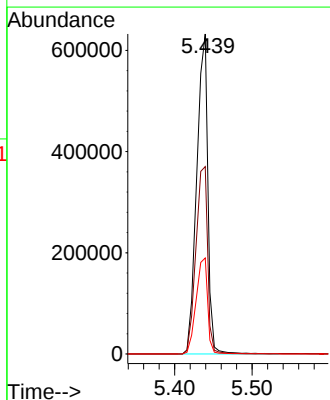



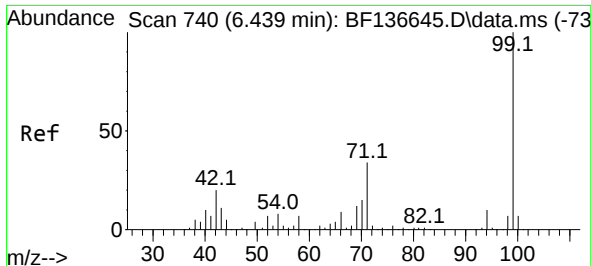

#7
Phenol-d6
Concen: 126.591 ng
RT: 6.434 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF136786.D
Acq: 28 Dec 2023 10:37




Instrument :
BNA_F
ClientSampleId :
PB157800BL

Tgt Ion: 99 Resp: 782633
Ion Ratio Lower Upper
99 100
42 19.3 16.1 24.1
71 33.7 27.4 41.2

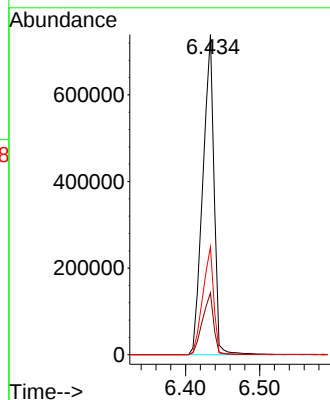

#19
n-Nitroso-di-n-propylamine
Concen: 17.156 ng
RT: 7.345 min Scan# 894
Delta R.T. 0.135 min
Lab File: BF136786.D
Acq: 28 Dec 2023 10:37

Tgt Ion: 70 Resp: 64296
Ion Ratio Lower Upper
70 100
42 48.5 54.2 81.4#
101 0.0 7.6 11.4#
130 2.2 17.1 25.7#

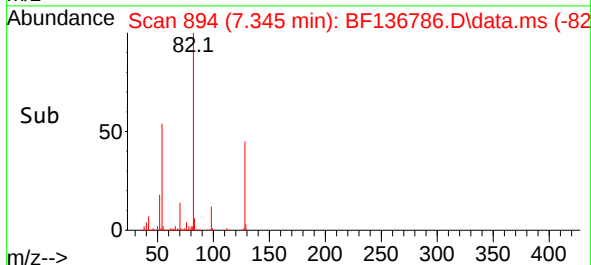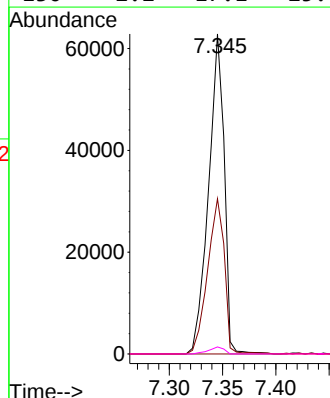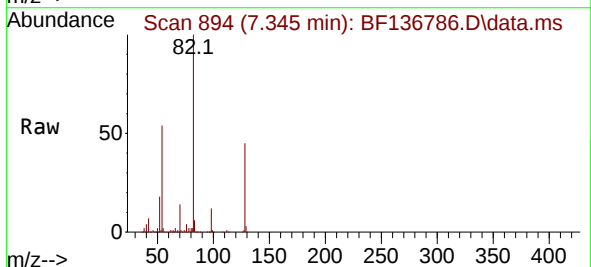







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.057 min Scan# 1017
Delta R.T. -0.012 min
Lab File: BF136786.D
Acq: 28 Dec 2023 10:37

Instrument :
BNA_F
ClientSampleId :
PB157800BL

Tgt Ion:136 Resp: 284163




Ion	Ratio	Lower	Upper
136	100		
137	10.9	9.0	13.4
54	8.9	7.2	10.8
68	5.5	4.9	7.3

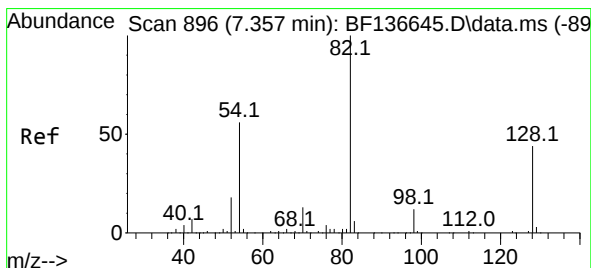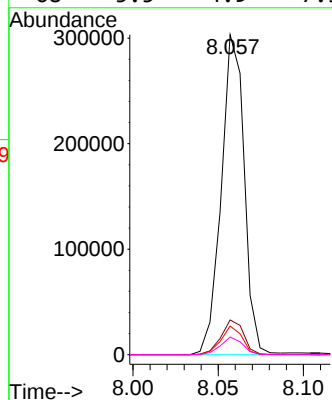

#23
Nitrobenzene-d5
Concen: 87.622 ng
RT: 7.345 min Scan# 894
Delta R.T. -0.012 min
Lab File: BF136786.D
Acq: 28 Dec 2023 10:37

Tgt Ion: 82 Resp: 486580

Ion	Ratio	Lower	Upper
82	100		
128	45.1	35.3	52.9
54	54.1	44.5	66.7


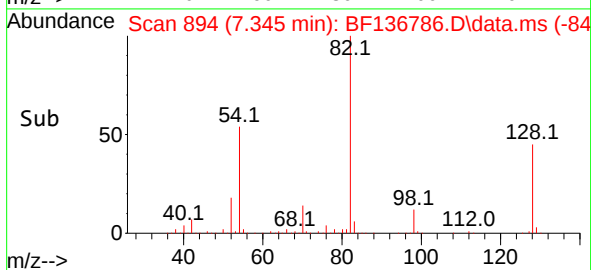
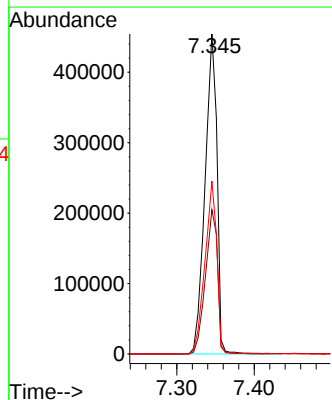
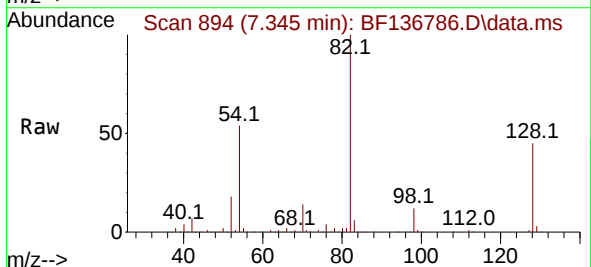




#25
Isophorone
Concen: 47.949 ng
RT: 7.345 min Scan# 894
Delta R.T. -0.271 min
Lab File: BF136786.D
Acq: 28 Dec 2023 10:37




Instrument :
BNA_F
ClientSampleId :
PB157800BL

Tgt Ion: 82 Resp: 484510
Ion Ratio Lower Upper
82 100
95 0.0 5.5 8.3#
138 0.0 14.5 21.7#

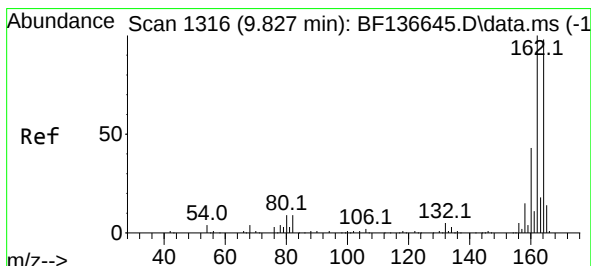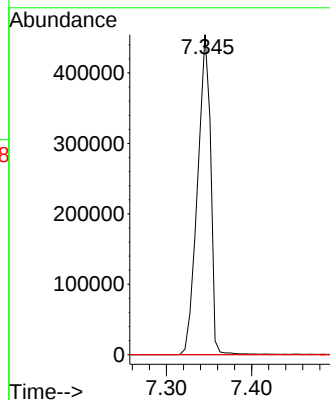

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.816 min Scan# 1314
Delta R.T. -0.012 min
Lab File: BF136786.D
Acq: 28 Dec 2023 10:37

Tgt Ion:164 Resp: 147860
Ion Ratio Lower Upper
164 100
162 102.9 81.6 122.4
160 45.1 34.9 52.3

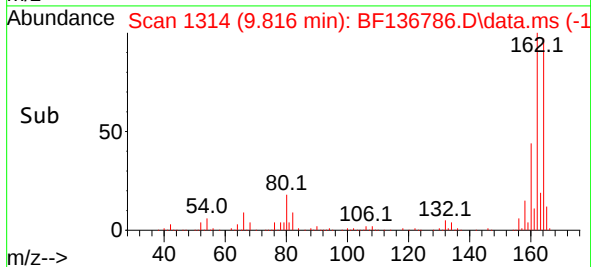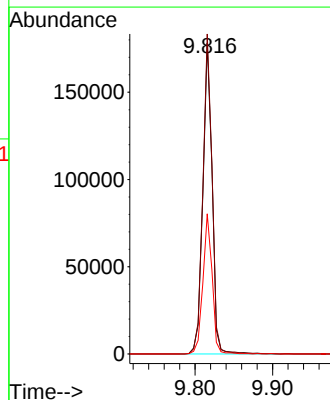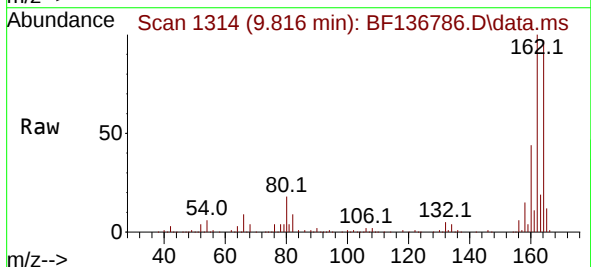



#42

2,4,6-Tribromophenol

Concen: 128.863 ng

RT: 10.616 min Scan# 1451

Delta R.T. -0.006 min

Lab File: BF136786.D

Acq: 28 Dec 2023 10:37

Instrument :

BNA_F

ClientSampleId :

PB157800BL





Tgt Ion:330 Resp: 224399

Ion Ratio Lower Upper

330 100

332 98.0 77.4 116.0

141 27.8 23.4 35.2

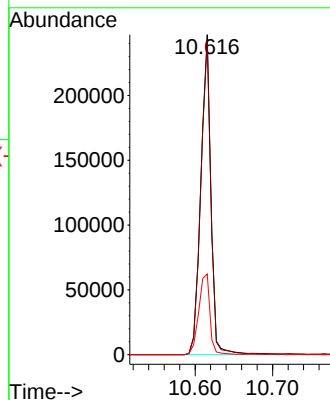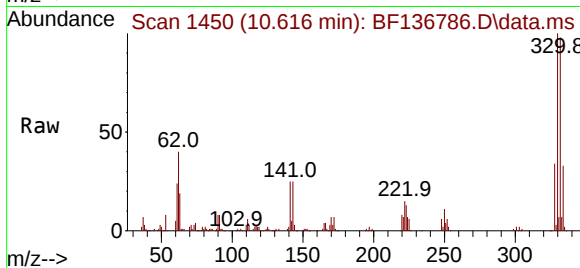

#45

2-Fluorobiphenyl

Concen: 88.485 ng

RT: 9.139 min Scan# 1199

Delta R.T. -0.012 min

Lab File: BF136786.D

Acq: 28 Dec 2023 10:37




Tgt Ion:172 Resp: 972757

Ion Ratio Lower Upper

172 100

171 35.4 29.0 43.6

170 23.1 19.0 28.4

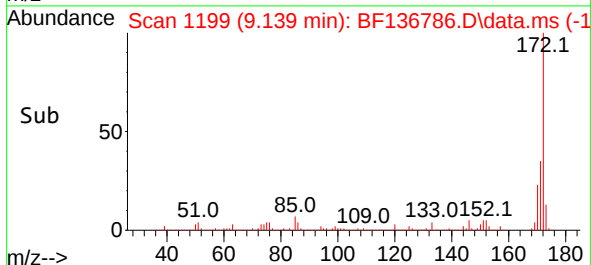
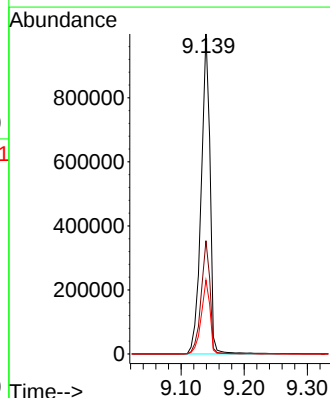
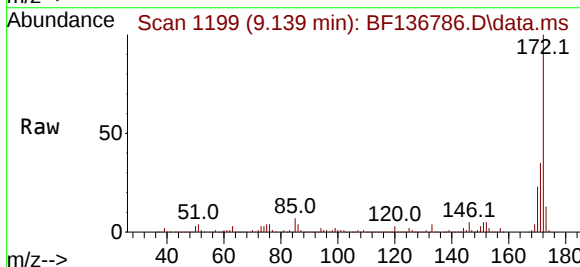




#50
Dimethylphthalate
Concen: 2.635 ng
RT: 9.816 min Scan# 1314
Delta R.T. 0.259 min
Lab File: BF136786.D
Acq: 28 Dec 2023 10:37




Instrument :
BNA_F
ClientSampleId :
PB157800BL

Tgt Ion:163 Resp: 28463
Ion Ratio Lower Upper
163 100
194 0.0 3.3 4.9#
164 519.3 7.8 11.6#

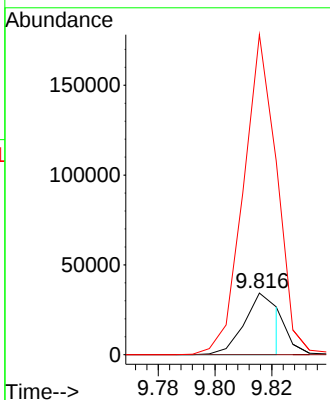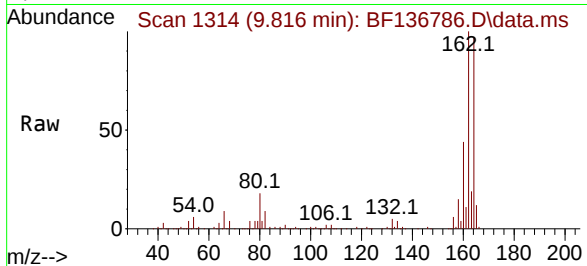

#51
2,6-Dinitrotoluene
Concen: 7.597 ng
RT: 9.816 min Scan# 1314
Delta R.T. 0.194 min
Lab File: BF136786.D
Acq: 28 Dec 2023 10:37


Tgt Ion:165 Resp: 18621
Ion Ratio Lower Upper
165 100
63 1.0 39.8 59.6#
89 1.2 38.8 58.2#

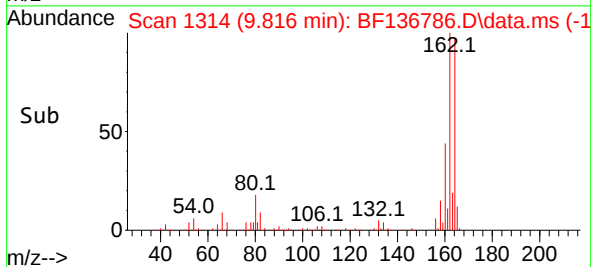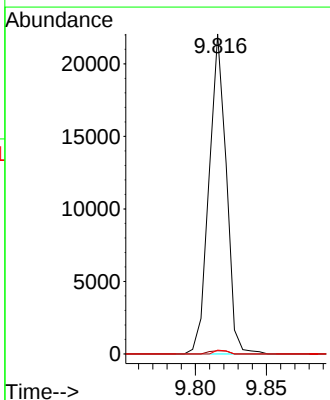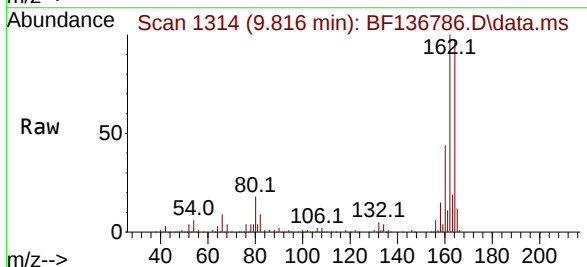






#57
2,4-Dinitrotoluene
Concen: 5.852 ng
RT: 9.816 min Scan# 11
Delta R.T. -0.206 min
Lab File: BF136786.D
Acq: 28 Dec 2023 10:37


Instrument :
BNA_F
ClientSampleId :
PB157800BL





Tgt Ion:165 Resp: 18621
Ion Ratio Lower Upper
165 100
63 1.0 41.0 61.6#
89 1.2 59.9 89.9#
182 0.0 2.0 3.0#

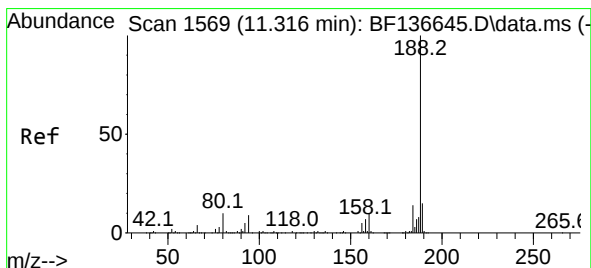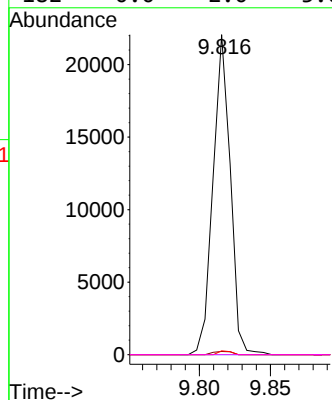


#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.310 min Scan# 1568
Delta R.T. -0.006 min
Lab File: BF136786.D
Acq: 28 Dec 2023 10:37

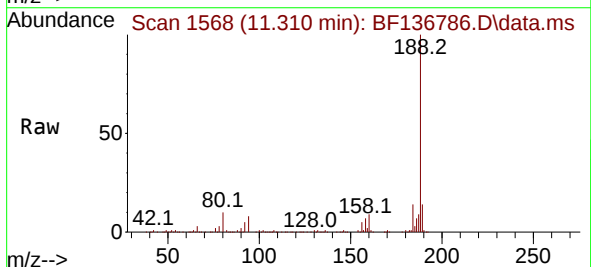

Tgt Ion:188 Resp: 290916
Ion Ratio Lower Upper
188 100
94 8.5 7.5 11.3
80 9.6 8.1 12.1



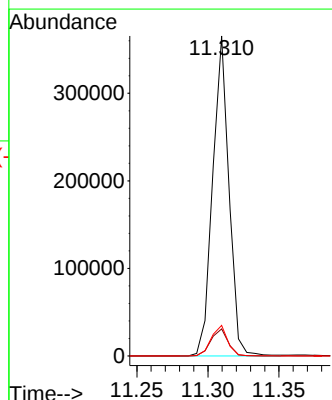



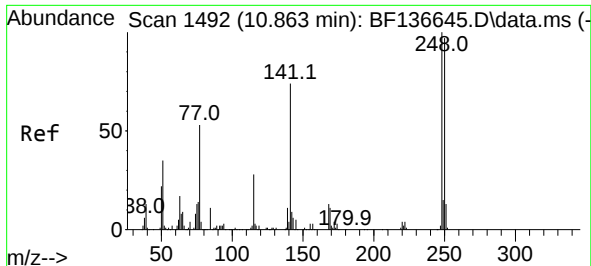

#67
4-Bromophenyl-phenylether
Concen: 4.045 ng
RT: 10.616 min Scan# 1492
Delta R.T. -0.247 min
Lab File: BF136786.D
Acq: 28 Dec 2023 10:37




Instrument :
BNA_F
ClientSampleId :
PB157800BL

Tgt Ion:248 Resp: 13070
Ion Ratio Lower Upper
248 100
250 205.1 77.8 116.6#
141 449.9 59.2 88.8#

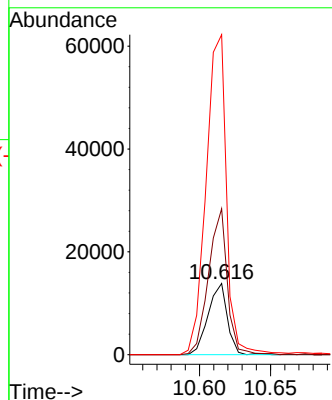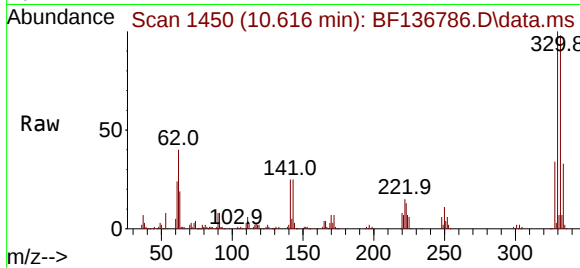

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.962 min Scan# 2019
Delta R.T. -0.006 min
Lab File: BF136786.D
Acq: 28 Dec 2023 10:37


Tgt Ion:240 Resp: 171769
Ion Ratio Lower Upper
240 100
120 12.2 10.3 15.5
236 24.9 19.4 29.2

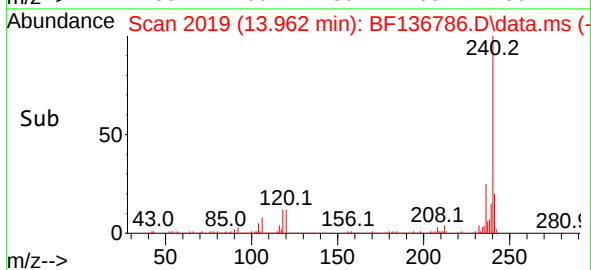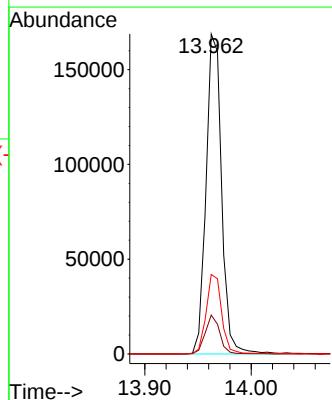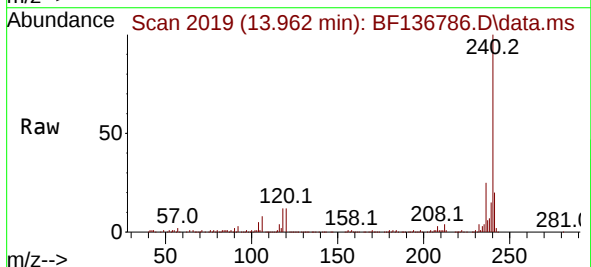






#79
 Terphenyl-d14
 Concen: 83.232 ng
 RT: 12.910 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF136786.D
 Acq: 28 Dec 2023 10:37

Instrument :
 BNA_F
 ClientSampleId :
 PB157800BL

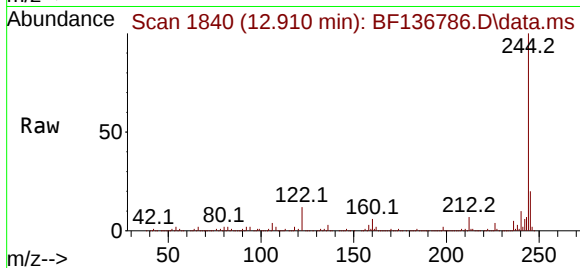

Tgt Ion:244 Resp: 1023041

Ion	Ratio	Lower	Upper
244	100		
212	6.5	5.0	7.4
122	12.1	9.0	13.4

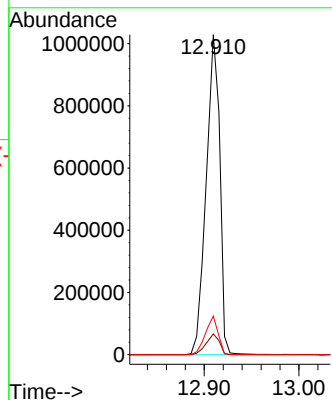

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.451 min Scan# 2272
 Delta R.T. 0.006 min
 Lab File: BF136786.D
 Acq: 28 Dec 2023 10:37

Tgt Ion:264 Resp: 146547

Ion	Ratio	Lower	Upper
264	100		
260	21.2	18.3	27.5
265	19.8	17.0	25.6

