

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122823\
 Data File : BF136788.D
 Acq On : 28 Dec 2023 11:38
 Operator : CG\JU
 Sample : PB157982TB
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157982TB

Quant Time: Dec 28 12:02:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.781	152	70689	20.000	ng	-0.01
21) Naphthalene-d8	8.057	136	270441	20.000	ng	-0.01
39) Acenaphthene-d10	9.816	164	142854	20.000	ng	-0.01
64) Phenanthrene-d10	11.310	188	286992	20.000	ng	0.00
76) Chrysene-d12	13.962	240	171287	20.000	ng	0.00
86) Perylene-d12	15.445	264	142610	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.434	112	566994	125.150	ng	0.00
7) Phenol-d6	6.434	99	706232	120.303	ng	0.00
23) Nitrobenzene-d5	7.345	82	439529	83.165	ng	-0.01
42) 2,4,6-Tribromophenol	10.616	330	200971	119.453	ng	0.00
45) 2-Fluorobiphenyl	9.139	172	891546	83.940	ng	-0.01
79) Terphenyl-d14	12.910	244	986926	80.520	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122823\
Data File : BF136788.D
Acq On : 28 Dec 2023 11:38
Operator : CG\JU
Sample : PB157982TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157982TB

Quant Time: Dec 28 12:02:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration



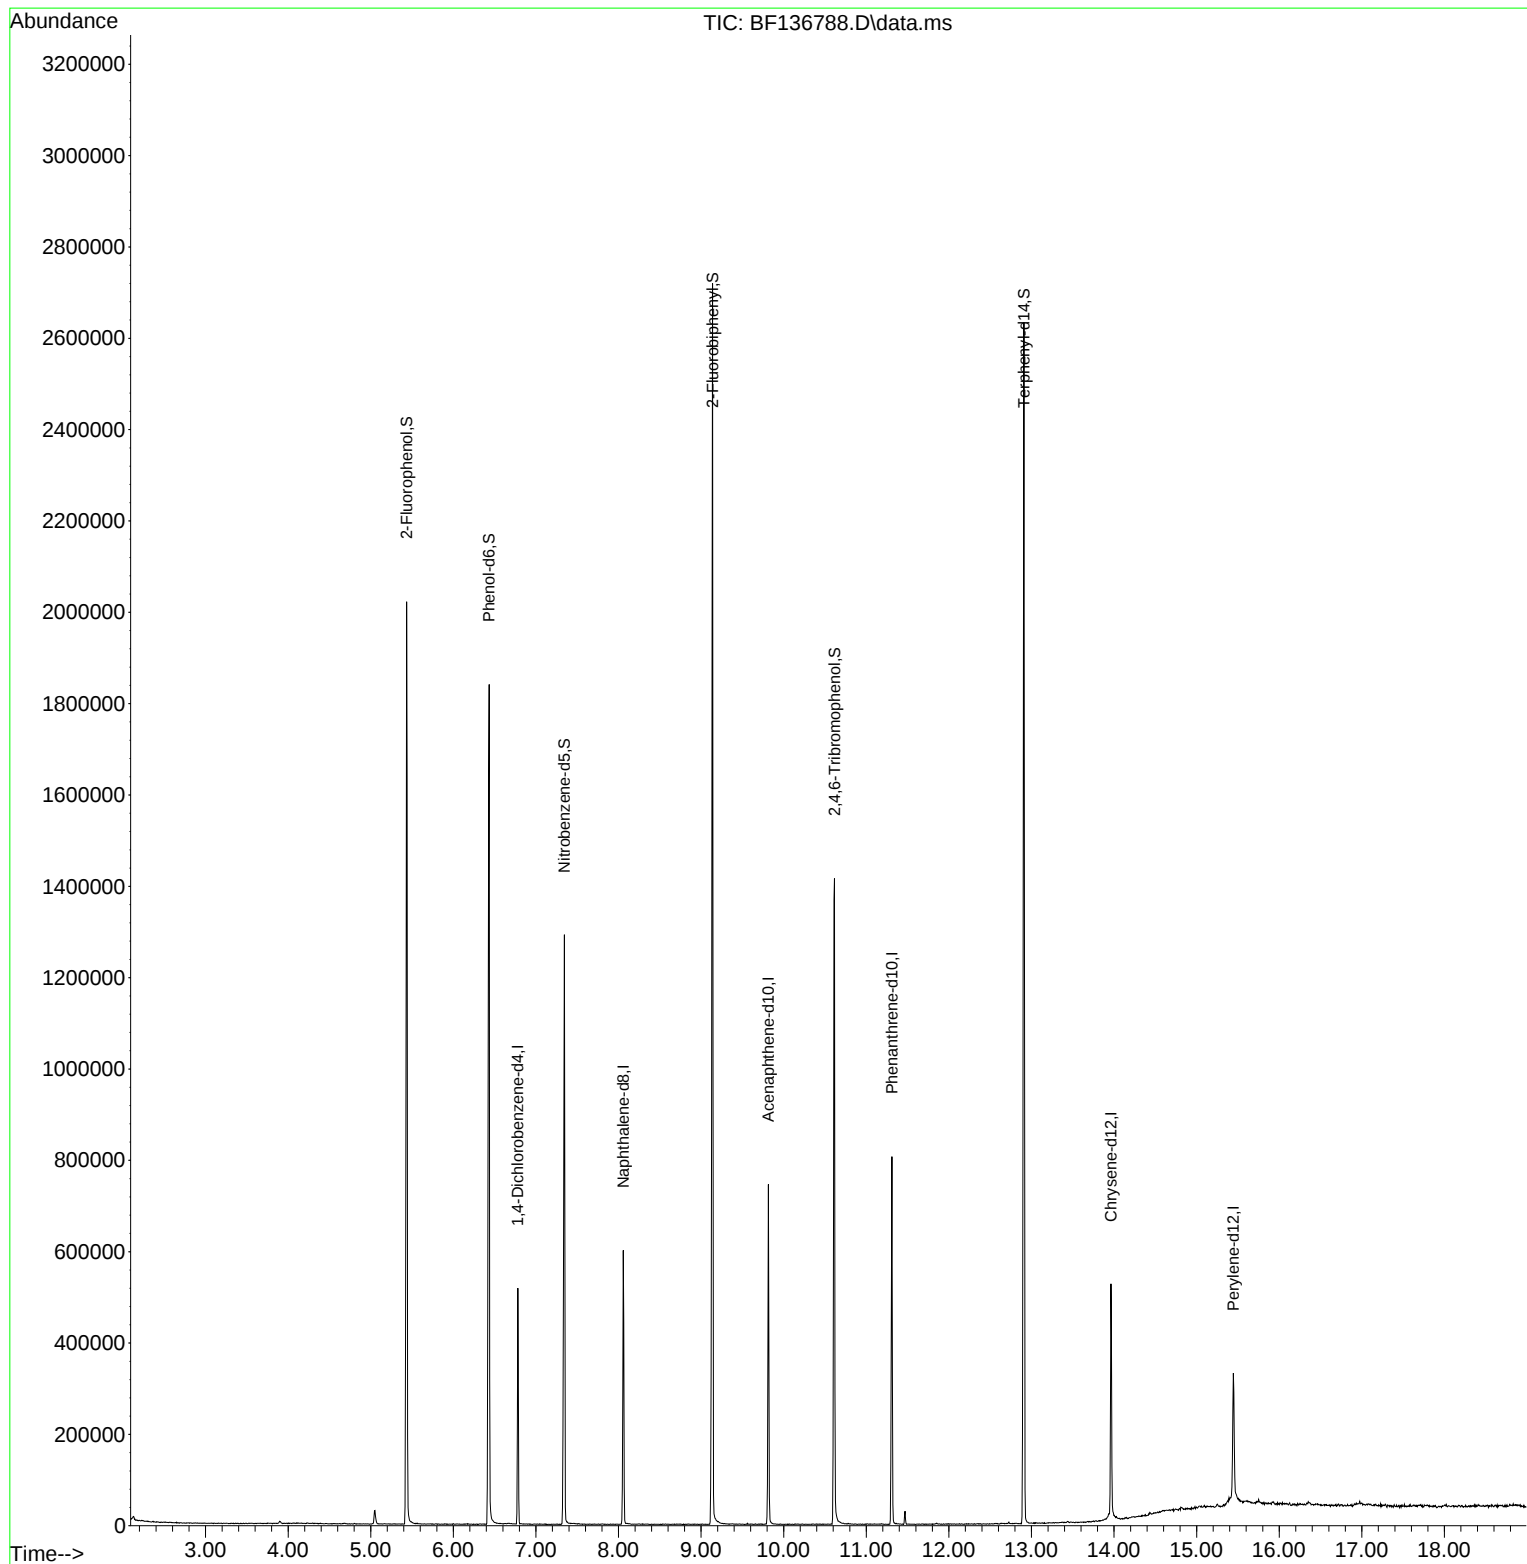




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.781 min Scan# 79
Delta R.T. -0.011 min
Lab File: BF136788.D
Acq: 28 Dec 2023 11:38




Instrument :
BNA_F
ClientSampleId :
PB157982TB


Tgt Ion:152 Resp: 70689
Ion Ratio Lower Upper
152 100
150 159.1 127.0 190.6
115 62.5 49.0 73.4

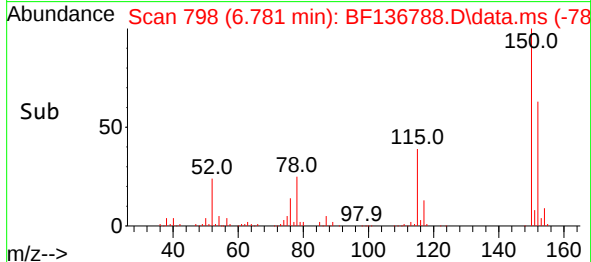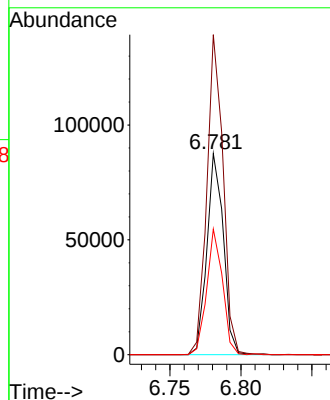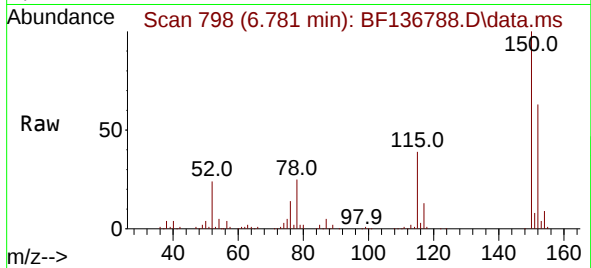

#5
2-Fluorophenol
Concen: 125.150 ng
RT: 5.434 min Scan# 569
Delta R.T. 0.006 min
Lab File: BF136788.D
Acq: 28 Dec 2023 11:38

Tgt Ion:112 Resp: 566994
Ion Ratio Lower Upper
112 100
64 63.4 51.1 76.7
63 32.3 26.1 39.1


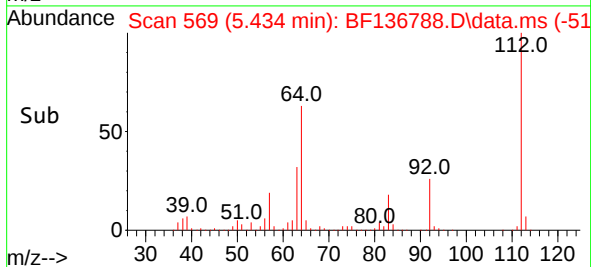
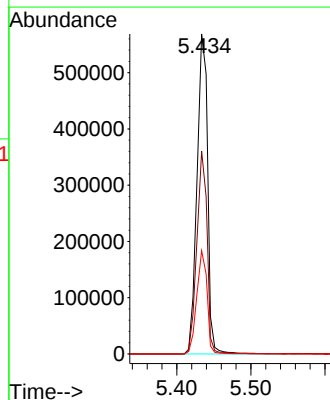
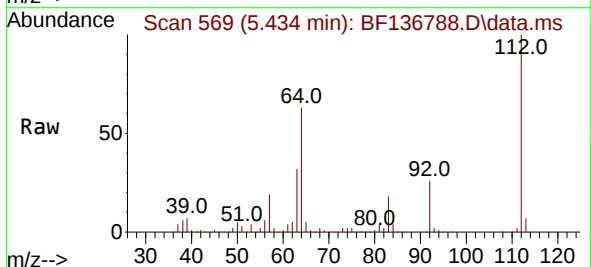


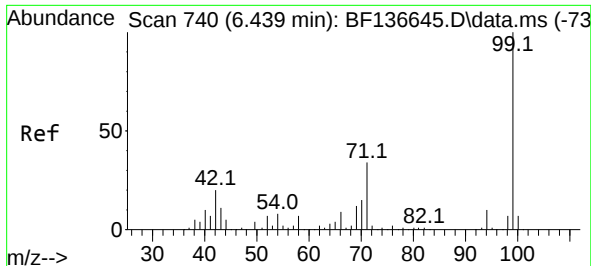

#7
Phenol-d6
Concen: 120.303 ng
RT: 6.434 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF136788.D
Acq: 28 Dec 2023 11:38




Instrument :
BNA_F
ClientSampleId :
PB157982TB


Tgt Ion: 99 Resp: 706232
Ion Ratio Lower Upper
99 100
42 18.7 16.1 24.1
71 32.6 27.4 41.2

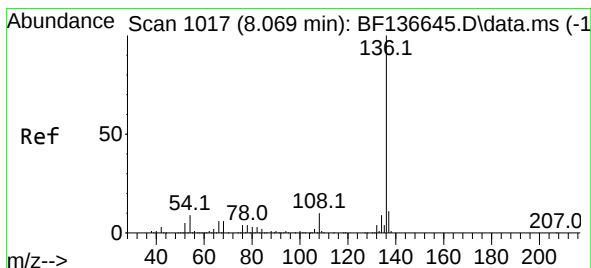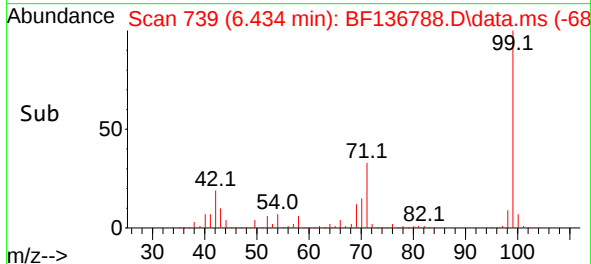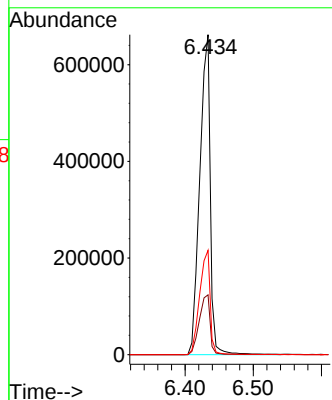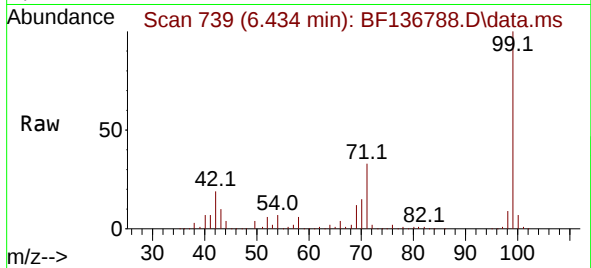

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.057 min Scan# 1015
Delta R.T. -0.012 min
Lab File: BF136788.D
Acq: 28 Dec 2023 11:38

Tgt Ion: 136 Resp: 270441
Ion Ratio Lower Upper
136 100
137 10.8 9.0 13.4
54 8.6 7.2 10.8
68 5.7 4.9 7.3

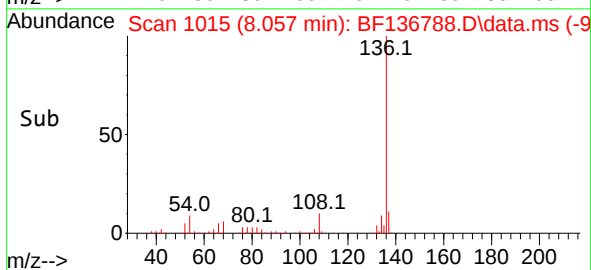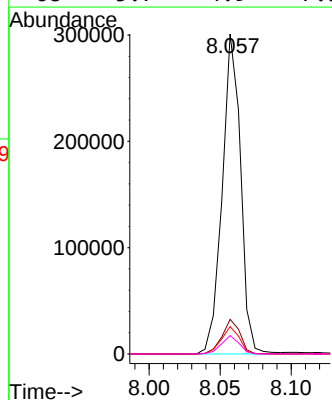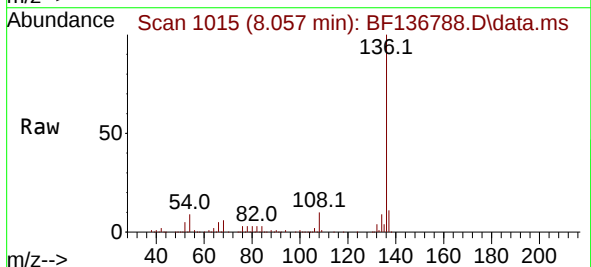

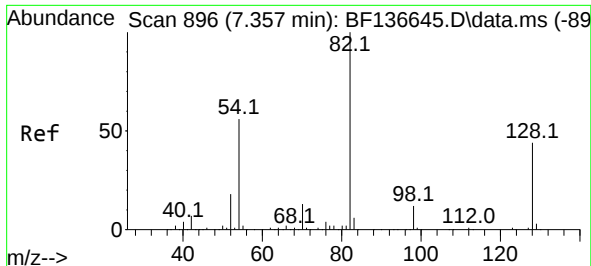

#23

Nitrobenzene-d5

Concen: 83.165 ng

RT: 7.345 min Scan# 894

Delta R.T. -0.012 min

Lab File: BF136788.D

Acq: 28 Dec 2023 11:38

Instrument :

BNA_F

ClientSampleId :

PB157982TB





Tgt Ion: 82 Resp: 439529

Ion Ratio Lower Upper

82 100

128 45.4 35.3 52.9

54 54.5 44.5 66.7

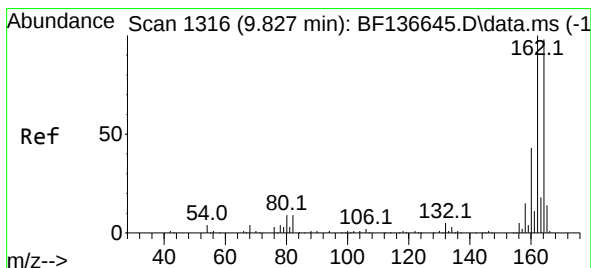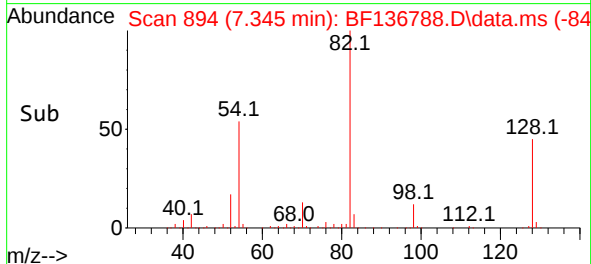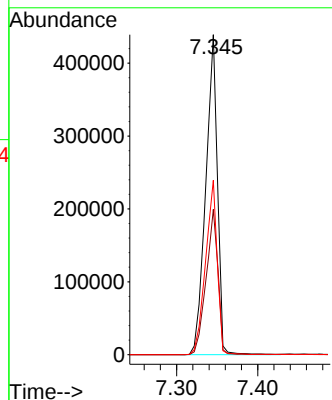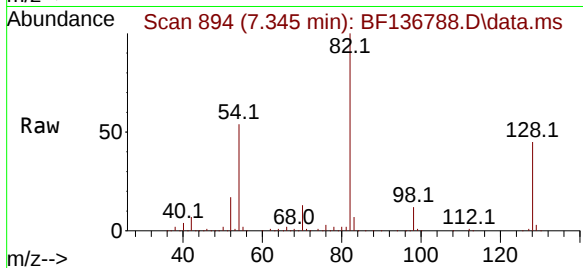

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.816 min Scan# 1314

Delta R.T. -0.012 min

Lab File: BF136788.D

Acq: 28 Dec 2023 11:38




Tgt Ion:164 Resp: 142854

Ion Ratio Lower Upper

164 100

162 99.0 81.6 122.4

160 44.9 34.9 52.3

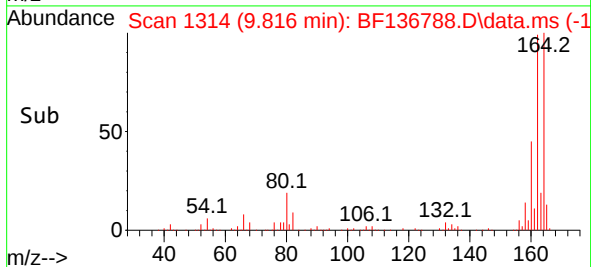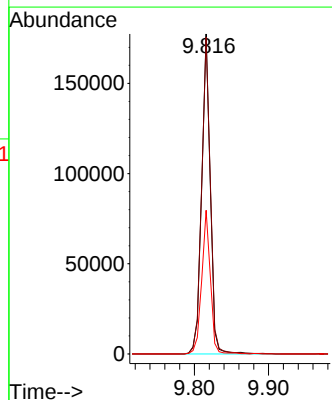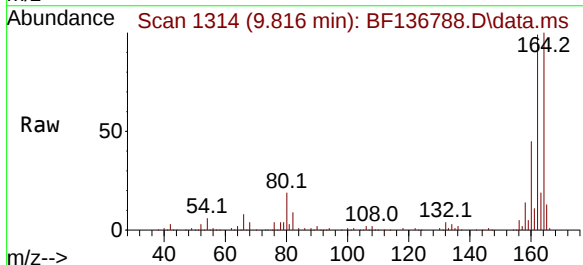



#42

2,4,6-Tribromophenol

Concen: 119.453 ng

RT: 10.616 min Scan# 1451

Delta R.T. -0.006 min

Lab File: BF136788.D


Acq: 28 Dec 2023 11:38

Instrument :

BNA_F

ClientSampleId :

PB157982TB

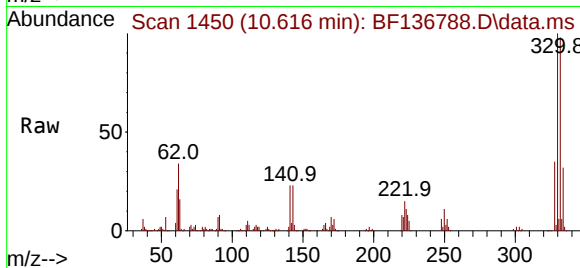




Tgt Ion:330 Resp: 200971

Ion Ratio Lower Upper

330 100

332 96.4 77.4 116.0

141 28.0 23.4 35.2

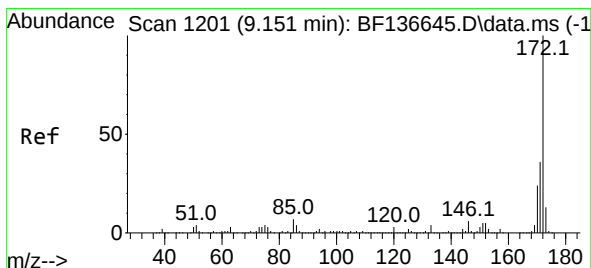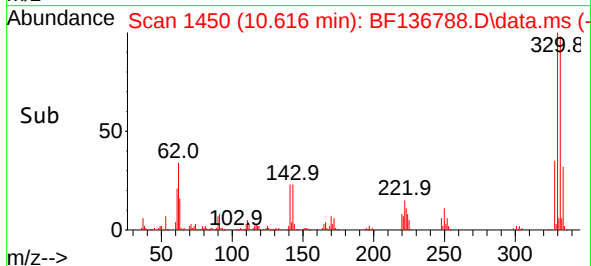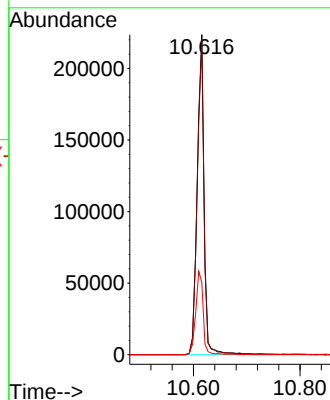

#45

2-Fluorobiphenyl

Concen: 83.940 ng

RT: 9.139 min Scan# 1199

Delta R.T. -0.012 min

Lab File: BF136788.D

Acq: 28 Dec 2023 11:38




Tgt Ion:172 Resp: 891546


Ion Ratio Lower Upper

172 100

171 35.5 29.0 43.6

170 23.8 19.0 28.4


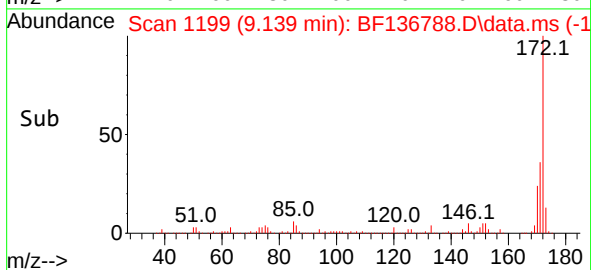
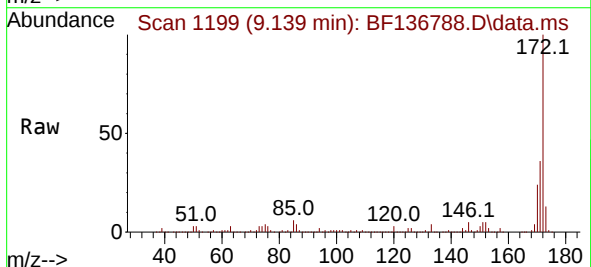
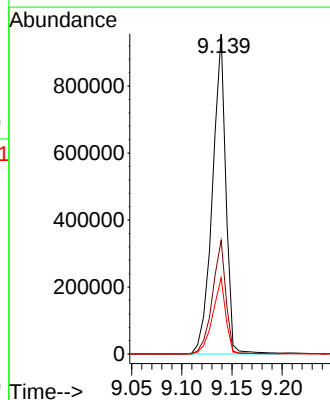


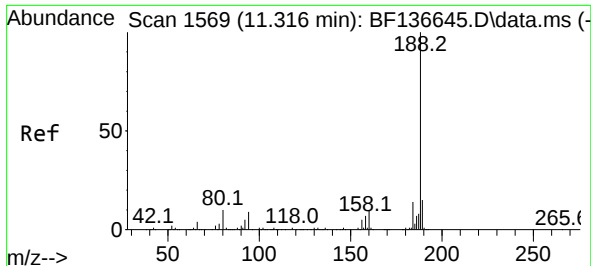

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.310 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF136788.D
Acq: 28 Dec 2023 11:38




Instrument :
BNA_F
ClientSampleId :
PB157982TB


Tgt Ion:188 Resp: 286992
Ion Ratio Lower Upper
188 100
94 8.7 7.5 11.3
80 9.5 8.1 12.1

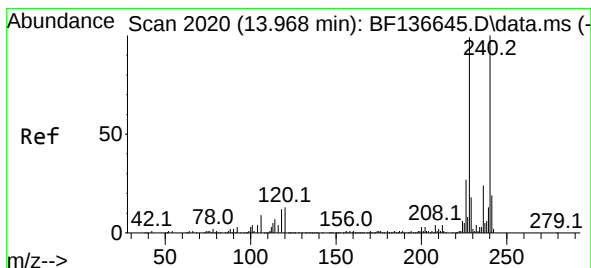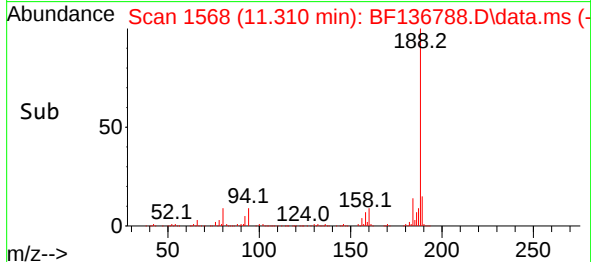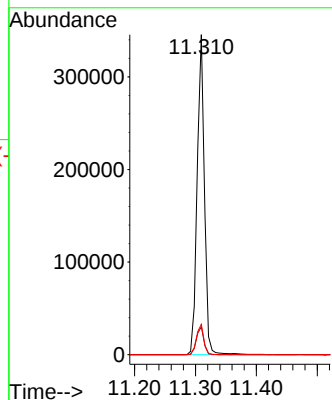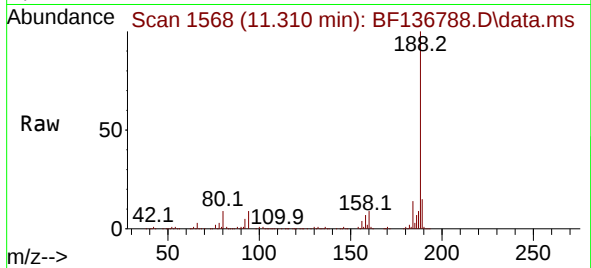

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.962 min Scan# 2019
Delta R.T. -0.006 min
Lab File: BF136788.D
Acq: 28 Dec 2023 11:38


Tgt Ion:240 Resp: 171287
Ion Ratio Lower Upper
240 100
120 11.2 10.3 15.5
236 25.3 19.4 29.2

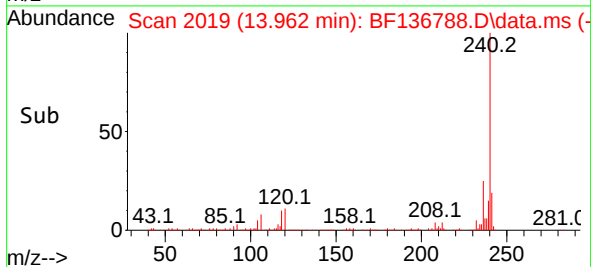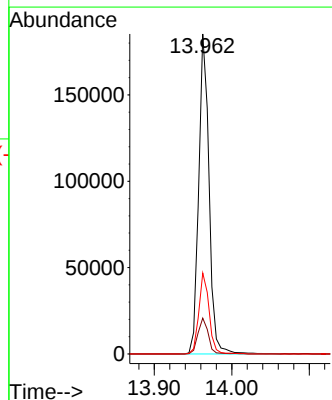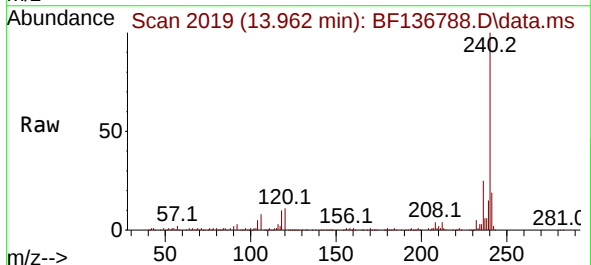



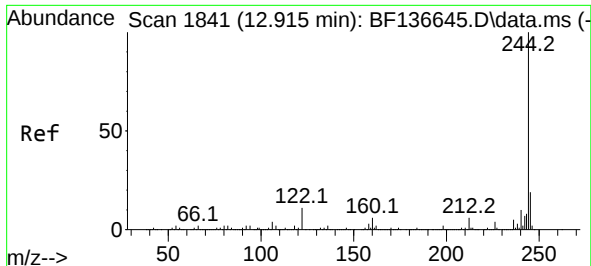


#79
 Terphenyl-d14
 Concen: 80.520 ng
 RT: 12.910 min Scan# 1840
 Delta R.T. -0.006 min
 Lab File: BF136788.D
 Acq: 28 Dec 2023 11:38

Instrument :
 BNA_F
 ClientSampleId :
 PB157982TB

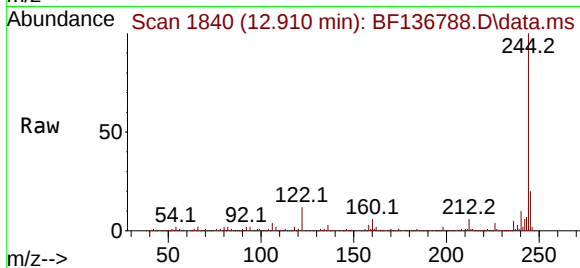

Tgt Ion:244 Resp: 986926
 Ion Ratio Lower Upper
 244 100
 212 6.5 5.0 7.4
 122 12.0 9.0 13.4

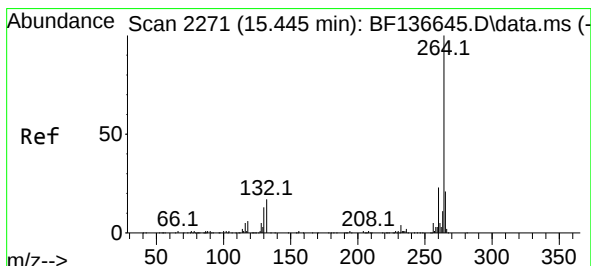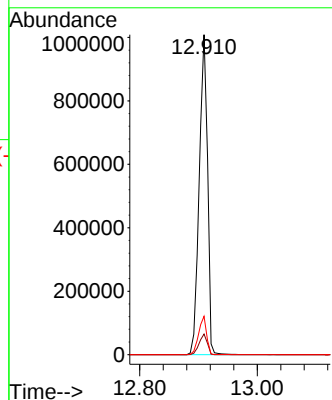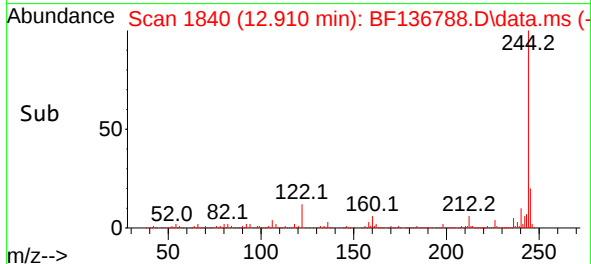

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.445 min Scan# 2271
 Delta R.T. -0.000 min
 Lab File: BF136788.D
 Acq: 28 Dec 2023 11:38

Tgt Ion:264 Resp: 142610
 Ion Ratio Lower Upper
 264 100
 260 24.2 18.3 27.5
 265 21.9 17.0 25.6

