

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122823\
 Data File : BF136797.D
 Acq On : 28 Dec 2023 17:11
 Operator : CG\JU
 Sample : PB157953BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157953BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	500	505	517	rVB	51602	84007	2.41%	0.415%
2	5.434	564	569	572	rBV	2529547	2755526	79.00%	13.624%
3	6.434	733	739	742	rBV	2418490	2724359	78.11%	13.470%
4	6.781	794	798	801	rBV	639781	497363	14.26%	2.459%
5	7.345	888	894	897	rBV	1604719	1859052	53.30%	9.192%
6	8.057	1010	1015	1018	rBV	815790	662218	18.99%	3.274%
7	9.139	1193	1199	1202	rBV	3565484	3487809	100.00%	17.245%
8	9.816	1309	1314	1317	rBV	861950	759819	21.78%	3.757%
9	10.610	1444	1449	1453	rBV	1887935	2027929	58.14%	10.027%
10	11.310	1564	1568	1571	rBV	903823	815297	23.38%	4.031%
11	12.910	1834	1840	1843	rBV	3394527	3471586	99.53%	17.165%
12	13.963	2015	2019	2030	rVB	638972	603846	17.31%	2.986%
13	15.439	2265	2270	2281	rVB2	330991	476482	13.66%	2.356%




Sum of corrected areas: 20225293

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122823\
Data File : BF136797.D
Acq On : 28 Dec 2023 17:11
Operator : CG\JU
Sample : PB157953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

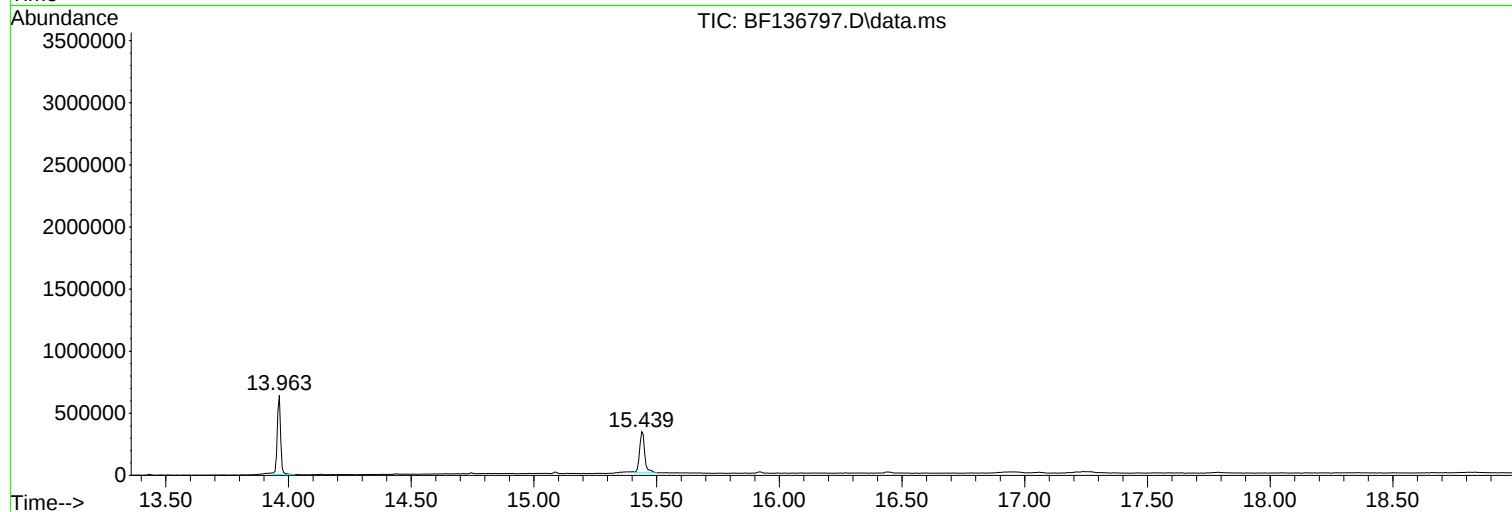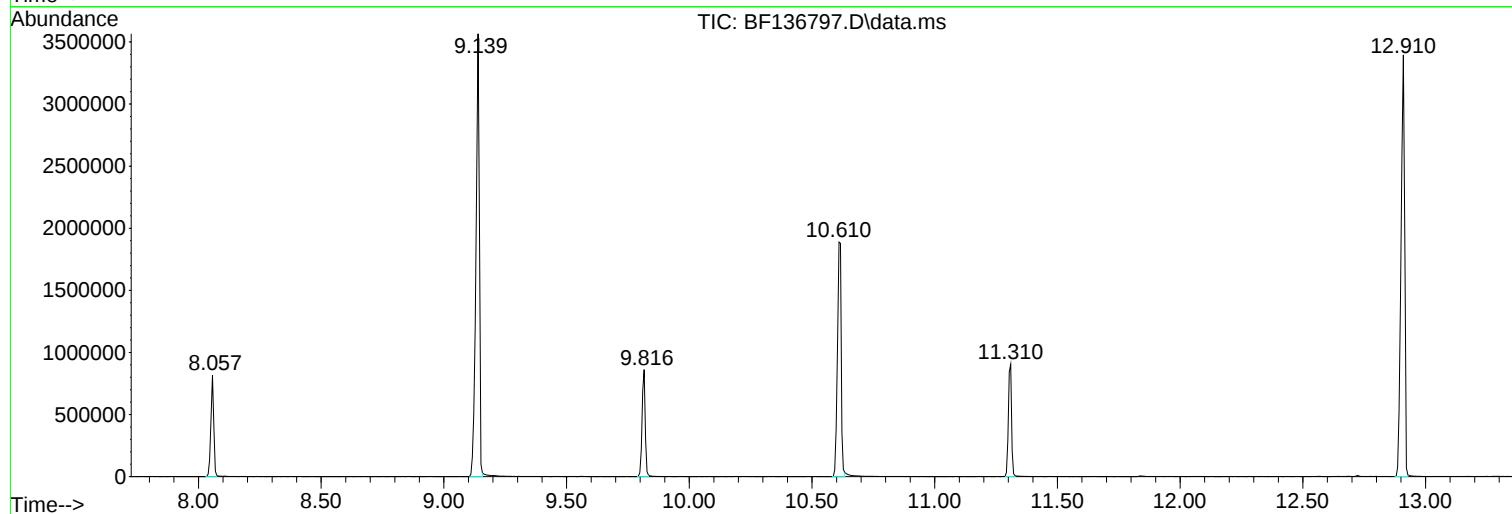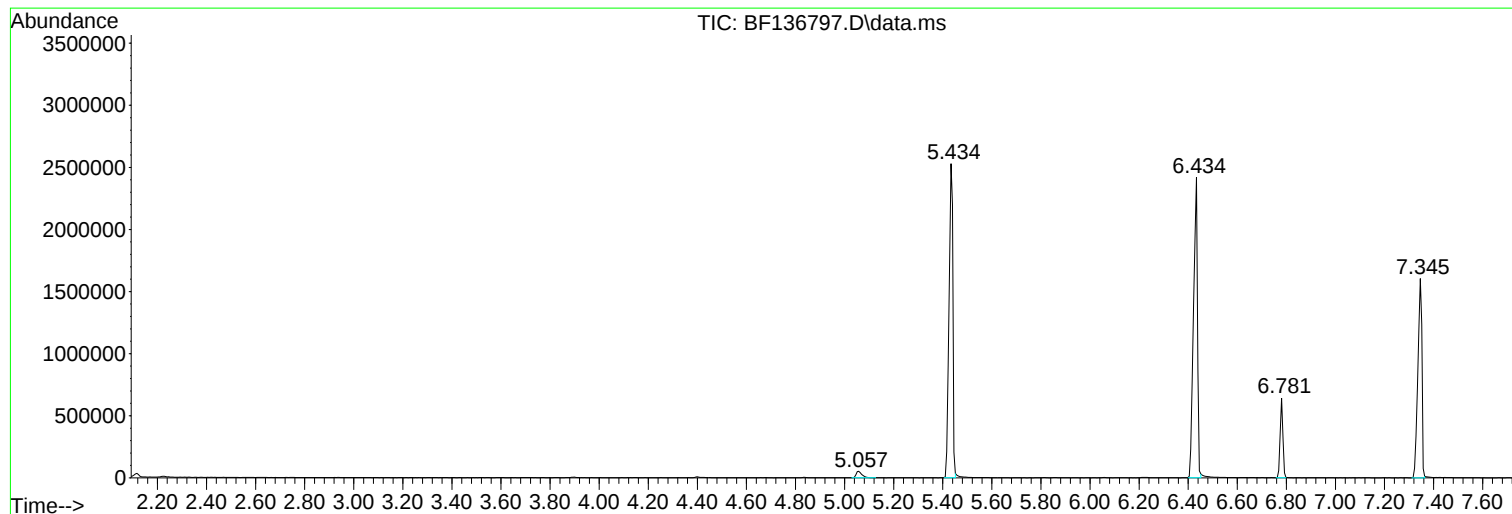

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122823\
Data File : BF136797.D
Acq On : 28 Dec 2023 17:11
Operator : CG\JU
Sample : PB157953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157953BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.057	3.38 ng	84007	1,4-Dichlorobenzene-d4	6.781

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	32		
3	Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	17		
4	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		
5	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	9		

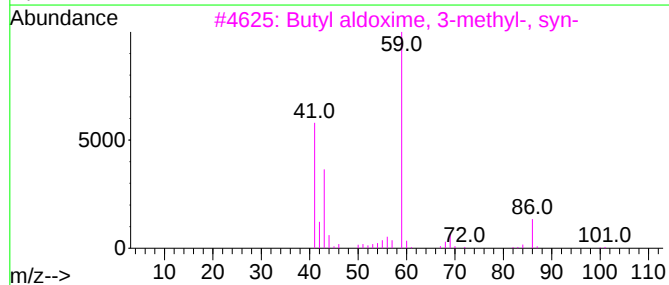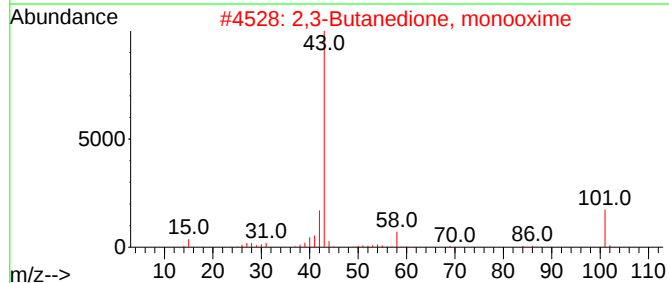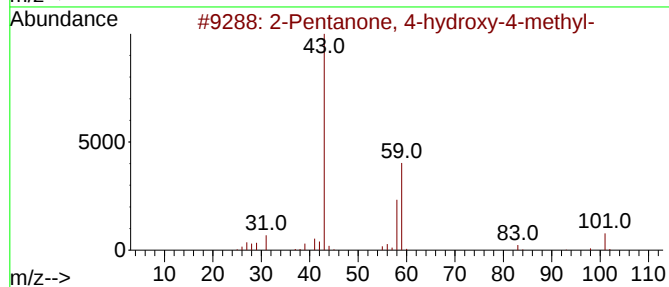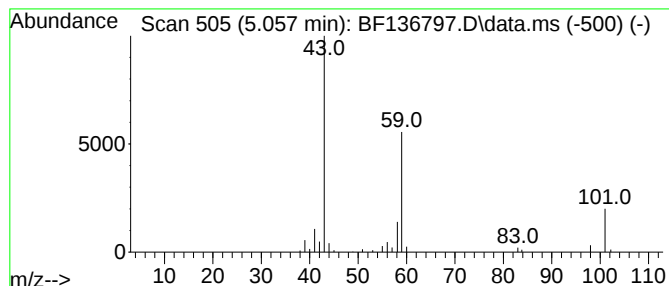

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122823\
Data File : BF136797.D
Acq On : 28 Dec 2023 17:11
Operator : CG\JU
Sample : PB157953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.057	3.4	ng	84007	1	6.781	497363	20.0