
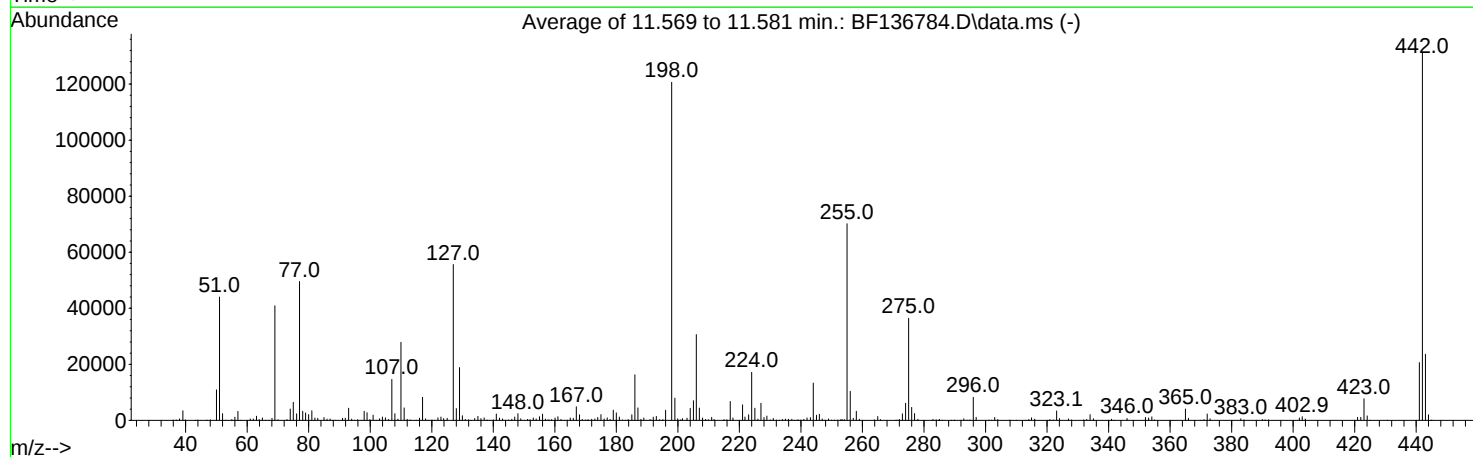


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122823\
Data File : BF136784.D
Acq On : 28 Dec 2023 09:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

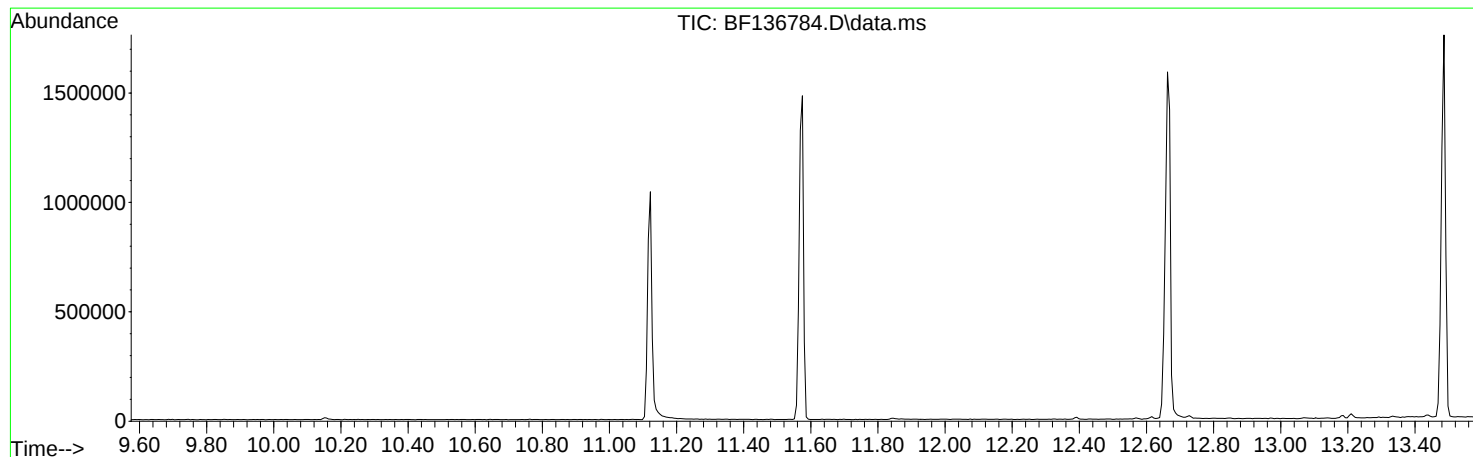




AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	44017	PASS
68	69	0.00	2	1.8	755	PASS
69	198	0.00	100	33.9	40857	PASS
70	69	0.00	2	0.6	227	PASS
127	198	10	80	46.1	55636	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	120645	PASS
199	198	5	9	6.6	7940	PASS
275	198	10	60	30.2	36409	PASS
365	198	1	100	3.3	4039	PASS
441	198	0.01	100	17.1	20612	PASS
442	442	50	100	100.0	131264	PASS
443	442	15	24	18.0	23580	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122823\
Data File : BF136784.D
Acq On : 28 Dec 2023 09:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 28 10:53:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

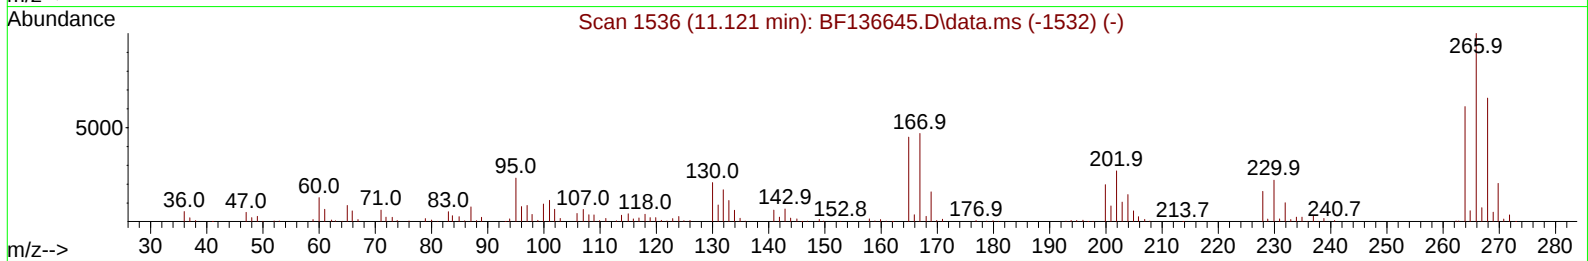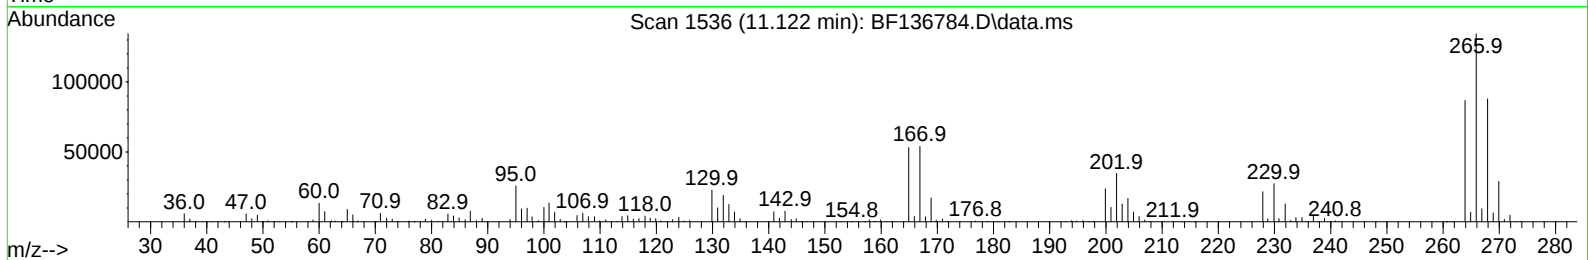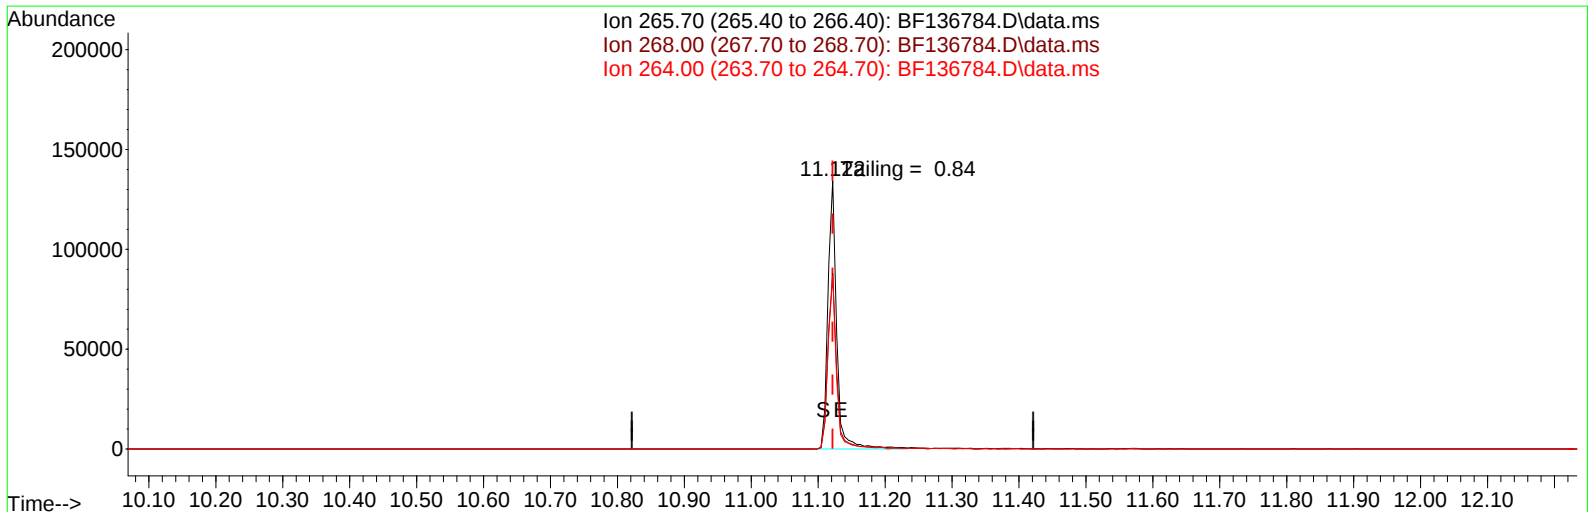

TIC: BF136784.D\data.ms

(70) Pentachlorophenol (C)

11.122min (+ 0.000) 41451.10 ng




response 123626

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	65.40
264.00	61.20	64.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122823\
Data File : BF136784.D
Acq On : 28 Dec 2023 09:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 28 10:53:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

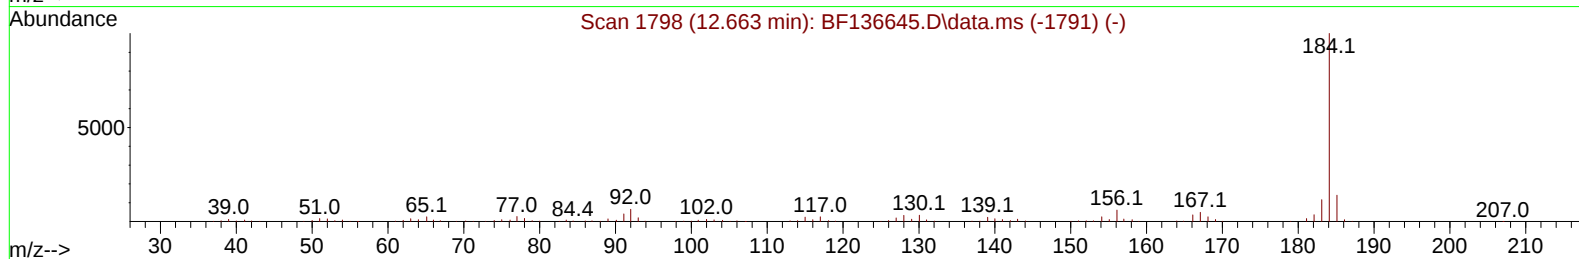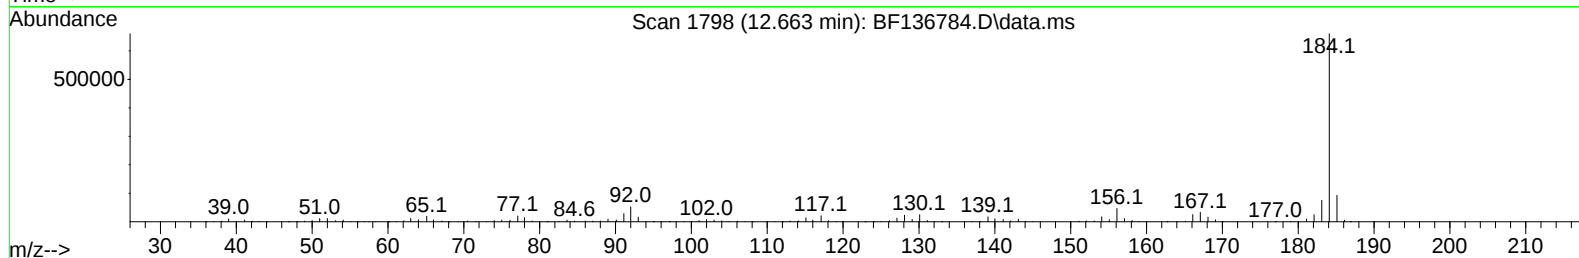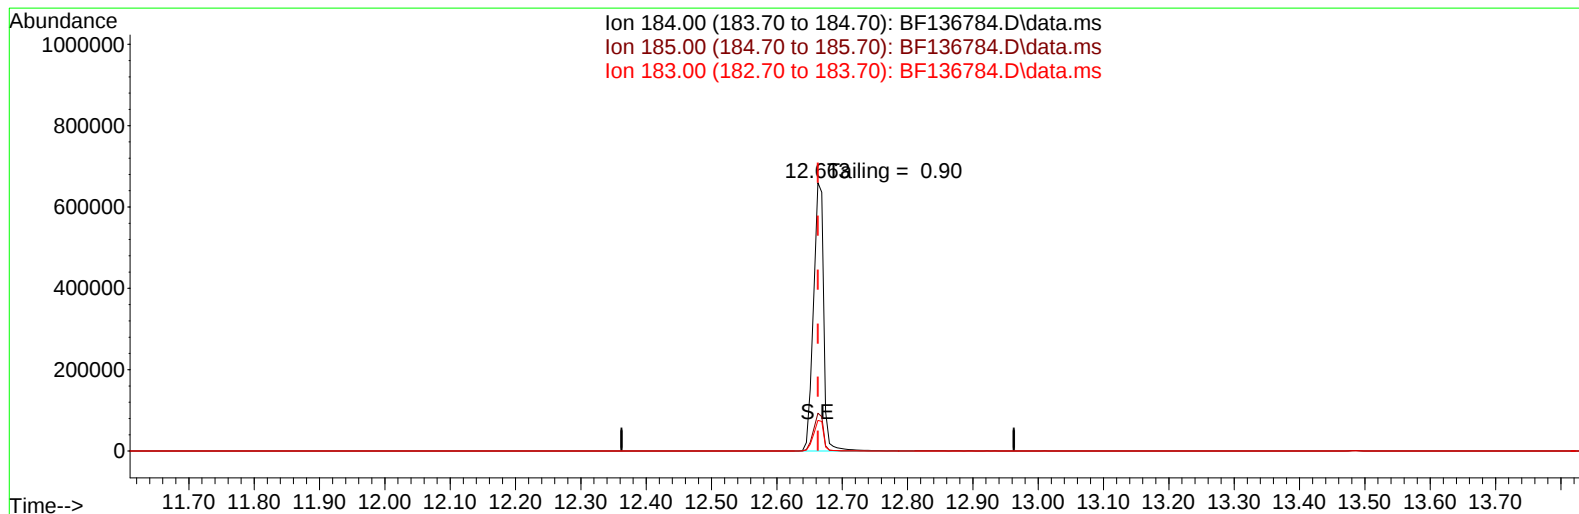

TIC: BF136784.D\data.ms

(77) Benzidine

12.663min (+ 0.000) 0.00 ng m

response 720782

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.08
183.00	11.60	11.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/28/2023	BNA_F	<u>BF136784.D</u>
Compound Name	Response	Retention Time
DDT	313181	13.486
DDD	6187	13.21
DDE	441	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6628	319809	2.07

Instrument :
BNA_F
ClientSampleId :
DFTPP