
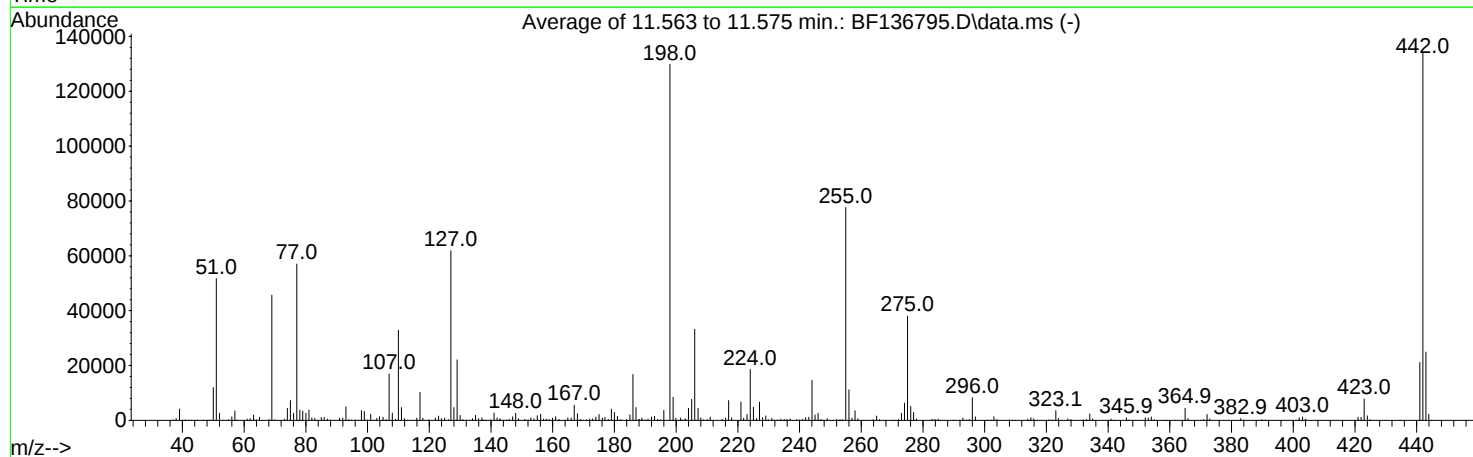


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122823\
Data File : BF136795.D
Acq On : 28 Dec 2023 15:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

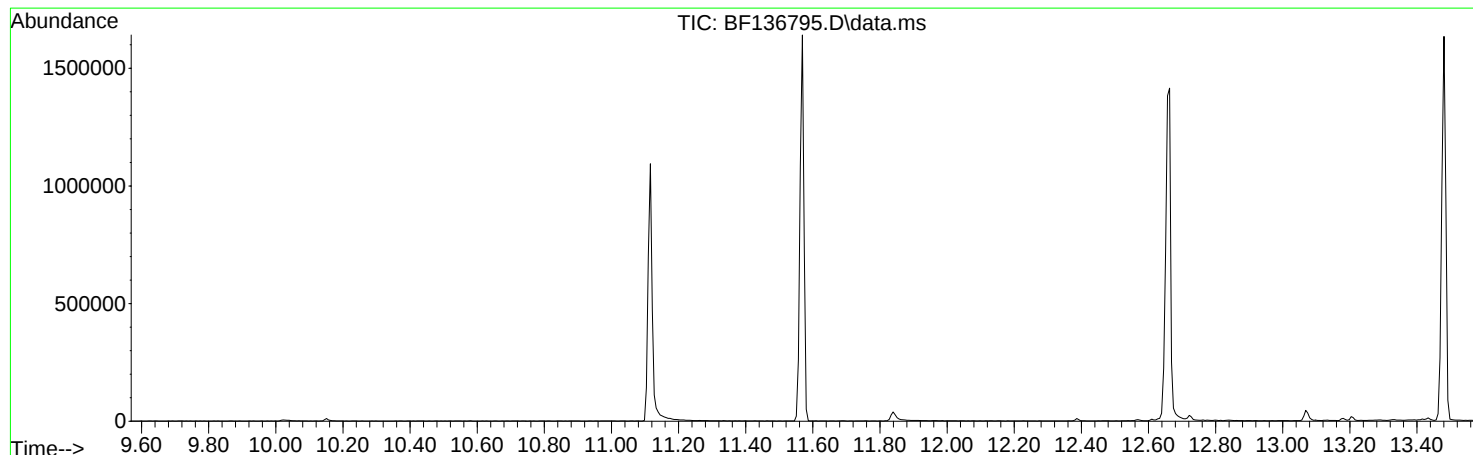




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	51704	PASS
68	69	0.00	2	0.9	420	PASS
69	198	0.00	100	35.2	45663	PASS
70	69	0.00	2	0.6	261	PASS
127	198	10	80	47.7	61867	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	129800	PASS
199	198	5	9	6.5	8385	PASS
275	198	10	60	29.3	38053	PASS
365	198	1	100	3.4	4384	PASS
441	198	0.01	100	16.3	21137	PASS
442	442	50	100	100.0	134128	PASS
443	442	15	24	18.6	24907	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122823\
Data File : BF136795.D
Acq On : 28 Dec 2023 15:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 28 15:57:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

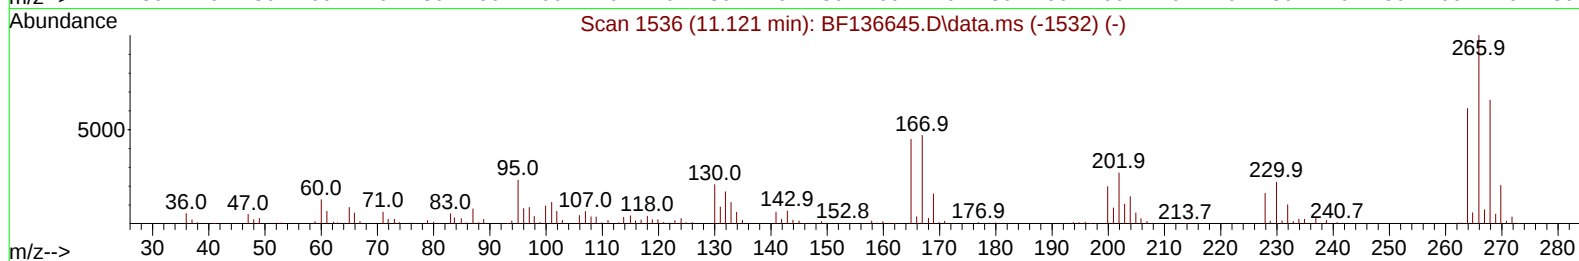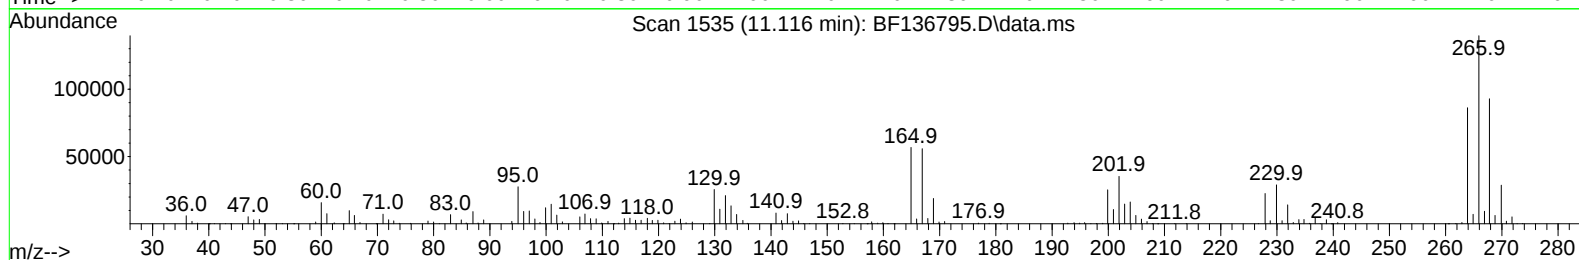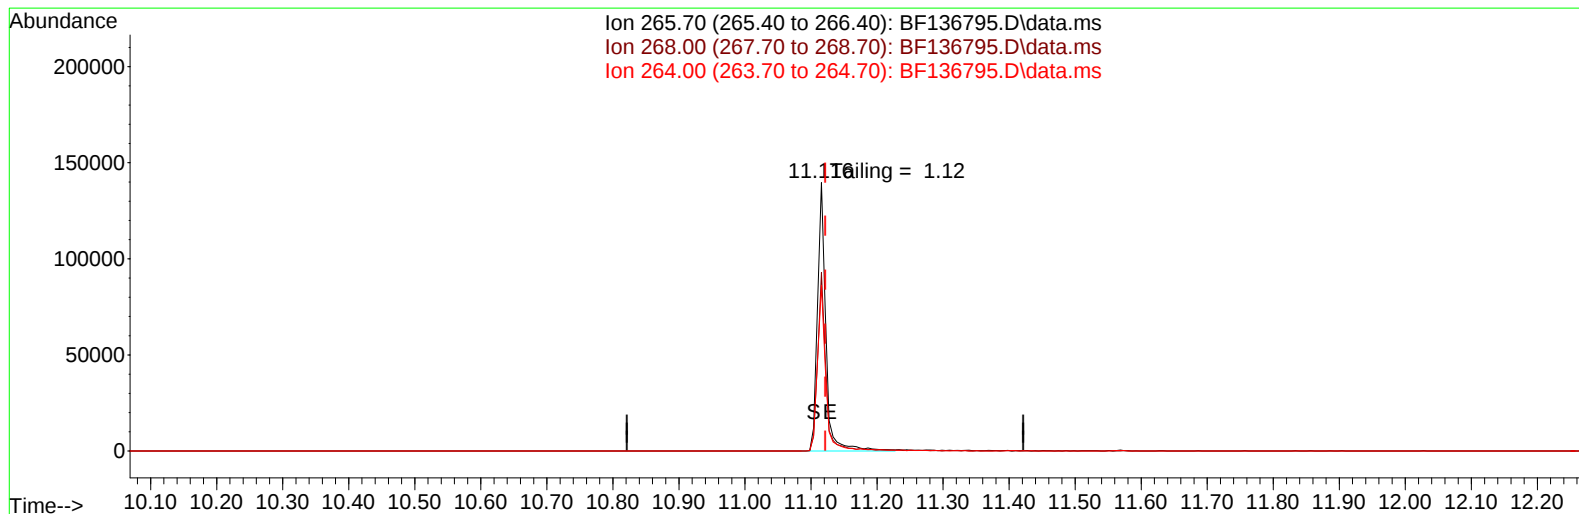

TIC: BF136795.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.006) 34129.26 ng




response 125415

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	66.49
264.00	61.20	61.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122823\
Data File : BF136795.D
Acq On : 28 Dec 2023 15:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 28 16:45:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

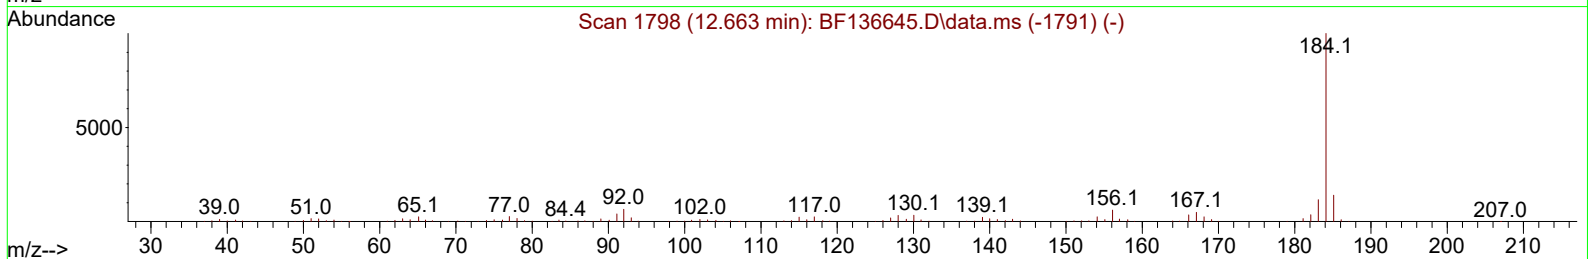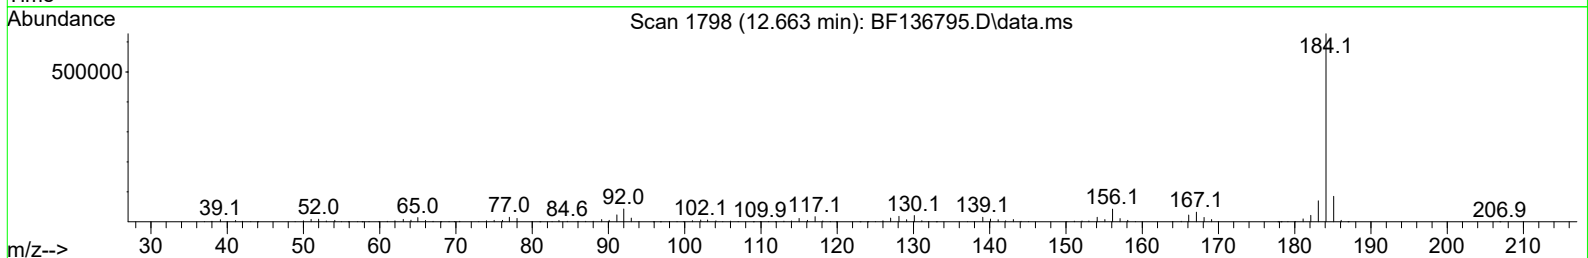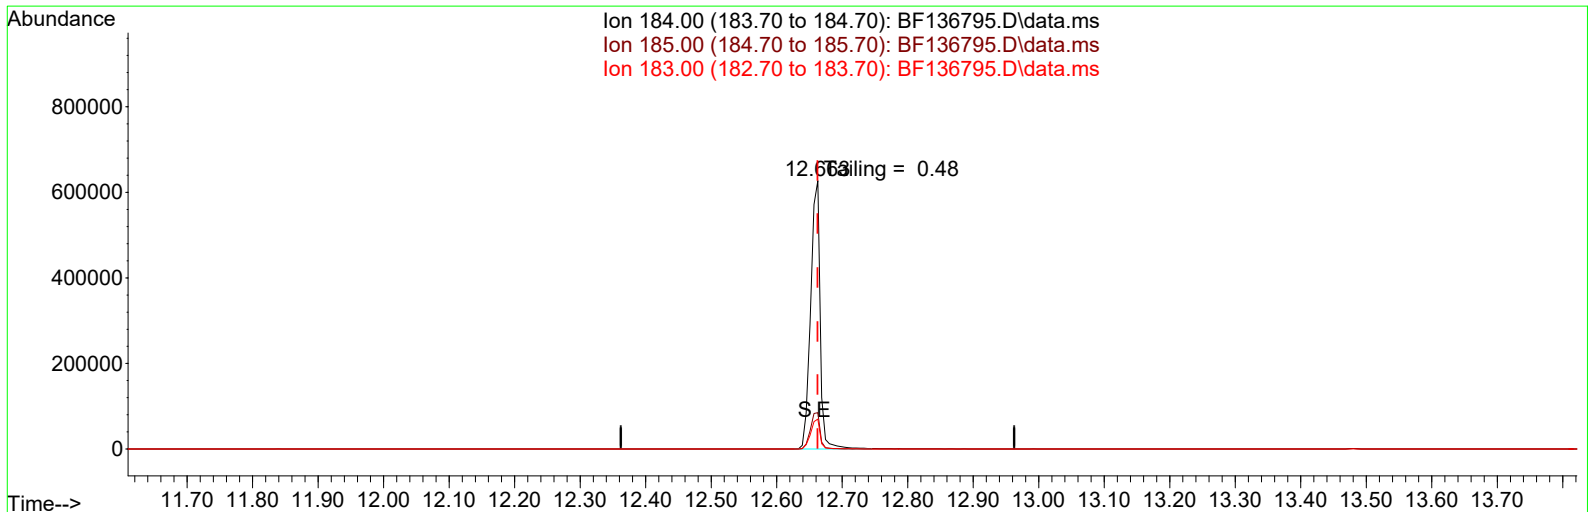

TIC: BF136795.D\data.ms

(77) Benzidine

12.663min (+ 0.000) 0.00 ng

response 630906

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.56
183.00	11.60	11.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/28/2023	BNA_F	<u>BF136795.D</u>
Compound Name	Response	Retention Time
DDT	292051	13.48
DDD	5916	13.204
DDE	488	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6404	298455	2.15

Instrument :
BNA_F
ClientSampleId :
DFTPP