
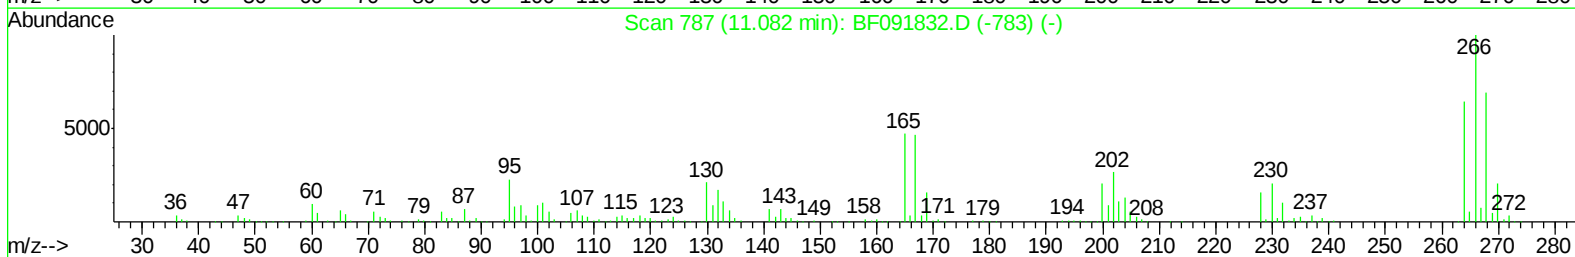
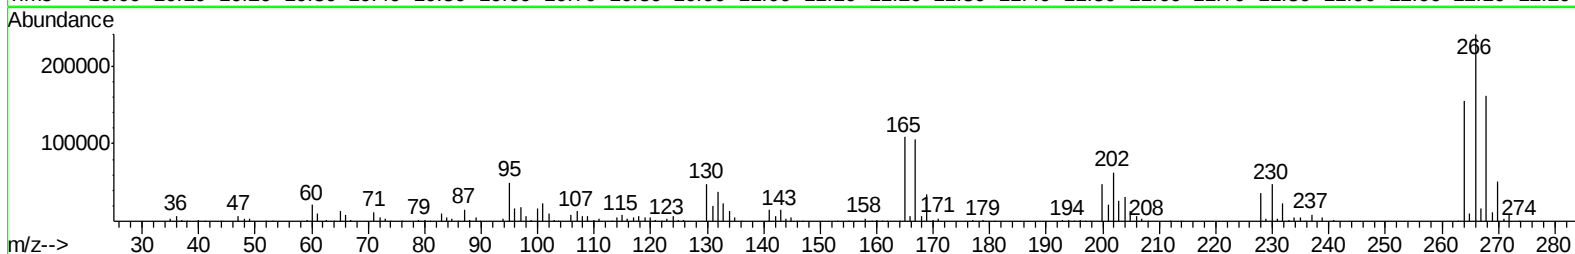


Data Path : Z:\HPCHEM1\BNA_F\Data\BF122916\
Data File : BF092015.D
Acq On : 29 Dec 2016 10:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 06:11:10 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 17:32:10 2016
Response via : Initial Calibration

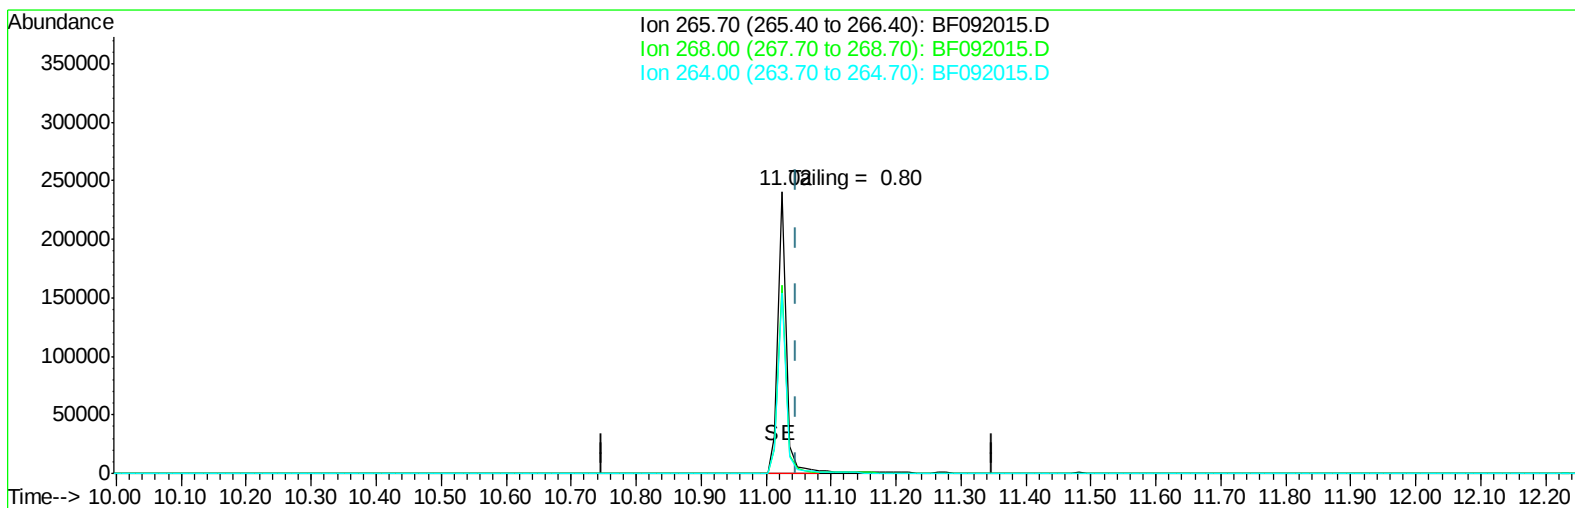

TIC: BF092015.D

(69) Pentachlorophenol (C)




11.025min (-0.023) 0.00ng

response 222388

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	67.04
264.00	62.90	64.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF122916\
Data File : BF092015.D
Acq On : 29 Dec 2016 10:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 06:11:10 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 17:32:10 2016
Response via : Initial Calibration

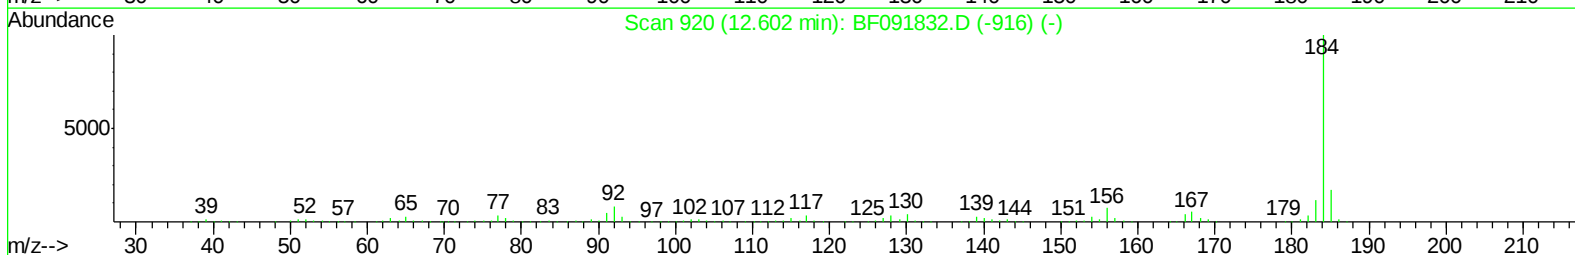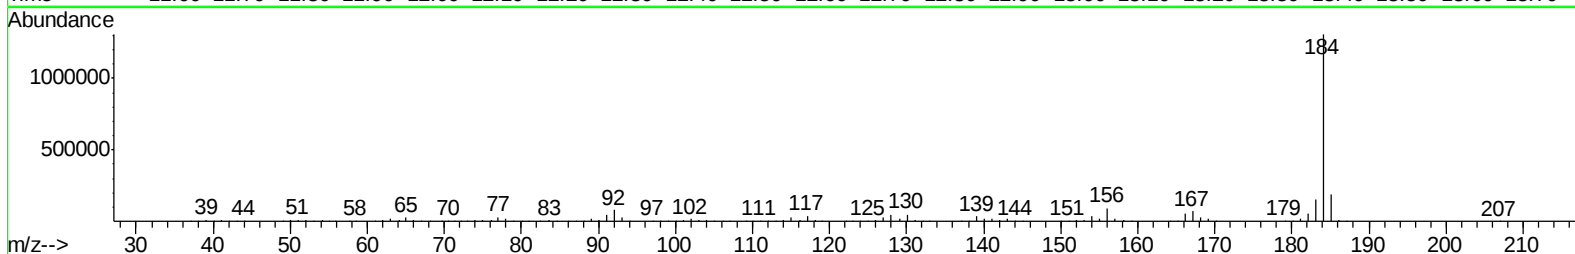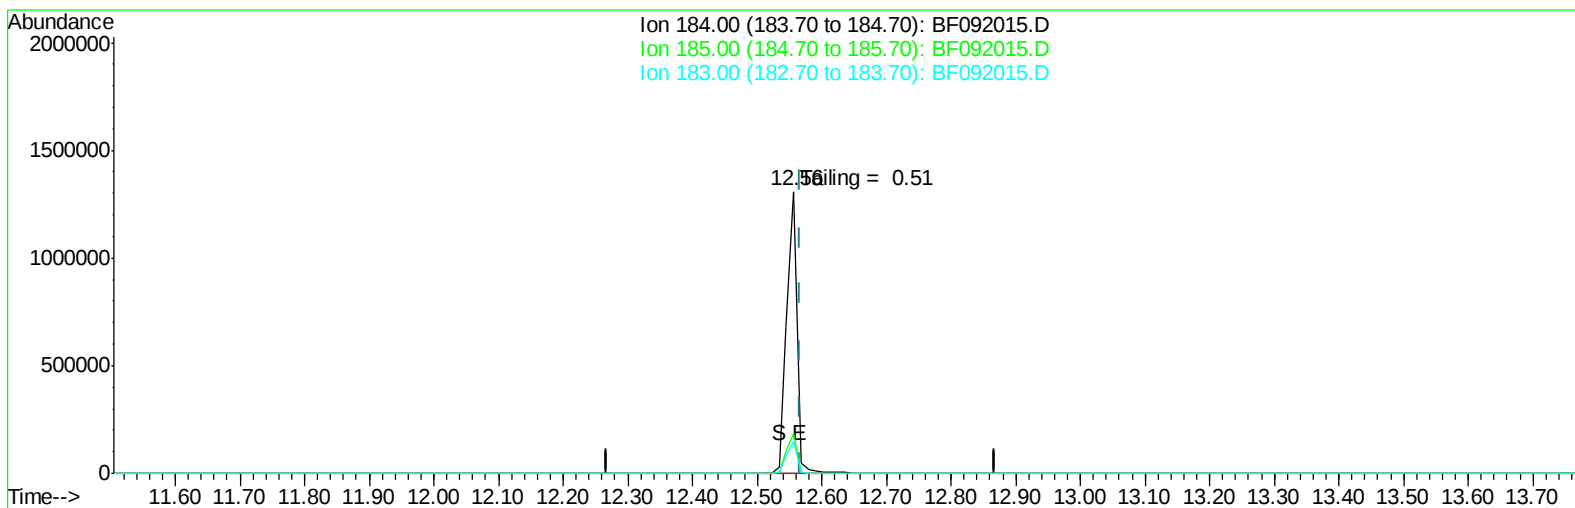

TIC: BF092015.D

(76) Benzidine

12.556min (-0.011) -20.00ng

response 1466630

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.17
183.00	11.50	11.59
0.00	0.00	0.00