

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122916\
 Data File : BF092026.D
 Acq On : 29 Dec 2016 16:13
 Operator : UM/SJ
 Sample : H6281-02RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-7RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.213	9	11	23	rVB2	18564	71405	1.24%	0.169%
2	4.830	238	240	249	rVB	639622	793375	13.72%	1.882%
3	5.299	279	281	288	rBV	3240188	3162546	54.70%	7.503%
4	6.350	371	373	381	rBV	2003826	1941101	33.58%	4.605%
5	6.465	381	383	386	rBV	5186809	4785788	82.78%	11.355%
6	6.693	400	403	405	rBV	1135403	1237272	21.40%	2.935%
7	6.842	414	416	419	rBV	3312282	4552055	78.74%	10.800%
8	7.265	450	453	455	rBV	3502972	3809463	65.89%	9.038%
9	7.973	513	515	518	rBV	1345122	1339321	23.17%	3.178%
10	8.693	575	578	579	rBV2	49602	71833	1.24%	0.170%
11	8.785	583	586	588	rBV2	35279	58932	1.02%	0.140%
12	8.876	592	594	595	rBV	45565	66339	1.15%	0.157%
13	8.979	600	603	604	rVB2	79823	99438	1.72%	0.236%
14	9.013	604	606	607	rBV	66855	84470	1.46%	0.200%
15	9.059	607	610	612	rBV	5930998	5781168	100.00%	13.716%
16	9.242	622	626	628	rBV	132430	190126	3.29%	0.451%
17	9.356	634	636	637	rBV2	48079	71497	1.24%	0.170%
18	9.390	637	639	641	rVV2	78252	110452	1.91%	0.262%
19	9.459	643	645	647	rVB	144502	158524	2.74%	0.376%
20	9.528	650	651	654	rBV2	70658	82812	1.43%	0.196%
21	9.596	654	657	659	rBV	112721	189391	3.28%	0.449%
22	9.733	666	669	671	rBV	1381059	1685696	29.16%	3.999%
23	10.099	699	701	704	rBV3	63059	118237	2.05%	0.281%
24	10.351	721	723	727	rBV3	107341	292470	5.06%	0.694%
25	10.522	735	738	741	rVB	3650460	4062792	70.28%	9.639%
26	10.911	770	772	774	rVB3	118859	152999	2.65%	0.363%
27	11.048	782	784	786	rBV2	110043	185550	3.21%	0.440%
28	11.208	796	798	800	rVB	1139353	1076341	18.62%	2.554%
29	11.254	800	802	804	rBV2	156017	158218	2.74%	0.375%
30	11.402	814	815	817	rVB	83796	79697	1.38%	0.189%
31	11.768	845	847	852	rVB2	200973	253856	4.39%	0.602%
32	12.545	913	915	926	rVB2	220939	362744	6.27%	0.861%
33	12.808	935	938	940	rBV	2900919	3728279	64.49%	8.846%
34	13.700	1014	1016	1020	rVB3	38052	66653	1.15%	0.158%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122916\
Data File : BF092026.D
Acq On : 29 Dec 2016 16:13
Operator : UM/SJ
Sample : H6281-02RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-7RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.837	1026	1028	1031	rBV	464695	621325	10.75%	1.474%
36	15.231	1147	1150	1152	rBV	322941	486592	8.42%	1.154%
37	17.380	1335	1338	1341	rBV3	31257	96863	1.68%	0.230%
38	18.306	1417	1419	1422	rBV3	21306	63183	1.09%	0.150%


Sum of corrected areas: 42148803

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122916\
Data File : BF092026.D
Acq On : 29 Dec 2016 16:13
Operator : UM/SJ
Sample : H6281-02RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-7RE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

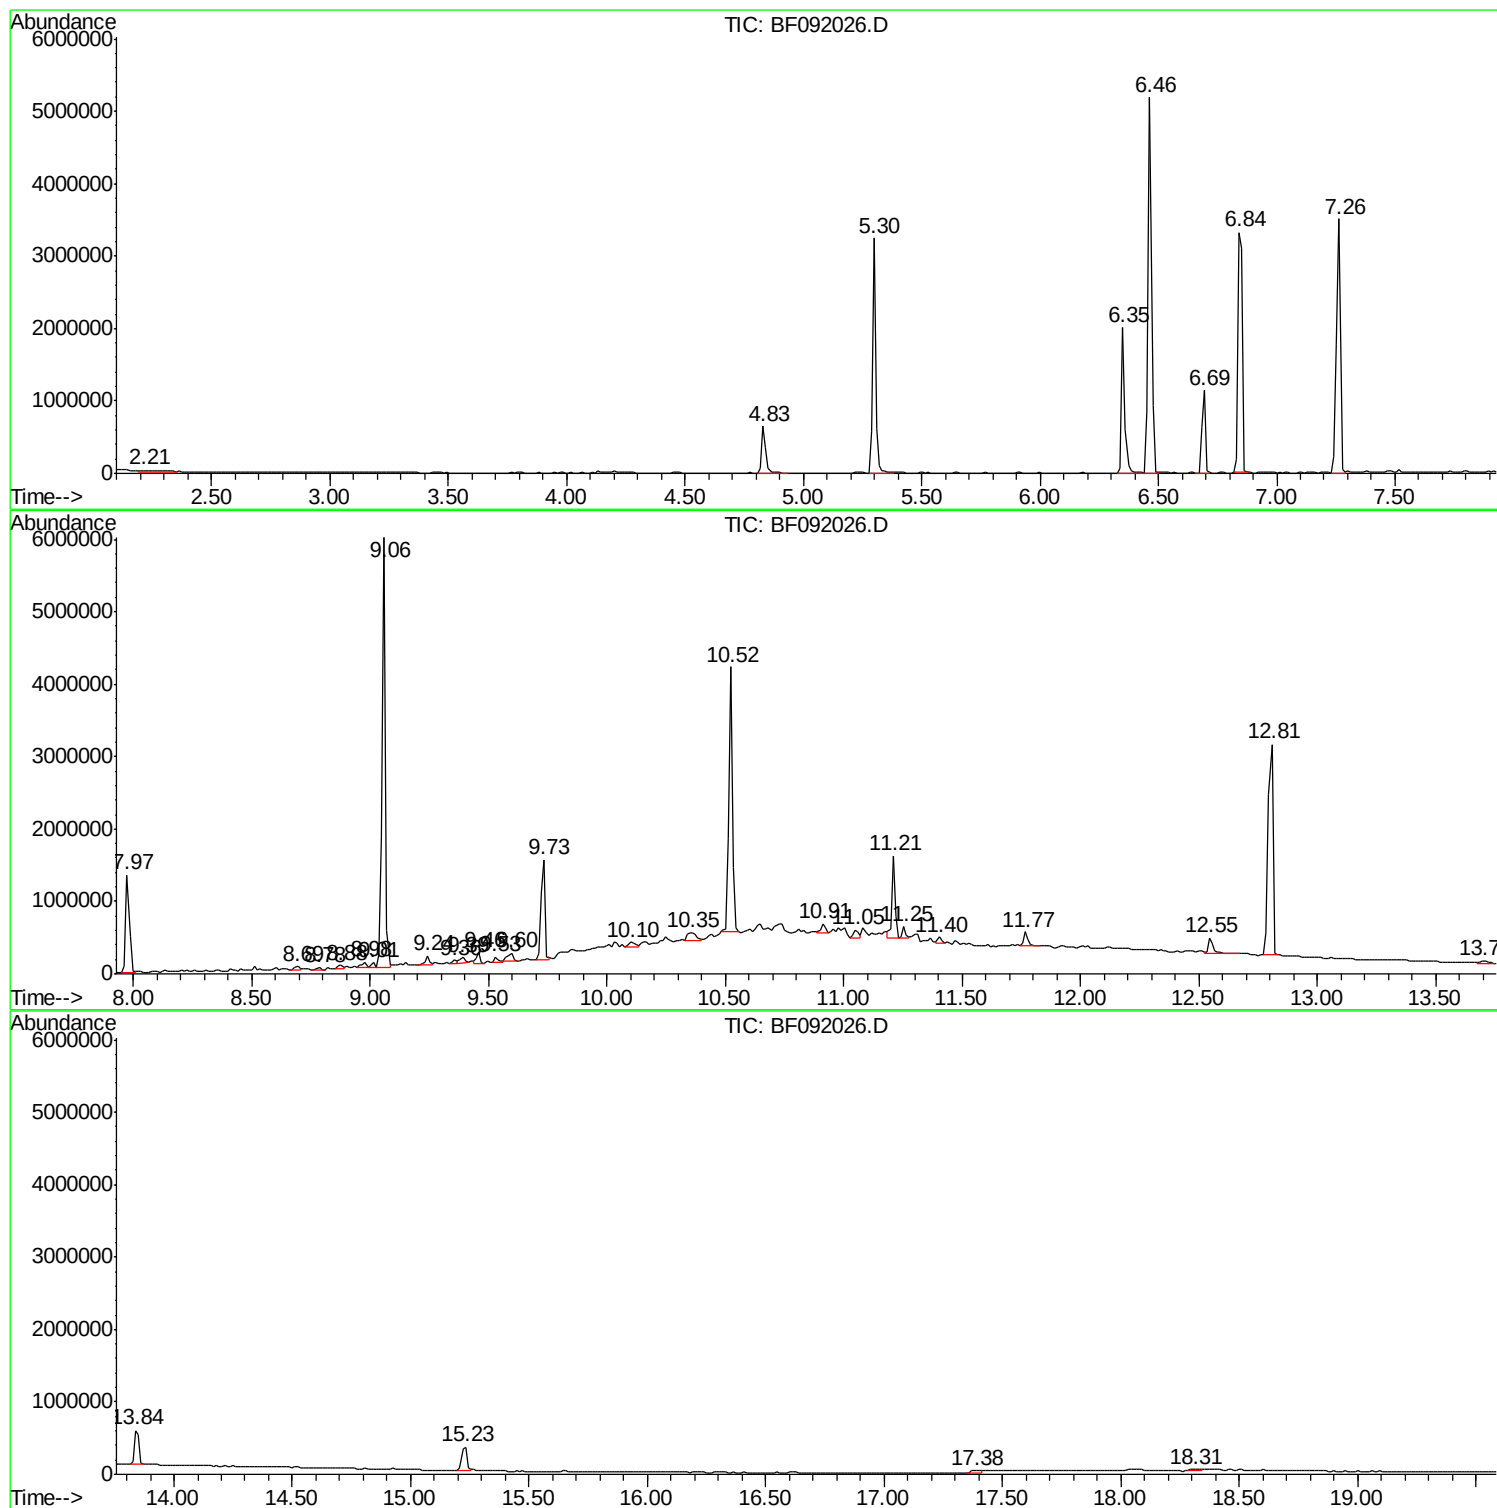

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF122916\
Data_File : BF092026.D
Acq_On : 29-Dec-2016 16:133
Operator : UM/SJJ
Sample : H6281-02REE
Misc :
ALS_Vial : 12 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
MW-7RE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
