

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122917\
 Data File : BF101818.D
 Acq On : 29 Dec 2017 10:19
 Operator : SJ/JU
 Sample : I7000-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Dec 29 13:24:56 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 29 13:21:45 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.78	152	157586	20.00	ng	0.00
21) Naphthalene-d8	8.06	136	621627	20.00	ng	0.00
38) Acenaphthene-d10	9.82	164	270333	20.00	ng	0.00
63) Phenanthrene-d10	11.32	188	483276	20.00	ng	0.00
75) Chrysene-d12	13.96	240	313374	20.00	ng	-0.01
86) Perylene-d12	15.43	264	318737	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	789462	74.62	ng	0.00
7) Phenol-d6	6.43	99	980451	74.47	ng	0.00
23) Nitrobenzene-d5	7.35	82	588561	52.70	ng	-0.01
41) 2,4,6-Tribromophenol	10.62	330	195780	75.16	ng	0.00
44) 2-Fluorobiphenyl	9.14	172	850307	48.79	ng	0.00
78) Terphenyl-d14	12.89	244	636853	48.99	ng	0.00
Target Compounds						
10) Phenol	6.45	94	34280	2.284	ng	# 45
19) n-Nitroso-di-n-propylamine	7.35	70	77195	8.928	ng	# 82
25) Isophorone	7.35	82	588561	26.273	ng	# 64
49) Dimethylphthalate	9.53	163	101207	4.654	ng	# 99
56) 2,4-Dinitrotoluene	9.82	165	35115	7.052	ng	# 24
66) 4-Bromophenyl-phenylether	10.62	248	12181	2.243	ng	# 1
70) Phenanthrene	11.34	178	125824	4.682	ng	# 99
74) Fluoranthene	12.53	202	146297	5.186	ng	# 97
77) Pyrene	12.76	202	118764	5.050	ng	# 99
80) Benzo(a)anthracene	13.96	228	52638	2.544	ng	# 97
82) Chrysene	13.99	228	52299	2.677	ng	# 98
87) Benzo(b)fluoranthene	15.01	252	88211	4.540	ng	# 95
88) Benzo(k)fluoranthene	15.01	252	88211	4.670	ng	# 98
89) Benzo(a)pyrene	15.38	252	43421	2.424	ng	# 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122917\
Data File : BF101818.D
Acq On : 29 Dec 2017 10:19
Operator : SJ/JU
Sample : I7000-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Dec 29 13:24:56 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 13:21:45 2017
Response via : Initial Calibration

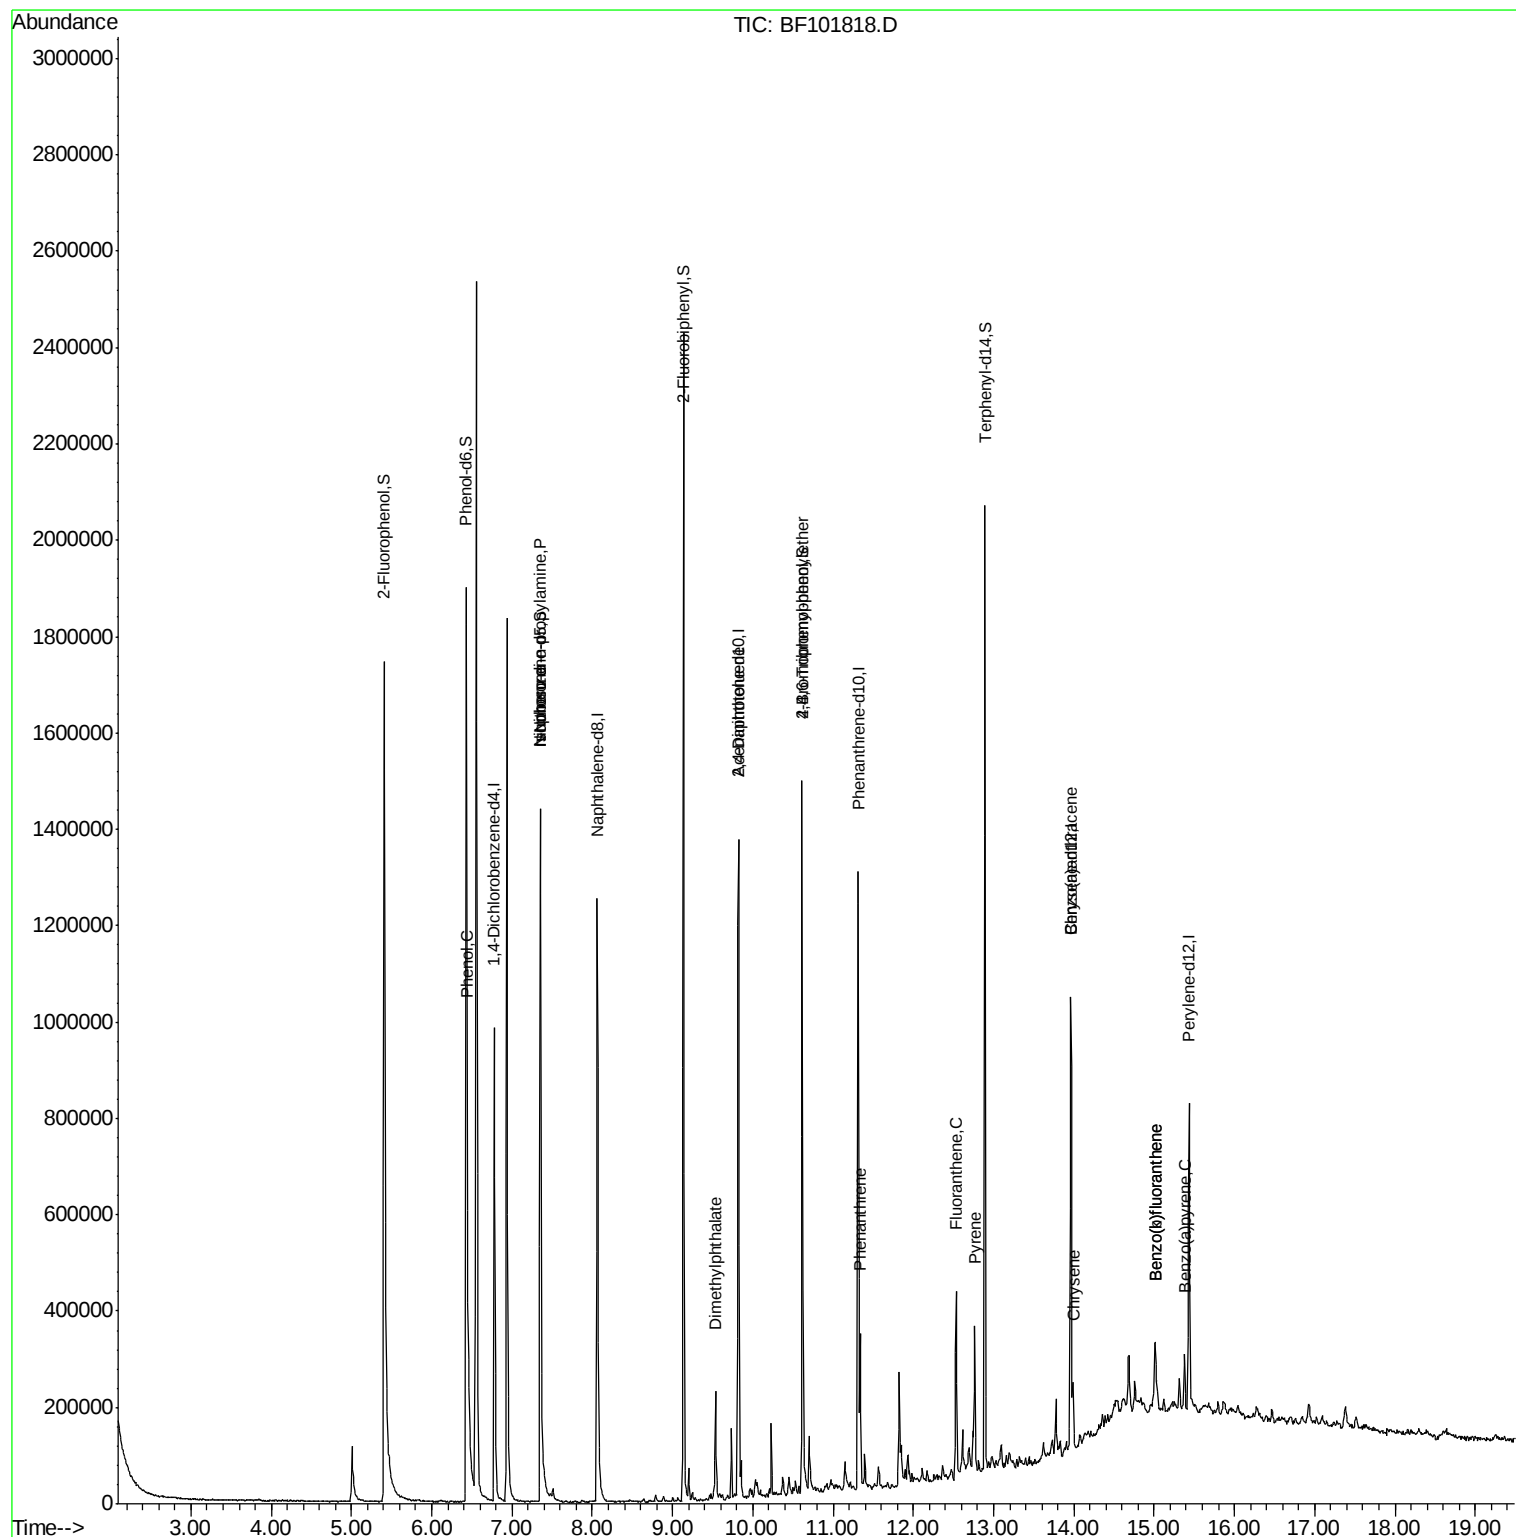



#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.78 min Scan# 798
 Delta R.T. 0.00 min
 Lab File: BF101818.D
 Acq: 29 Dec 2017 10:19

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.8	124.6	186.8
115	62.0	50.1	75.1

