
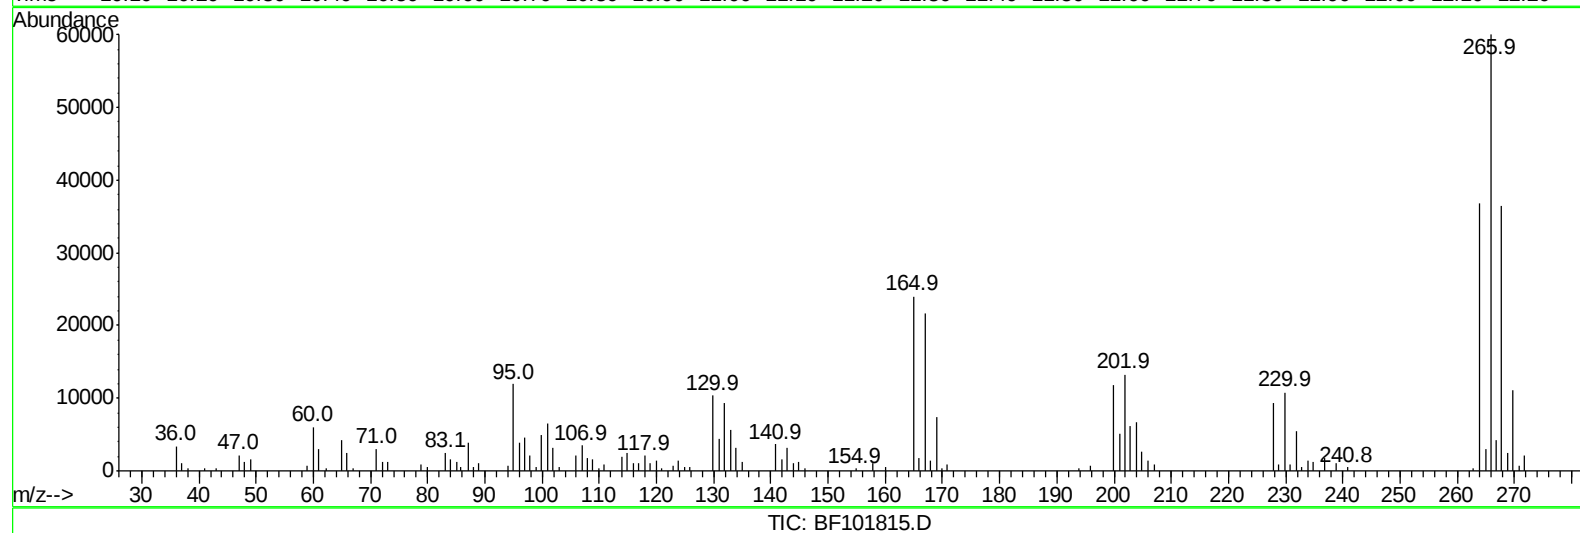


Data Path : Z:\HPCHEM1\BNA F\Data\BF122917\
Data File : BF101815.D
Acq On : 29 Dec 2017 8:52
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 01 00:00:54 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 13:21:45 2017
Response via : Initial Calibration

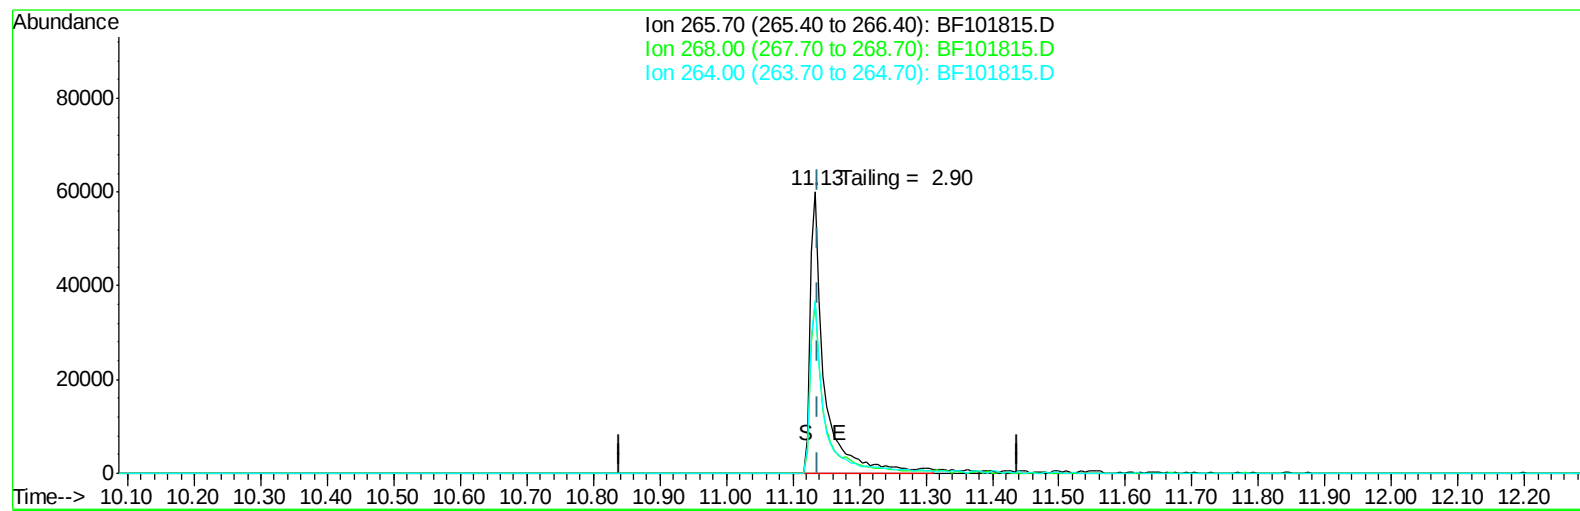

(69) Pentachlorophenol (C)



11.133min (-0.006) 48178.74ng

response 89543

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.86
264.00	61.90	61.27
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF122917\
Data File : BF101815.D
Acq On : 29 Dec 2017 8:52
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 01 00:00:54 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 13:21:45 2017
Response via : Initial Calibration

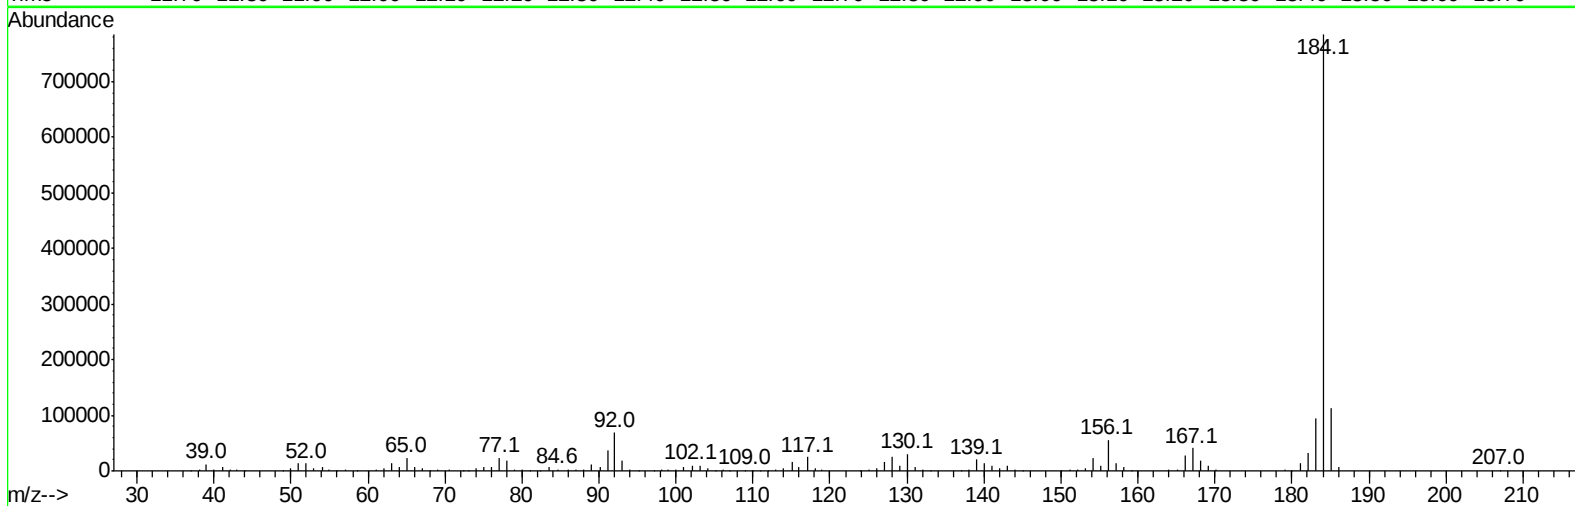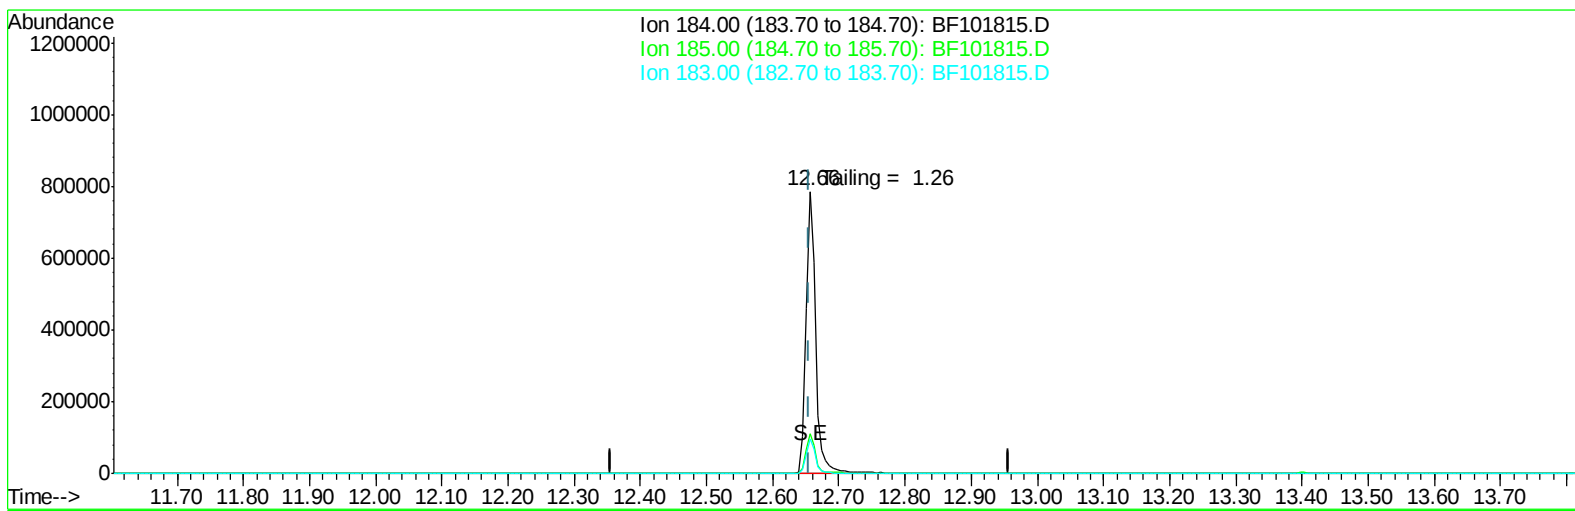

TIC: BF101815.D

(76) Benzidine

12.657min (+0.000) 0.00ng

response 813397

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.33
183.00	11.60	12.08
0.00	0.00	0.00