
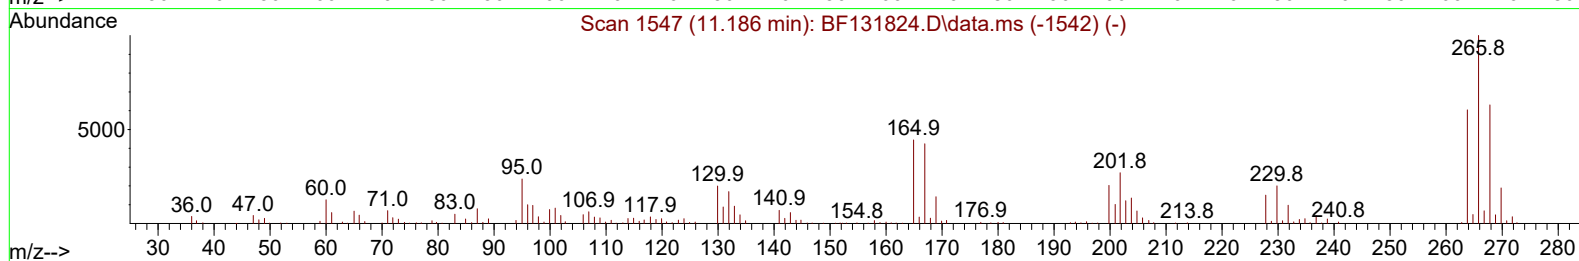
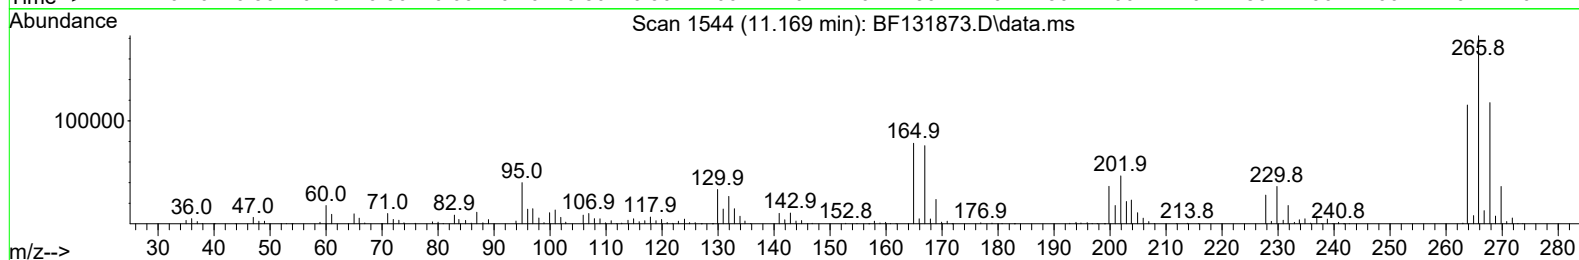


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF122922\  
Data File : BF131873.D  
Acq On : 29 Dec 2022 11:24  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 04:50:30 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF122422.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 30 02:06:40 2022  
Response via : Initial Calibration

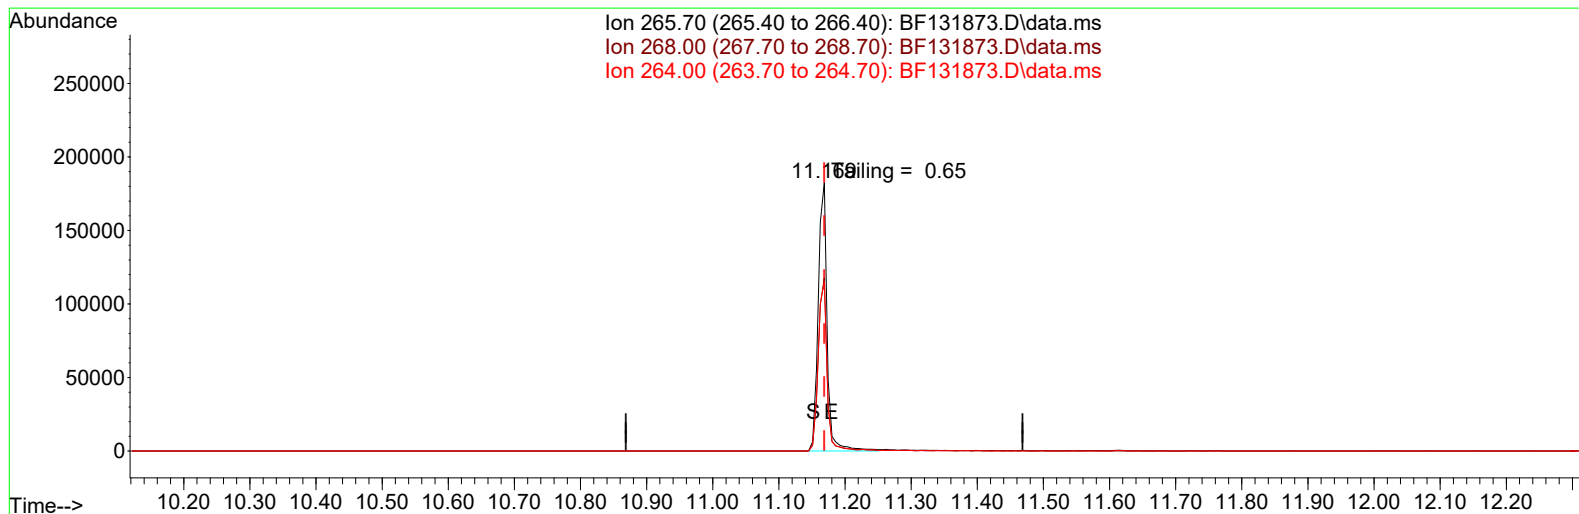

TIC: BF131873.D\data.ms

**(70) Pentachlorophenol (C)**




11.169min (-0.000) 30784.55 ng

response 173968

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.10  | 64.47  |
| 264.00 | 60.40  | 63.22  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF122922\  
Data File : BF131873.D  
Acq On : 29 Dec 2022 11:24  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 04:50:30 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF122422.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 30 02:06:40 2022  
Response via : Initial Calibration

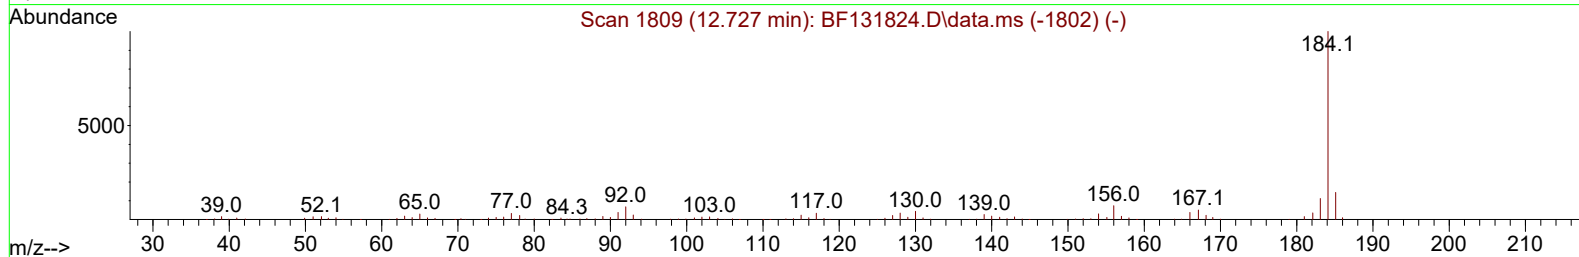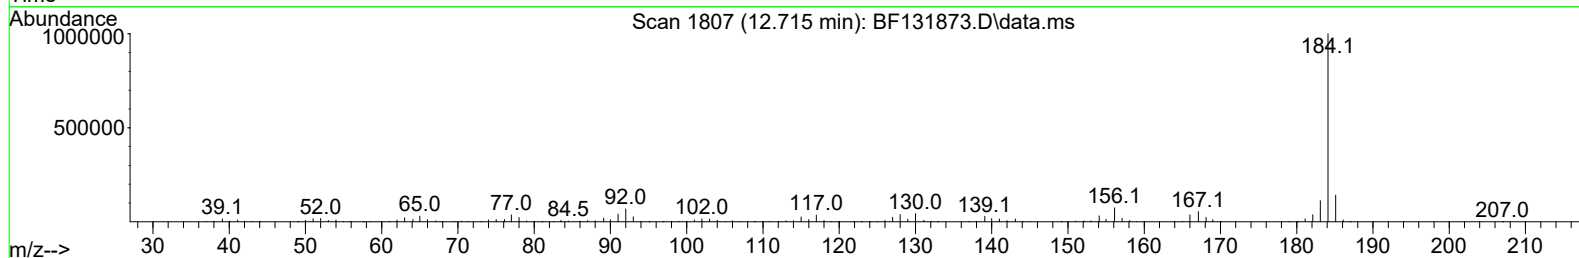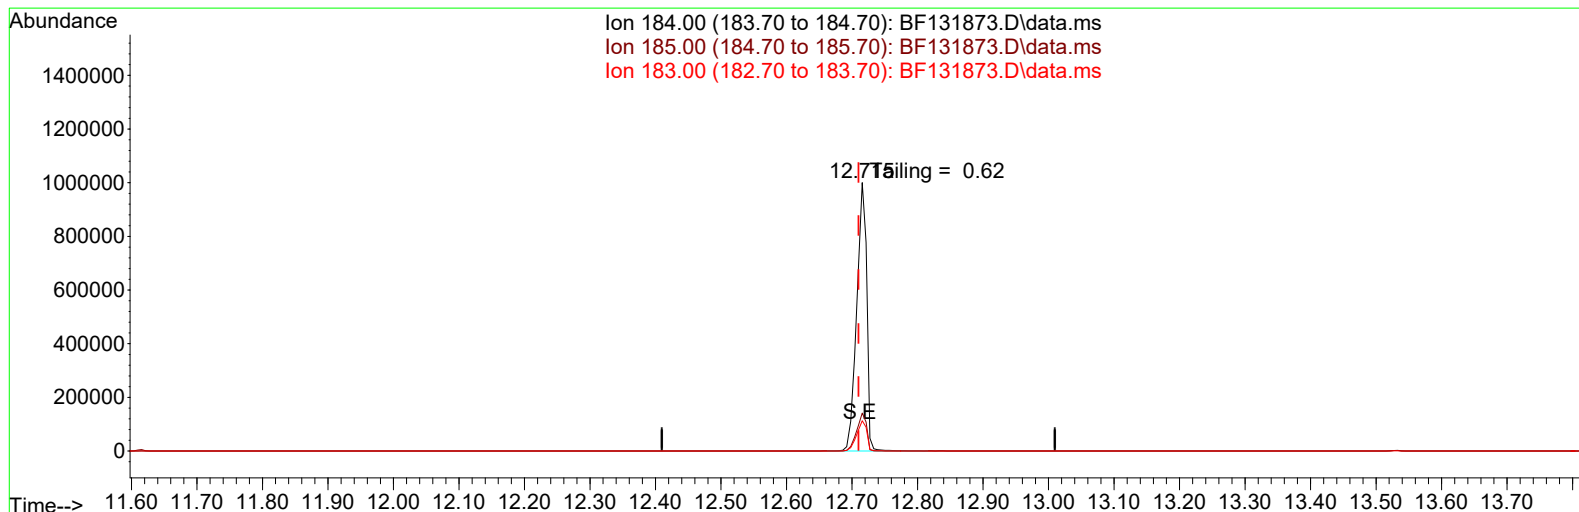

TIC: BF131873.D\data.ms

**(77) Benzidine**

12.715min (+ 0.006) 0.00 ng

response 1066149

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.50  | 14.15  |
| 183.00 | 11.20  | 11.27  |
| 0.00   | 0.00   | 0.00   |