


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122922\
 Data File : BF131873.D
 Acq On : 29 Dec 2022 11:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 30 02:06:40 2022

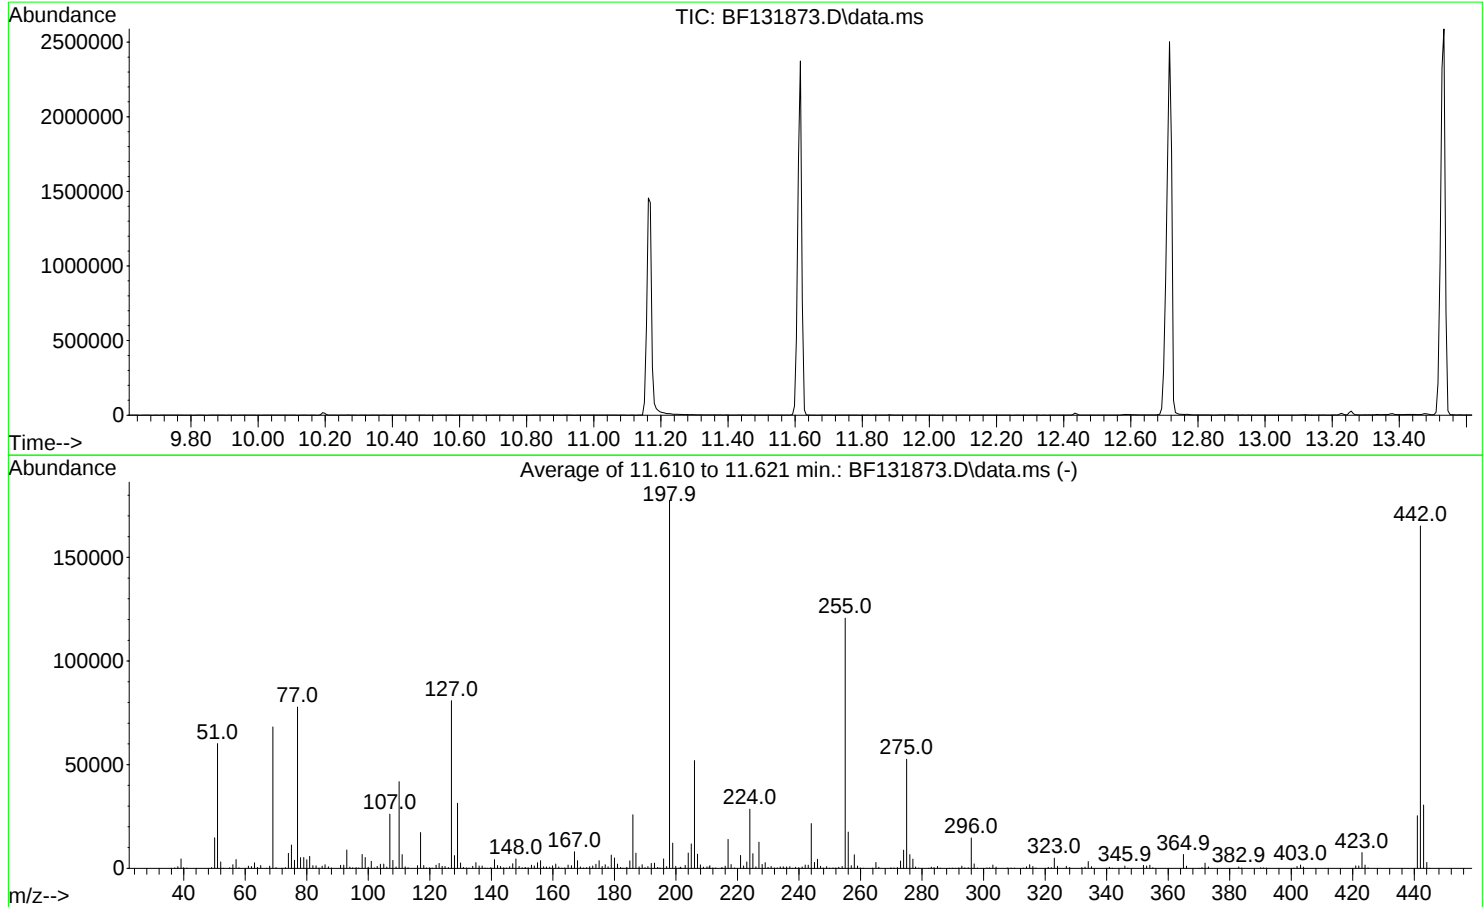




AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	60190	PASS
68	69	0.00	2	1.5	1054	PASS
69	198	0.00	100	38.4	68212	PASS
70	69	0.00	2	0.5	327	PASS
127	198	10	80	45.6	80891	PASS
197	198	0.00	2	0.5	846	PASS
198	198	100	100	100.0	177477	PASS
199	198	5	9	6.9	12178	PASS
275	198	10	60	29.6	52587	PASS
365	198	1	100	3.8	6663	PASS
441	198	0.01	100	14.3	25389	PASS
442	442	50	100	100.0	165131	PASS
443	442	15	24	18.5	30547	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122922\
Data File : BF131873.D
Acq On : 29 Dec 2022 11:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 30 04:50:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 30 02:06:40 2022
Response via : Initial Calibration

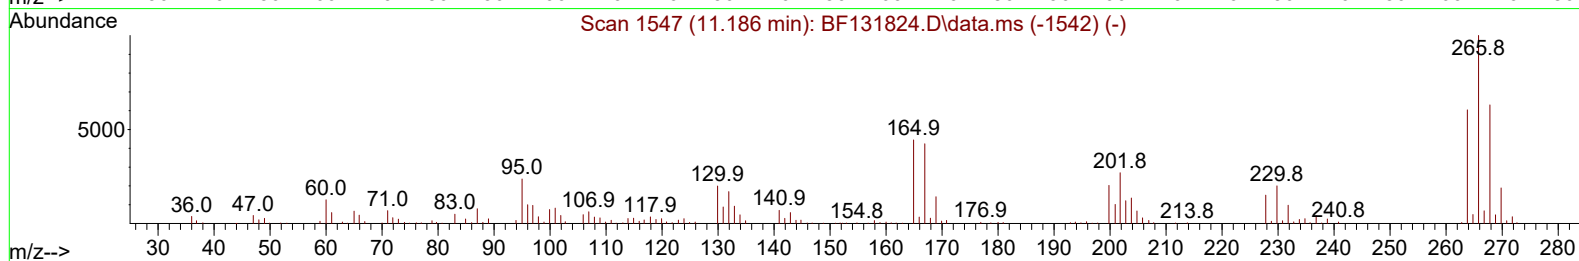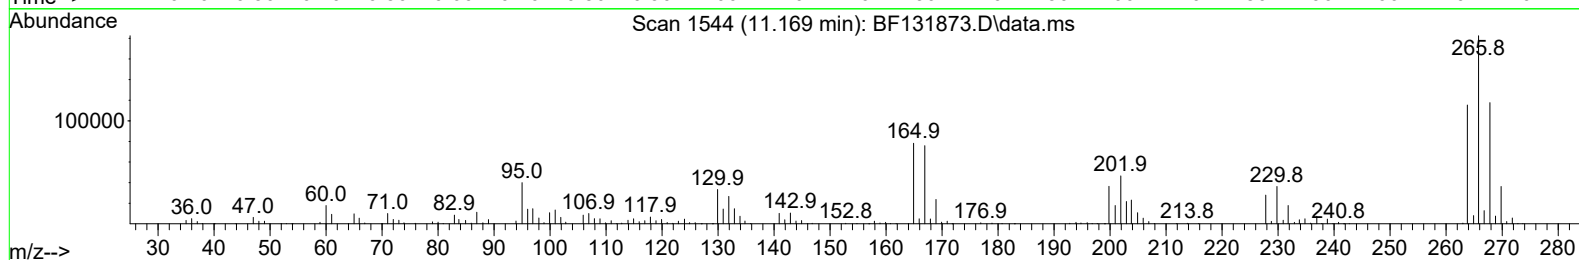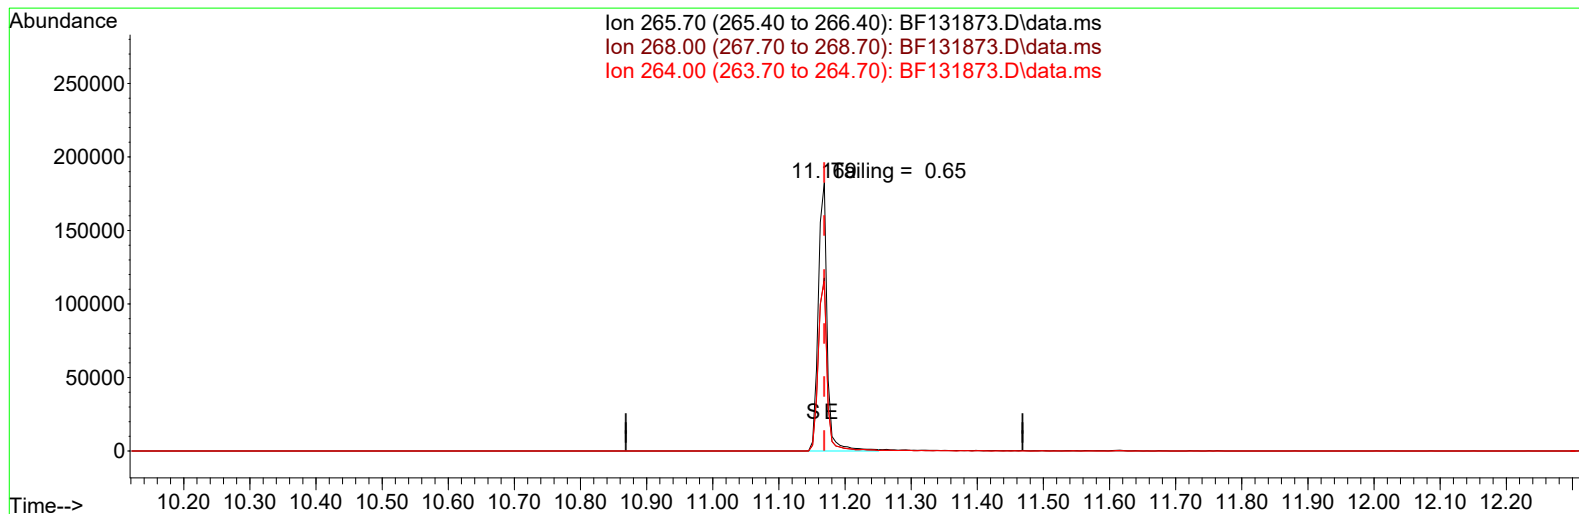

TIC: BF131873.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.000) 30784.55 ng




response 173968

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.47
264.00	60.40	63.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122922\
Data File : BF131873.D
Acq On : 29 Dec 2022 11:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 30 04:50:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 30 02:06:40 2022
Response via : Initial Calibration

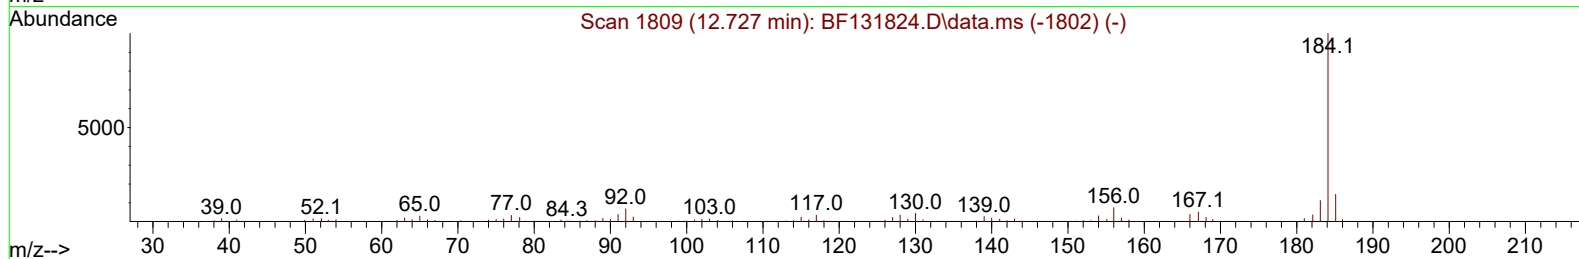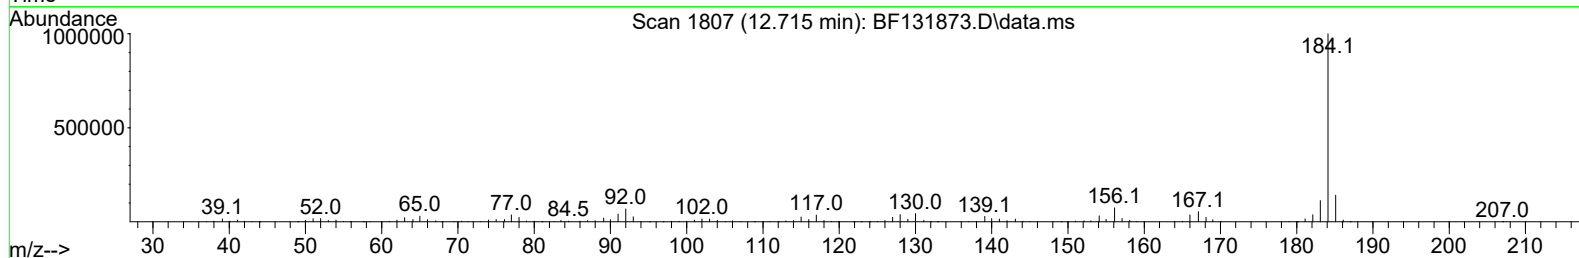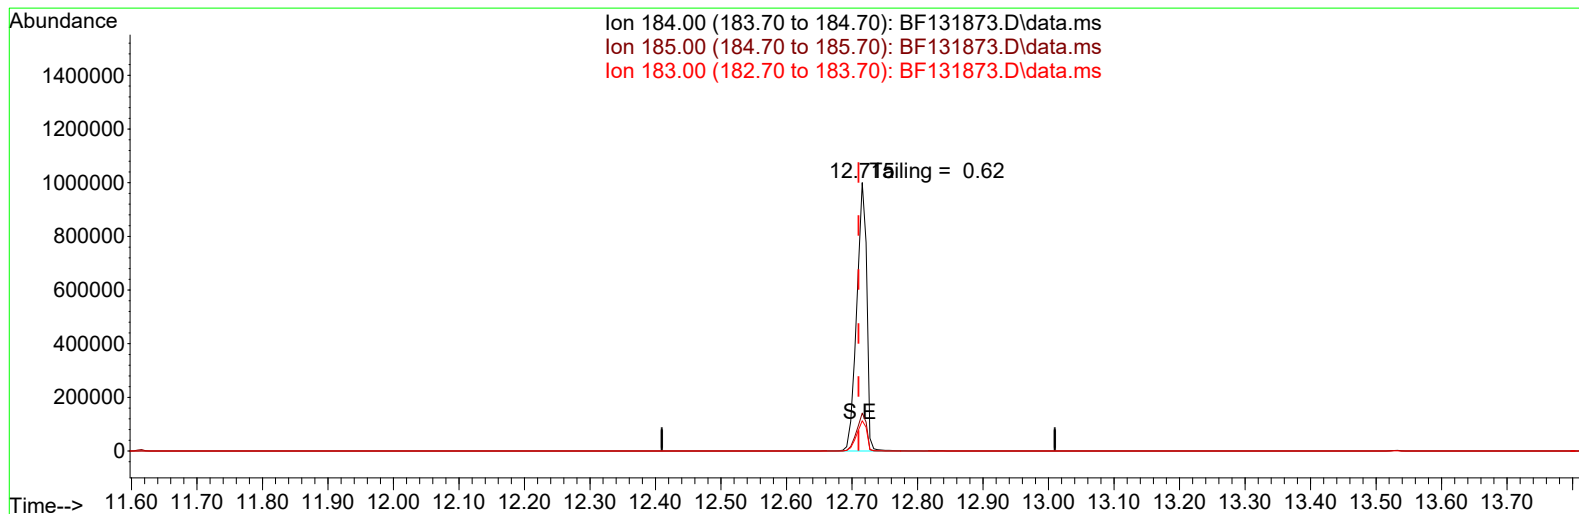

TIC: BF131873.D\data.ms

(77) Benzidine

12.715min (+ 0.006) 0.00 ng

response 1066149

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.15
183.00	11.20	11.27
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/29/2022	BNA_F	<u>BF131873.D</u>
Compound Name	Response	Retention Time
DDT	482894	13.533
DDD	6783	13.257
DDE	743	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7526	490420	1.53

Instrument :
BNA_F
ClientSampleId :
DFTPP