

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
 Data File : BF136836.D
 Acq On : 29 Dec 2023 18:46
 Operator : CG\JU
 Sample : 05897-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GHL-SS-39

Quant Time: Dec 30 01:03:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.781	152	72861	20.000	ng	-0.01
21) Naphthalene-d8	8.057	136	273379	20.000	ng	-0.01
39) Acenaphthene-d10	9.816	164	138483	20.000	ng	-0.01
64) Phenanthrene-d10	11.304	188	265406	20.000	ng	-0.01
76) Chrysene-d12	13.963	240	140813	20.000	ng	# 0.00
86) Perylene-d12	15.439	264	141590	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.422	112	403976	86.510	ng	0.00
7) Phenol-d6	6.428	99	508886	84.102	ng	-0.01
23) Nitrobenzene-d5	7.346	82	322624	60.389	ng	-0.01
42) 2,4,6-Tribromophenol	10.610	330	147453	90.410	ng	-0.01
45) 2-Fluorobiphenyl	9.134	172	646663	62.806	ng	-0.02
79) Terphenyl-d14	12.904	244	594164	58.967	ng	-0.01
Target Compounds						Qvalue
19) n-Nitroso-di-n-propyla...	7.346	70	42128	11.485	ng	# 70
25) Isophorone	7.346	82	322618	33.187	ng	# 65
50) Dimethylphthalate	9.816	163	28264	2.794	ng	# 1
51) 2,6-Dinitrotoluene	9.816	165	17627	7.678	ng	# 30
57) 2,4-Dinitrotoluene	9.816	165	17627	5.915	ng	# 21
67) 4-Bromophenyl-phenylether	10.610	248	8868	3.009	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136836.D
Acq On : 29 Dec 2023 18:46
Operator : CG\JU
Sample : 05897-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GHL-SS-39

Quant Time: Dec 30 01:03:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration




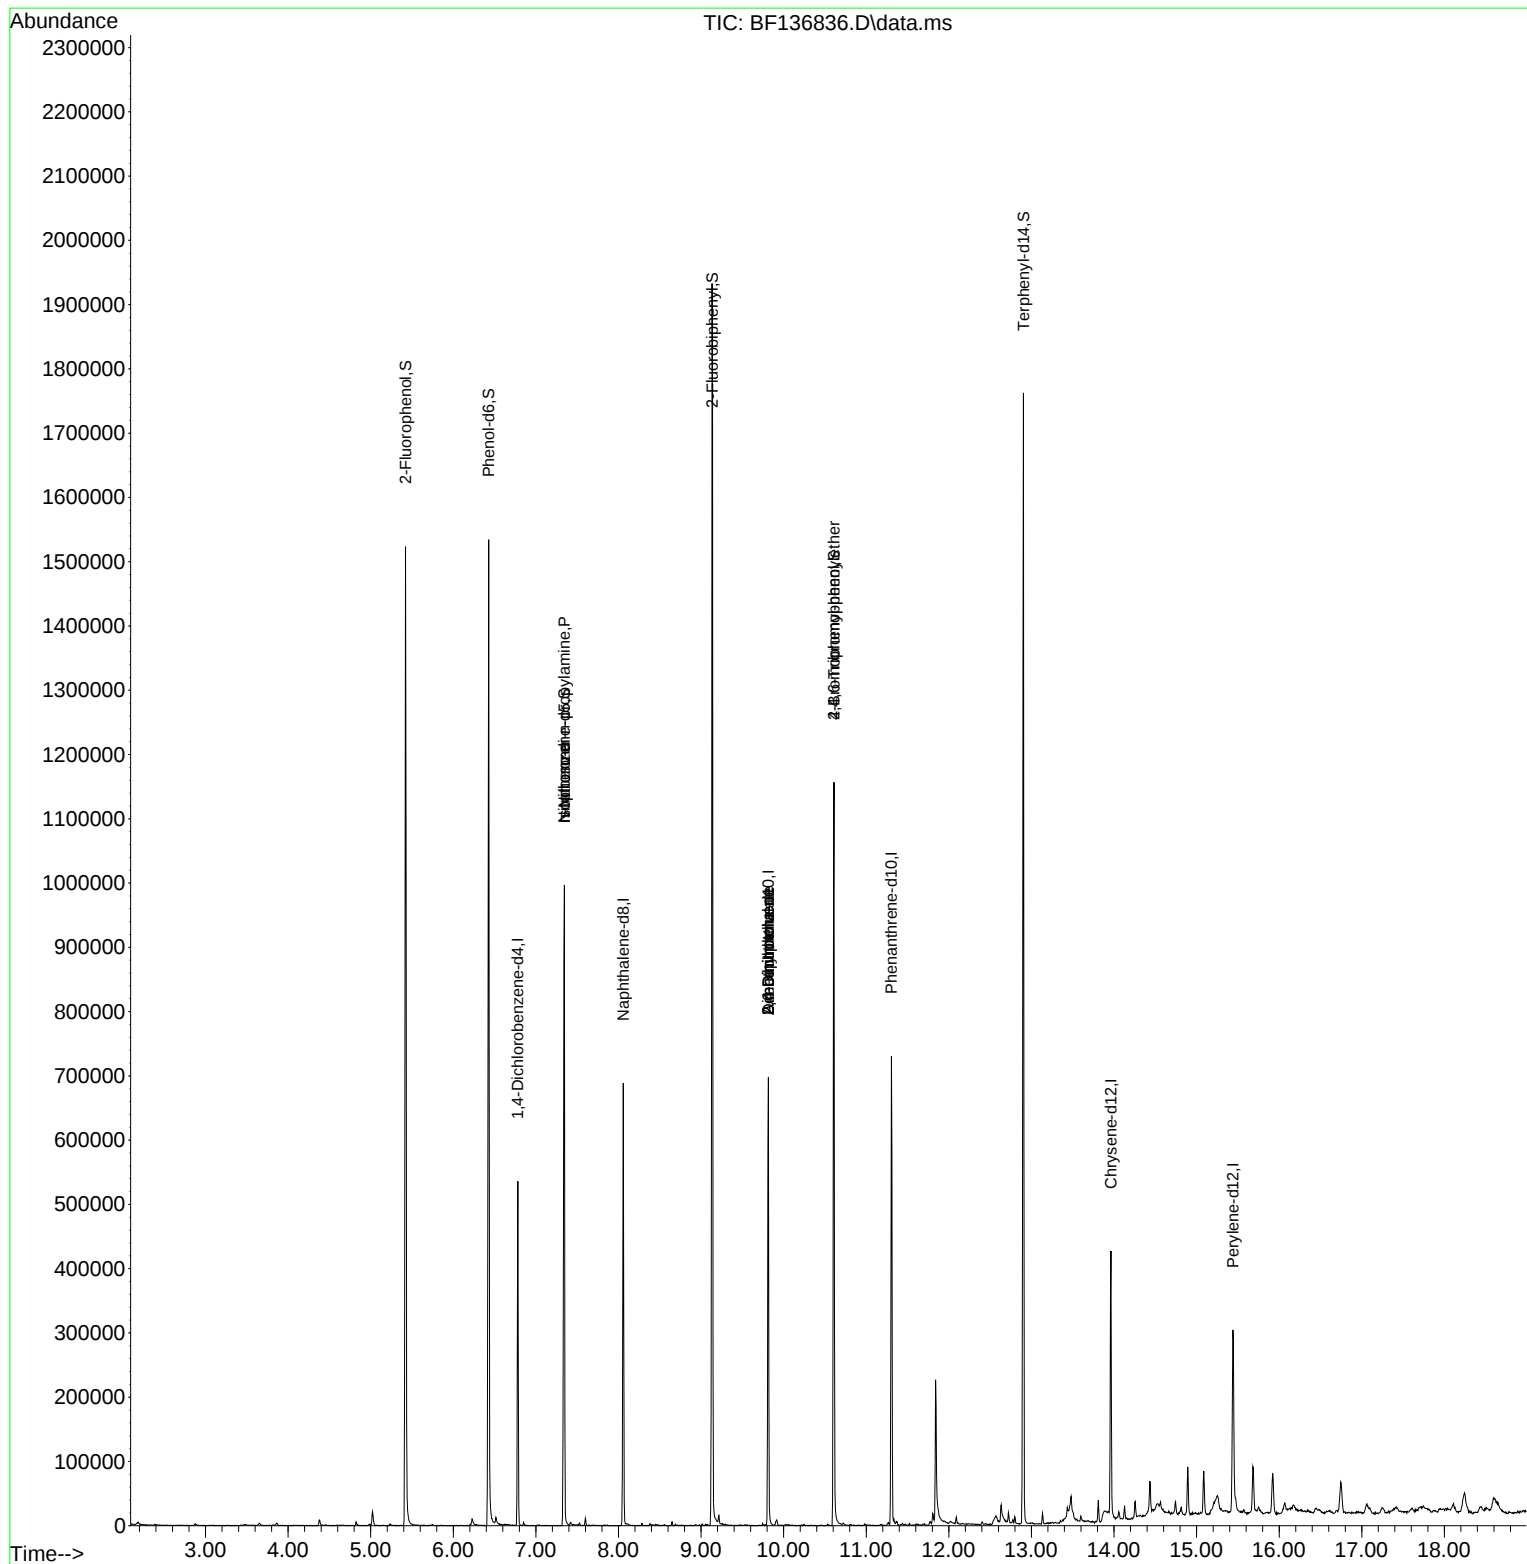


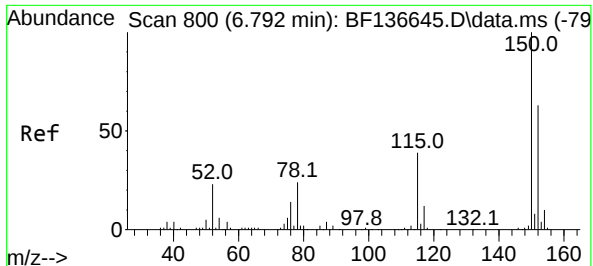

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.781 min Scan# 79
Delta R.T. -0.011 min
Lab File: BF136836.D
Acq: 29 Dec 2023 18:46




Instrument :
BNA_F
ClientSampleId :
GHL-SS-39


Tgt Ion:152 Resp: 72861
Ion Ratio Lower Upper
152 100
150 154.7 127.0 190.6
115 58.4 49.0 73.4

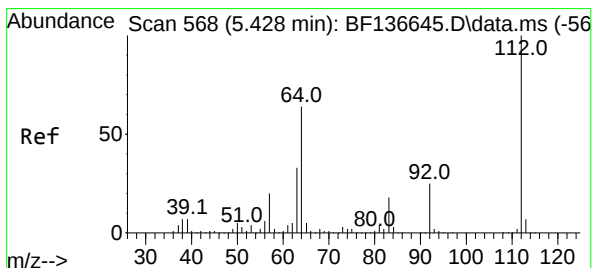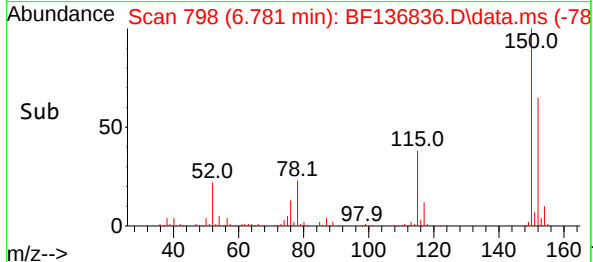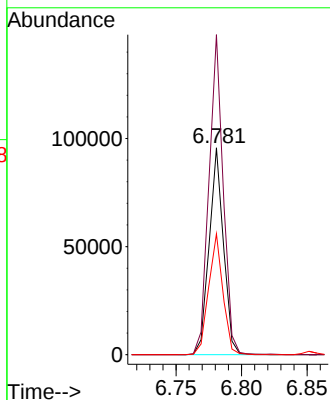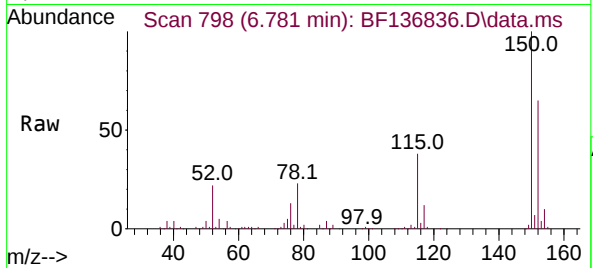

#5
2-Fluorophenol
Concen: 86.510 ng
RT: 5.422 min Scan# 567
Delta R.T. -0.006 min
Lab File: BF136836.D
Acq: 29 Dec 2023 18:46

Tgt Ion:112 Resp: 403976
Ion Ratio Lower Upper
112 100
64 64.1 51.1 76.7
63 31.7 26.1 39.1


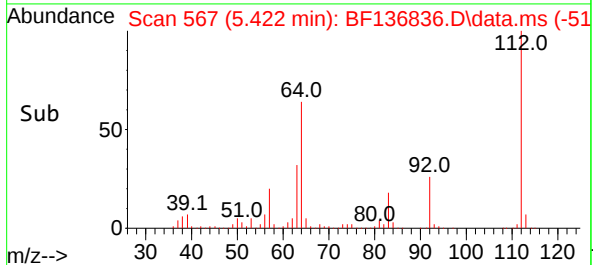
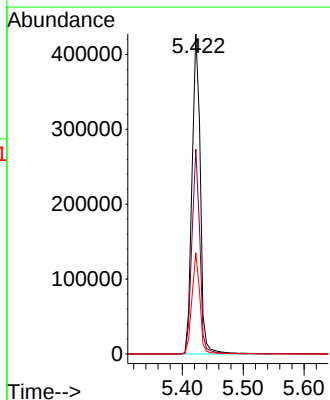
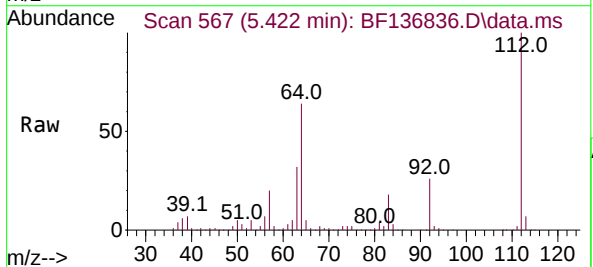


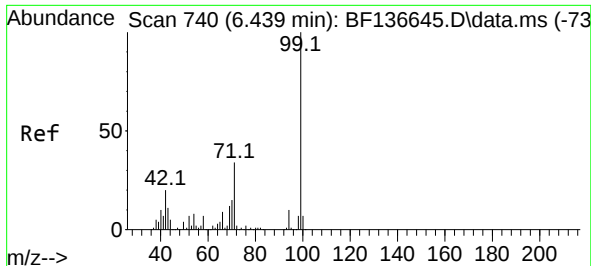

#7
Phenol-d6
Concen: 84.102 ng
RT: 6.428 min Scan# 71
Delta R.T. -0.011 min
Lab File: BF136836.D
Acq: 29 Dec 2023 18:46




Instrument :
BNA_F
ClientSampleId :
GHL-SS-39

Tgt Ion: 99 Resp: 508886
Ion Ratio Lower Upper
99 100
42 19.9 16.1 24.1
71 33.1 27.4 41.2

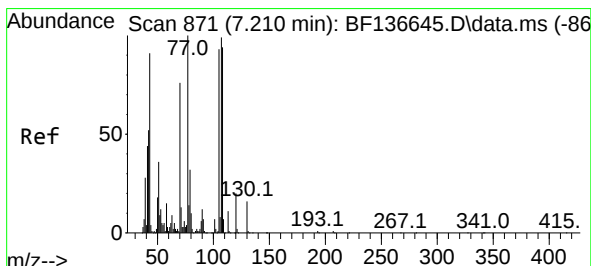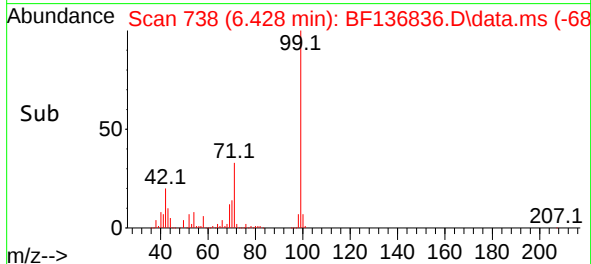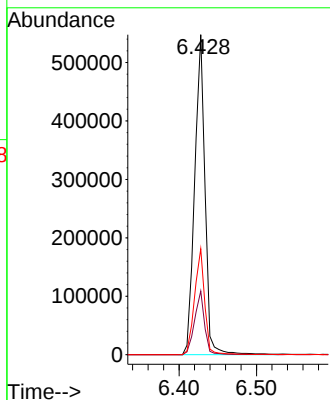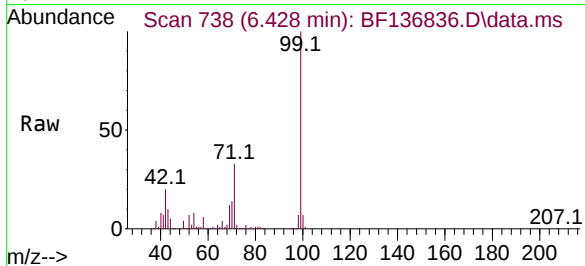

#19
n-Nitroso-di-n-propylamine
Concen: 11.485 ng
RT: 7.346 min Scan# 894
Delta R.T. 0.136 min
Lab File: BF136836.D
Acq: 29 Dec 2023 18:46

Tgt Ion: 70 Resp: 42128
Ion Ratio Lower Upper
70 100
42 46.0 54.2 81.4#
101 0.0 7.6 11.4#
130 2.5 17.1 25.7#

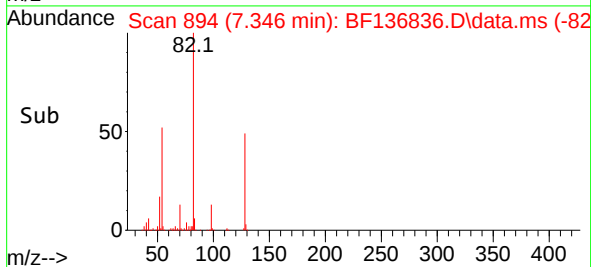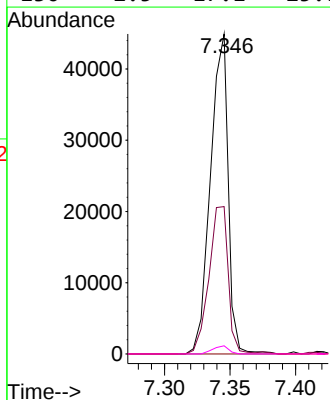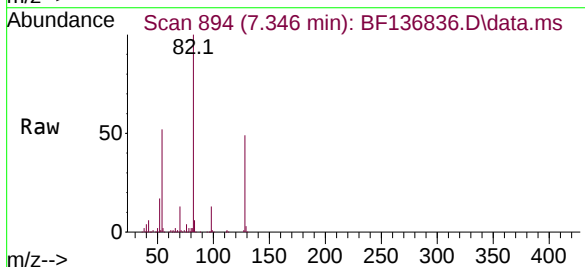







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.057 min Scan# 1015
Delta R.T. -0.011 min
Lab File: BF136836.D
Acq: 29 Dec 2023 18:46

Instrument :
BNA_F
ClientSampleId :
GHL-SS-39

Tgt Ion:136 Resp: 273379




Ion	Ratio	Lower	Upper
136	100		
137	10.4	9.0	13.4
54	7.6	7.2	10.8
68	5.5	4.9	7.3

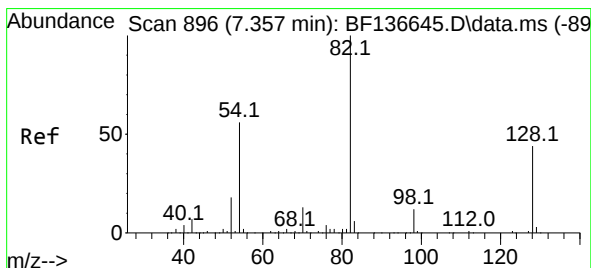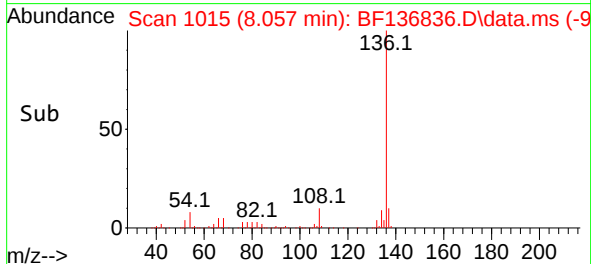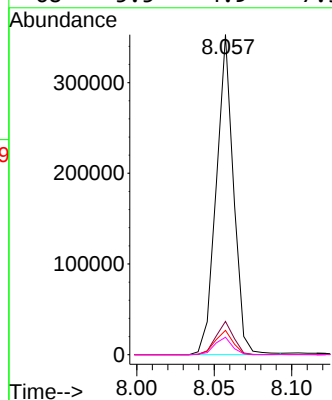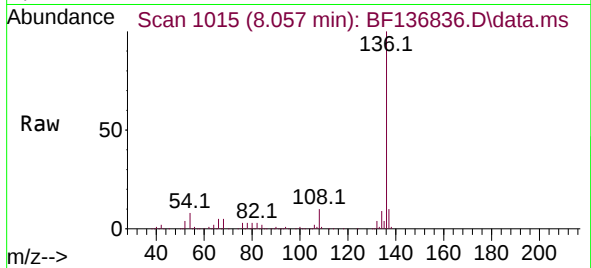

#23
Nitrobenzene-d5
Concen: 60.389 ng
RT: 7.346 min Scan# 894
Delta R.T. -0.011 min
Lab File: BF136836.D
Acq: 29 Dec 2023 18:46

Tgt Ion: 82 Resp: 322624


Ion	Ratio	Lower	Upper
82	100		
128	48.6	35.3	52.9
54	51.6	44.5	66.7

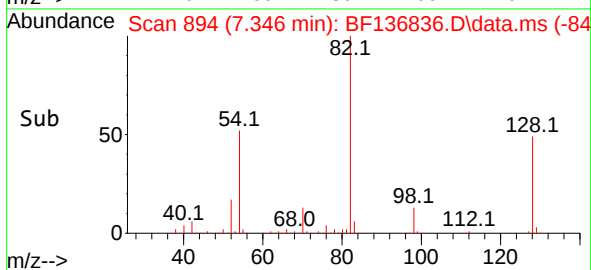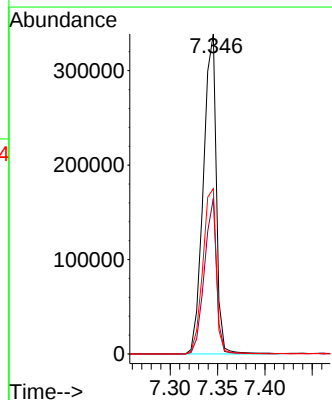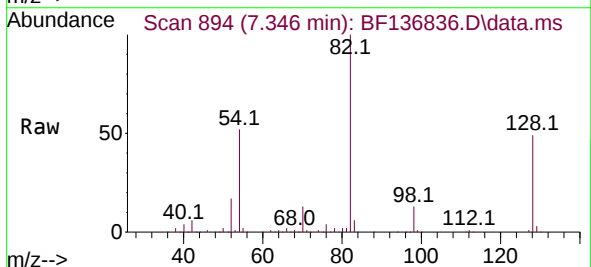






#25
Isophorone
Concen: 33.187 ng
RT: 7.346 min Scan# 894
Delta R.T. -0.270 min
Lab File: BF136836.D
Acq: 29 Dec 2023 18:46


Instrument :
BNA_F
ClientSampleId :
GHL-SS-39

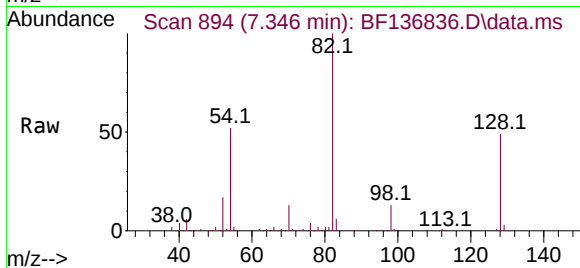



Tgt Ion: 82 Resp: 322618
Ion Ratio Lower Upper
82 100
95 0.0 5.5 8.3#
138 0.0 14.5 21.7#

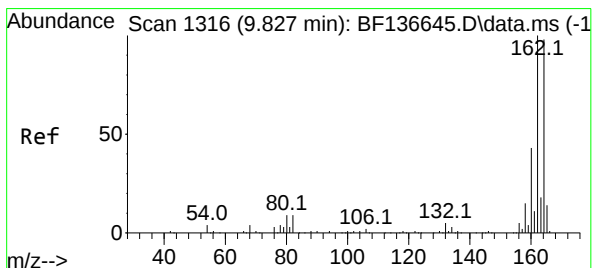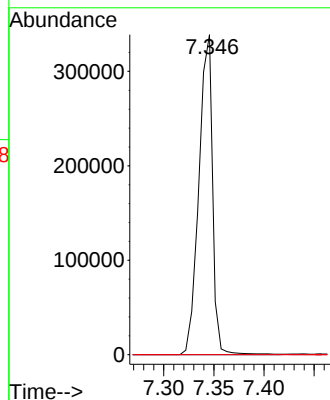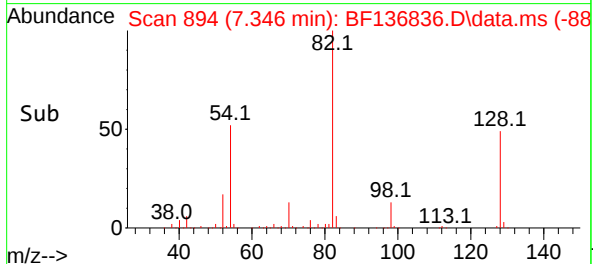

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.816 min Scan# 1314
Delta R.T. -0.011 min
Lab File: BF136836.D
Acq: 29 Dec 2023 18:46

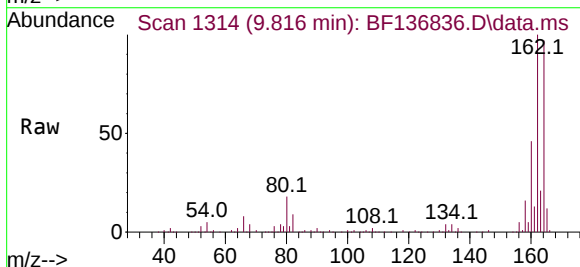

Tgt Ion:164 Resp: 138483
Ion Ratio Lower Upper
164 100
162 102.8 81.6 122.4
160 47.4 34.9 52.3

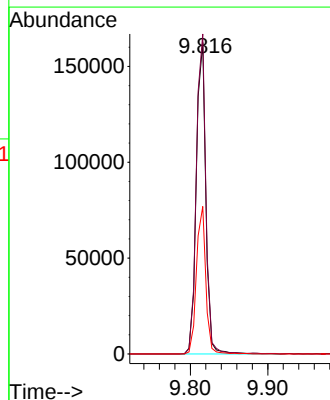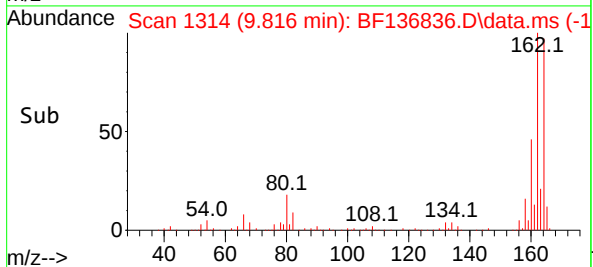



#42

2,4,6-Tribromophenol

Concen: 90.410 ng

RT: 10.610 min Scan# 1451

Delta R.T. -0.011 min

Lab File: BF136836.D

Acq: 29 Dec 2023 18:46

Instrument :

BNA_F

ClientSampleId :

GHL-SS-39




Tgt Ion:330 Resp: 147453

Ion Ratio Lower Upper

330 100

332 95.2 77.4 116.0

141 28.2 23.4 35.2

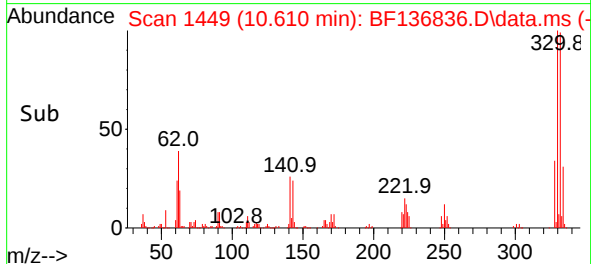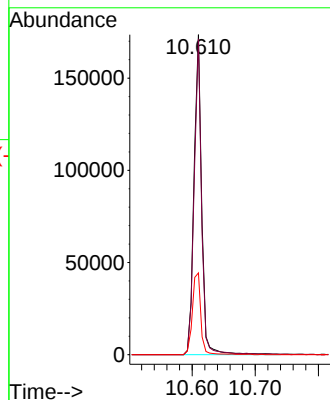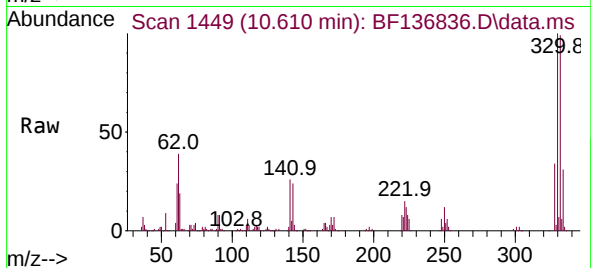

#45

2-Fluorobiphenyl

Concen: 62.806 ng

RT: 9.134 min Scan# 1198

Delta R.T. -0.017 min

Lab File: BF136836.D

Acq: 29 Dec 2023 18:46




Tgt Ion:172 Resp: 646663


Ion Ratio Lower Upper

172 100

171 36.1 29.0 43.6

170 23.3 19.0 28.4

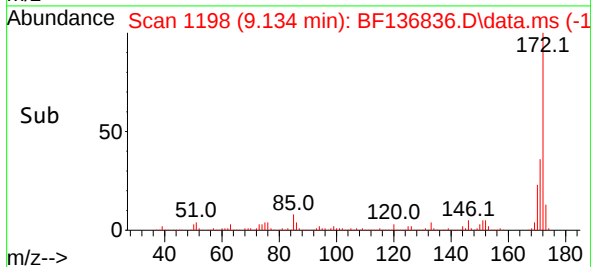
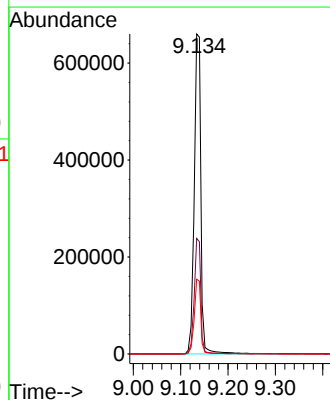
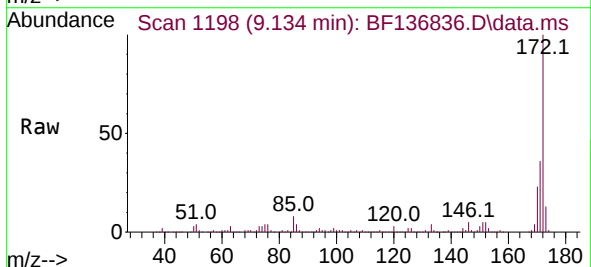


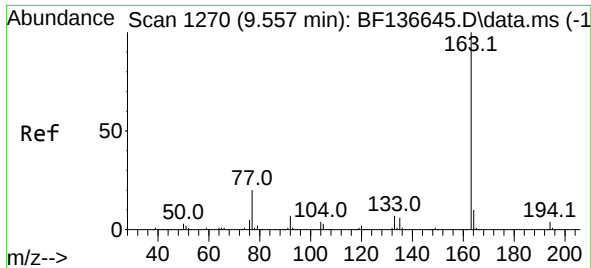

#50
Dimethylphthalate
Concen: 2.794 ng
RT: 9.816 min Scan# 11
Delta R.T. 0.259 min
Lab File: BF136836.D
Acq: 29 Dec 2023 18:46




Instrument :
BNA_F
ClientSampleId :
GHL-SS-39

Tgt Ion:163 Resp: 28264
Ion Ratio Lower Upper
163 100
194 0.0 3.3 4.9#
164 472.0 7.8 11.6#

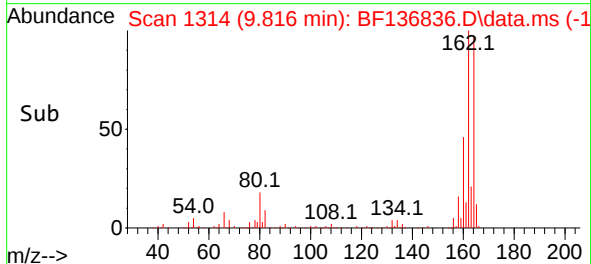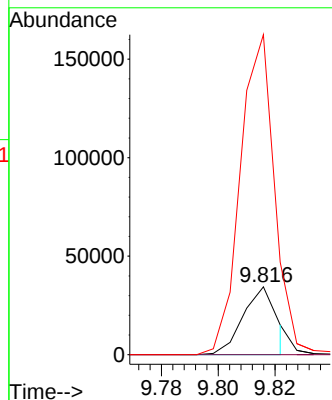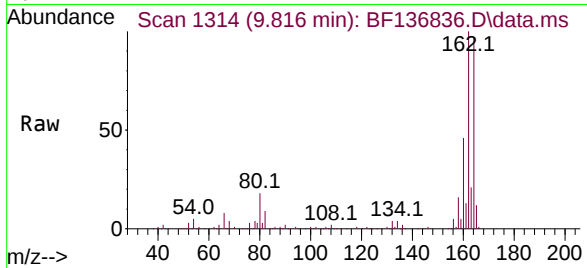

#51
2,6-Dinitrotoluene
Concen: 7.678 ng
RT: 9.816 min Scan# 1314
Delta R.T. 0.194 min
Lab File: BF136836.D
Acq: 29 Dec 2023 18:46

Tgt Ion:165 Resp: 17627
Ion Ratio Lower Upper
165 100
63 1.3 39.8 59.6#
89 1.0 38.8 58.2#

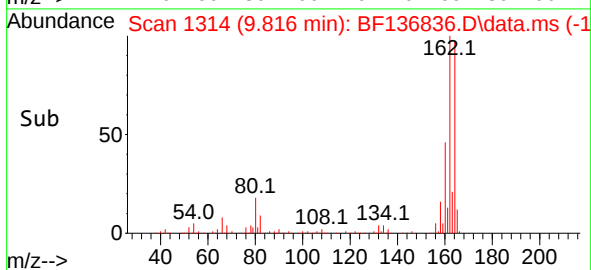
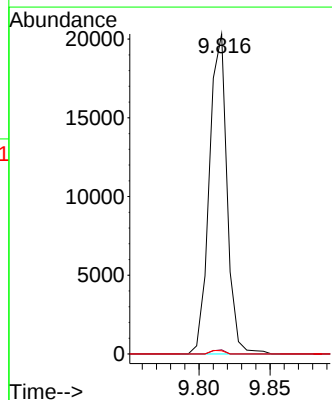
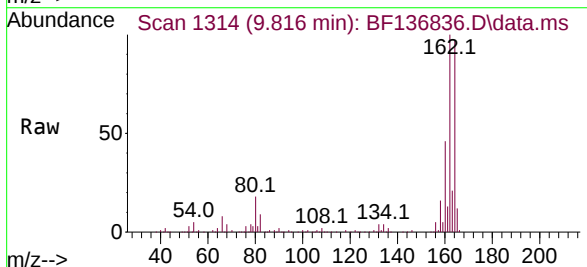




#57
2,4-Dinitrotoluene
Concen: 5.915 ng
RT: 9.816 min Scan# 11
Delta R.T. -0.206 min
Lab File: BF136836.D
Acq: 29 Dec 2023 18:46




Instrument :
BNA_F
ClientSampleId :
GHL-SS-39


Tgt Ion:165 Resp: 17627
Ion Ratio Lower Upper
165 100
63 1.3 41.0 61.6#
89 1.0 59.9 89.9#
182 0.0 2.0 3.0#

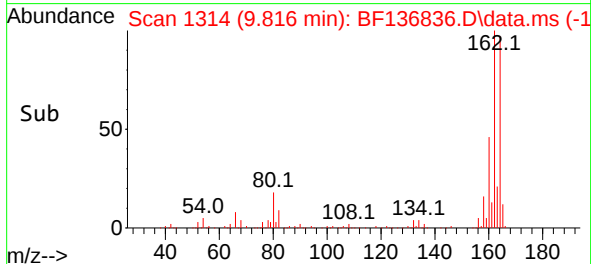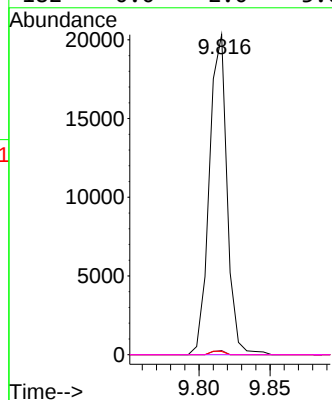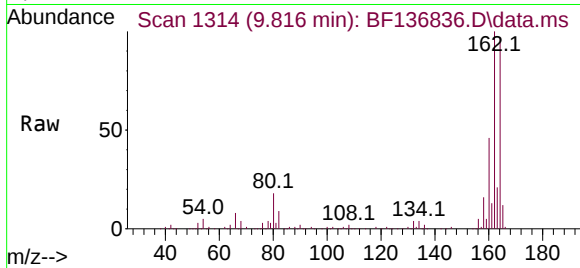

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.304 min Scan# 1567
Delta R.T. -0.011 min
Lab File: BF136836.D
Acq: 29 Dec 2023 18:46

Tgt Ion:188 Resp: 265406
Ion Ratio Lower Upper
188 100
94 9.4 7.5 11.3
80 10.5 8.1 12.1


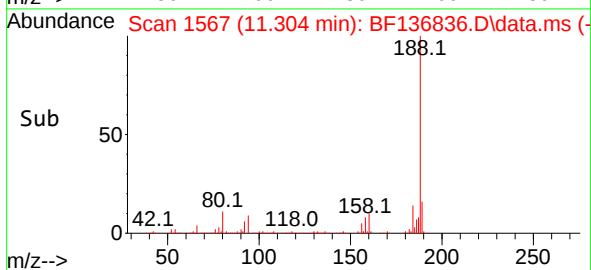
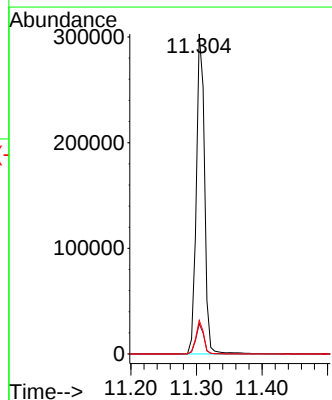
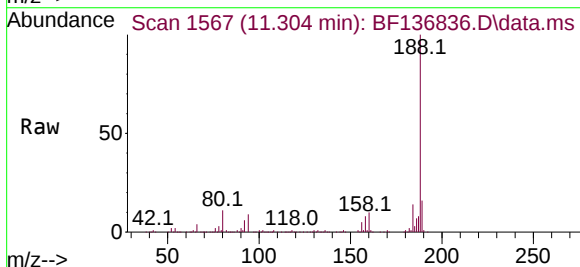


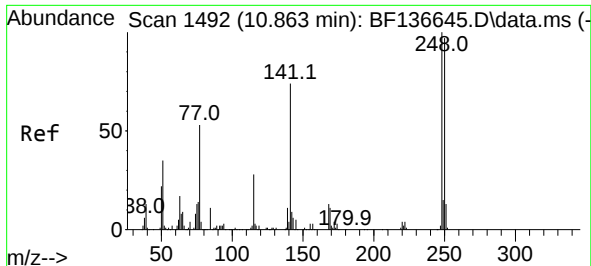

#67
4-Bromophenyl-phenylether
Concen: 3.009 ng
RT: 10.610 min Scan# 1492
Delta R.T. -0.253 min
Lab File: BF136836.D
Acq: 29 Dec 2023 18:46




Instrument :
BNA_F
ClientSampleId :
GHL-SS-39

Tgt Ion:248 Resp: 8868
Ion Ratio Lower Upper
248 100
250 201.7 77.8 116.6#
141 431.1 59.2 88.8#

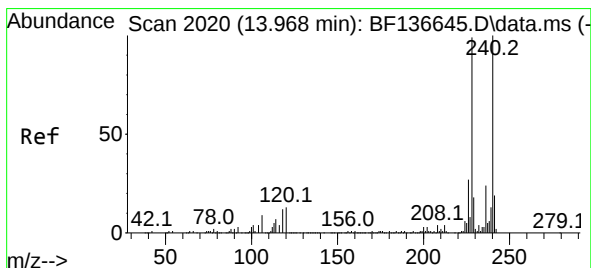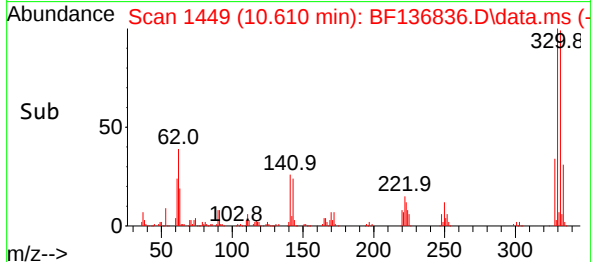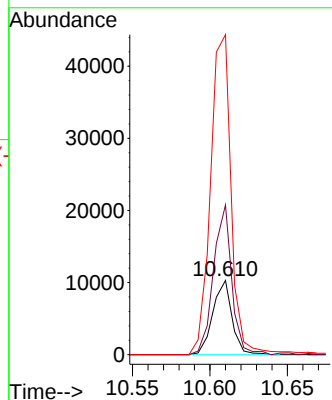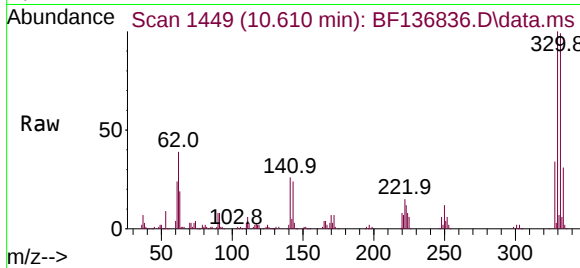

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.963 min Scan# 2019
Delta R.T. -0.006 min
Lab File: BF136836.D
Acq: 29 Dec 2023 18:46


Tgt Ion:240 Resp: 140813
Ion Ratio Lower Upper
240 100
120 9.5 10.3 15.5#
236 25.5 19.4 29.2

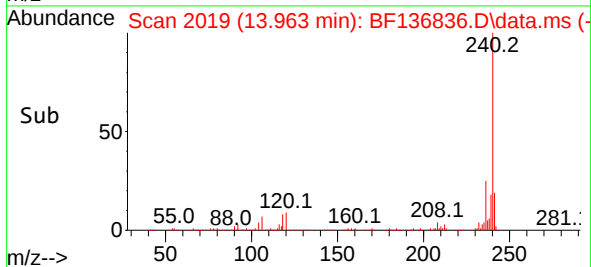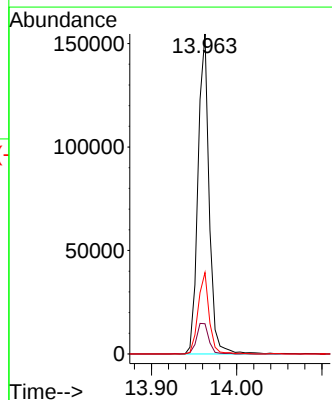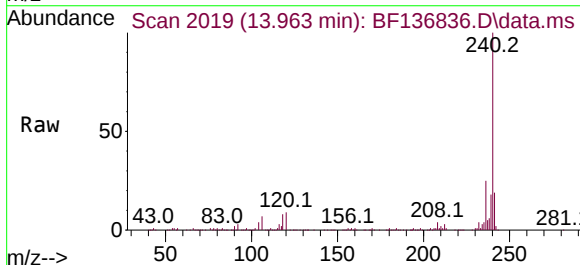






#79
 Terphenyl-d14
 Concen: 58.967 ng
 RT: 12.904 min Scan# 1839
 Delta R.T. -0.011 min
 Lab File: BF136836.D
 Acq: 29 Dec 2023 18:46

Instrument :
 BNA_F
 ClientSampleId :
 GHL-SS-39

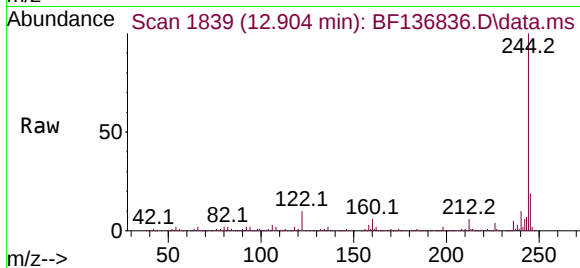

Tgt Ion:244 Resp: 594164
 Ion Ratio Lower Upper
 244 100
 212 6.3 5.0 7.4
 122 10.1 9.0 13.4

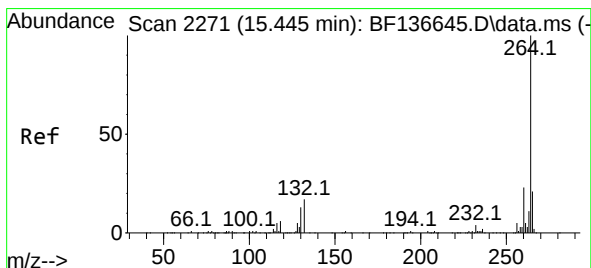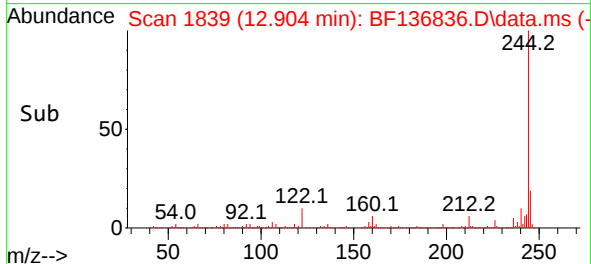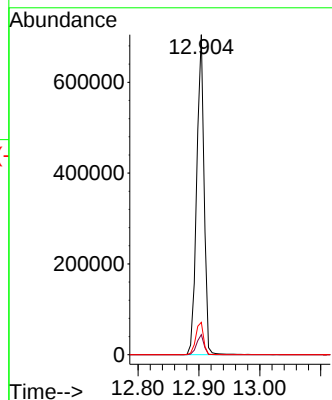

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.439 min Scan# 2270
 Delta R.T. -0.006 min
 Lab File: BF136836.D
 Acq: 29 Dec 2023 18:46

Tgt Ion:264 Resp: 141590
 Ion Ratio Lower Upper
 264 100
 260 23.9 18.3 27.5
 265 20.9 17.0 25.6

