
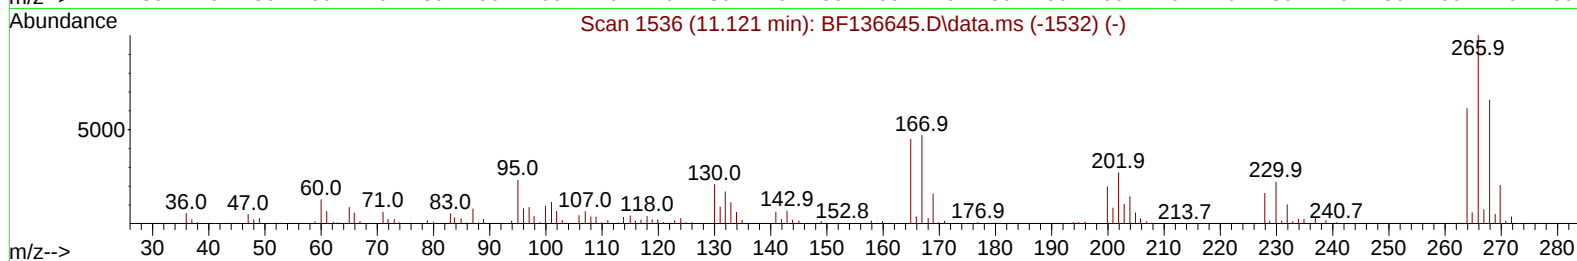
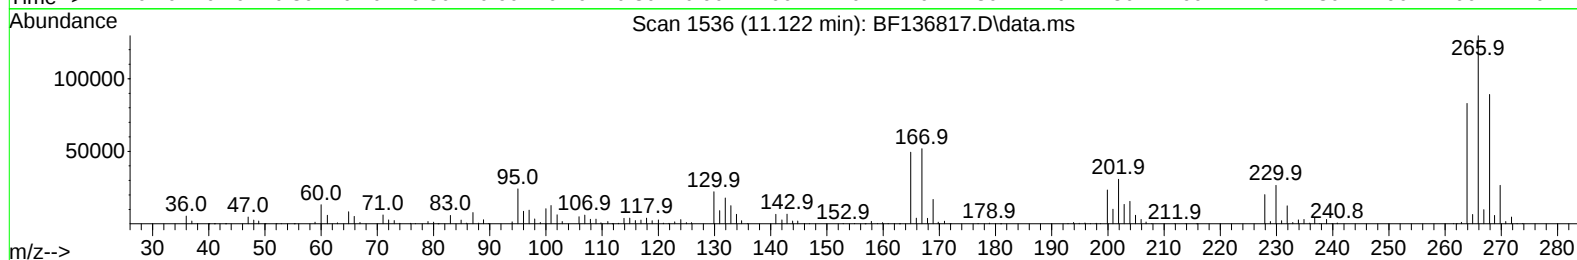


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136817.D
Acq On : 29 Dec 2023 09:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 10:08:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

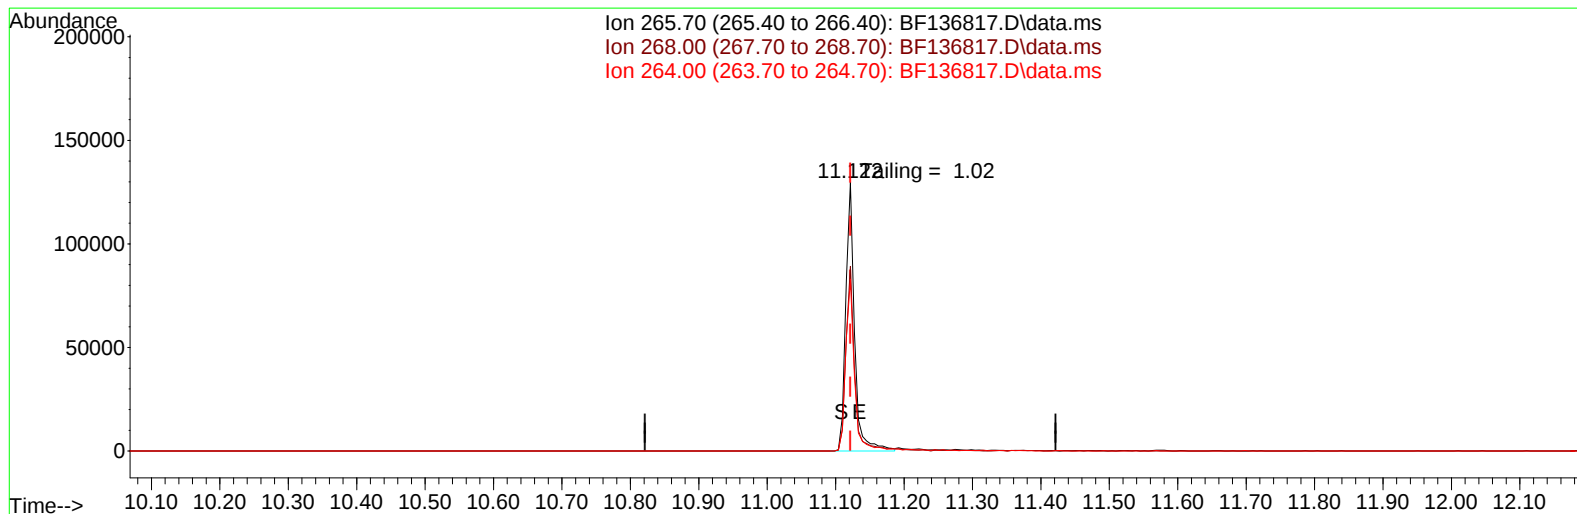

TIC: BF136817.D\data.ms

(70) Pentachlorophenol (C)




11.122min (+ 0.000) 39770.90 ng

response 116550

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	68.78
264.00	61.20	64.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136817.D
Acq On : 29 Dec 2023 09:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 10:08:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

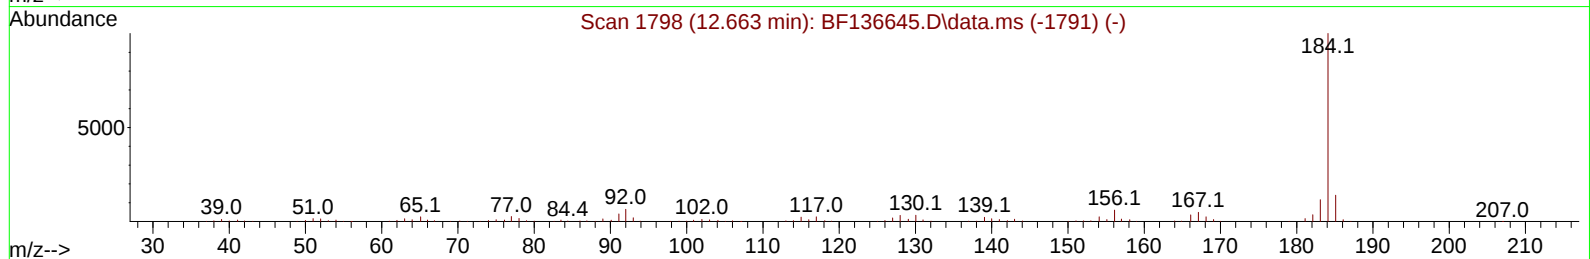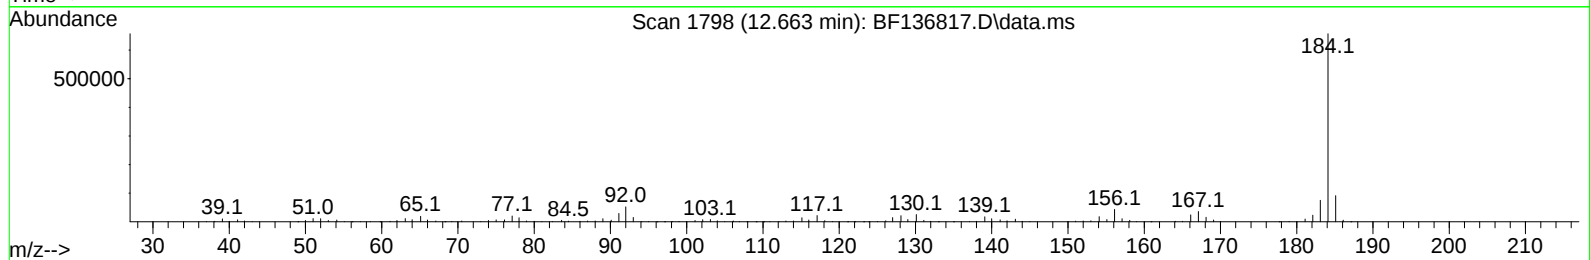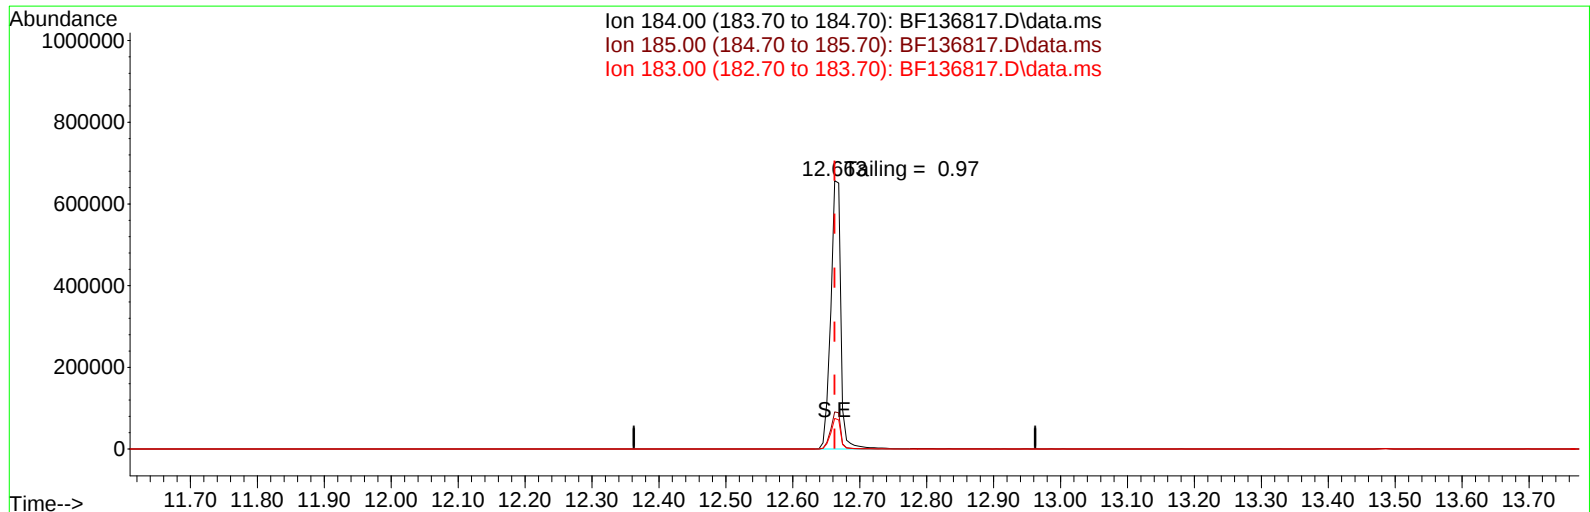

TIC: BF136817.D\data.ms

(77) Benzidine**12.663min (+ 0.000) 374275.79 ng****response 684219**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.86
183.00	11.60	11.42
0.00	0.00	0.00