
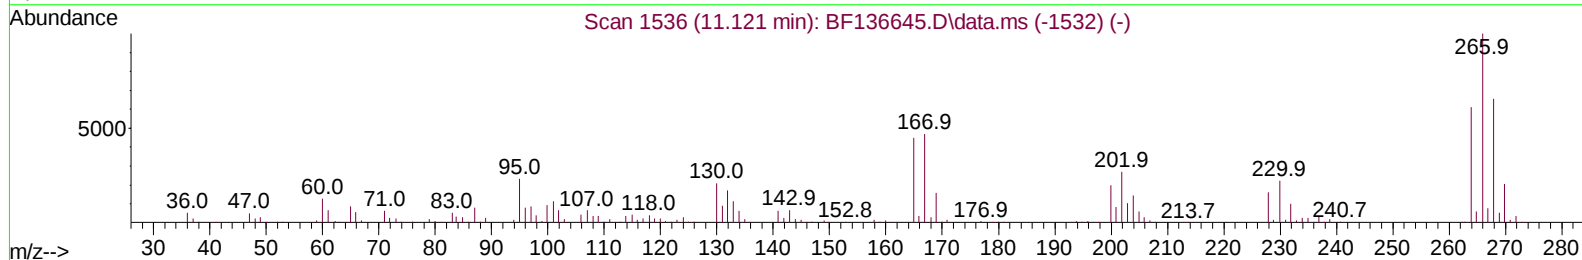
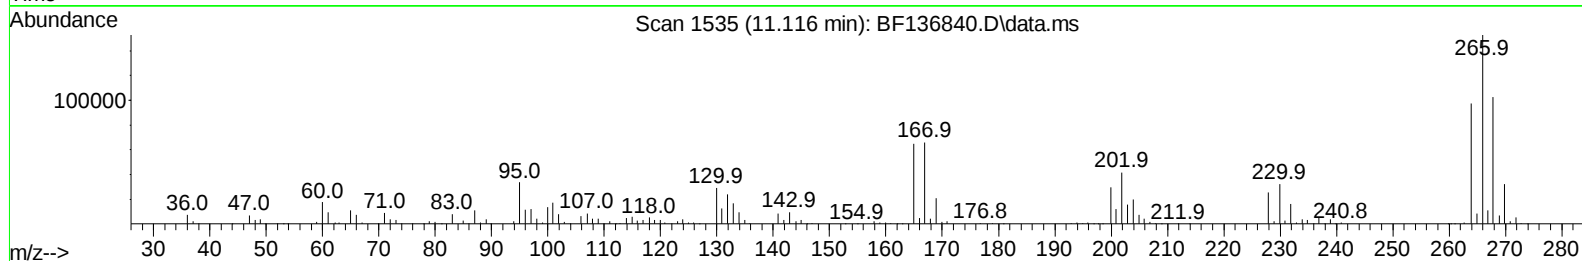


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF122923\  
Data File : BF136840.D  
Acq On : 29 Dec 2023 21:23  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 01:28:36 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF122023.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Dec 21 01:54:25 2023  
Response via : Initial Calibration

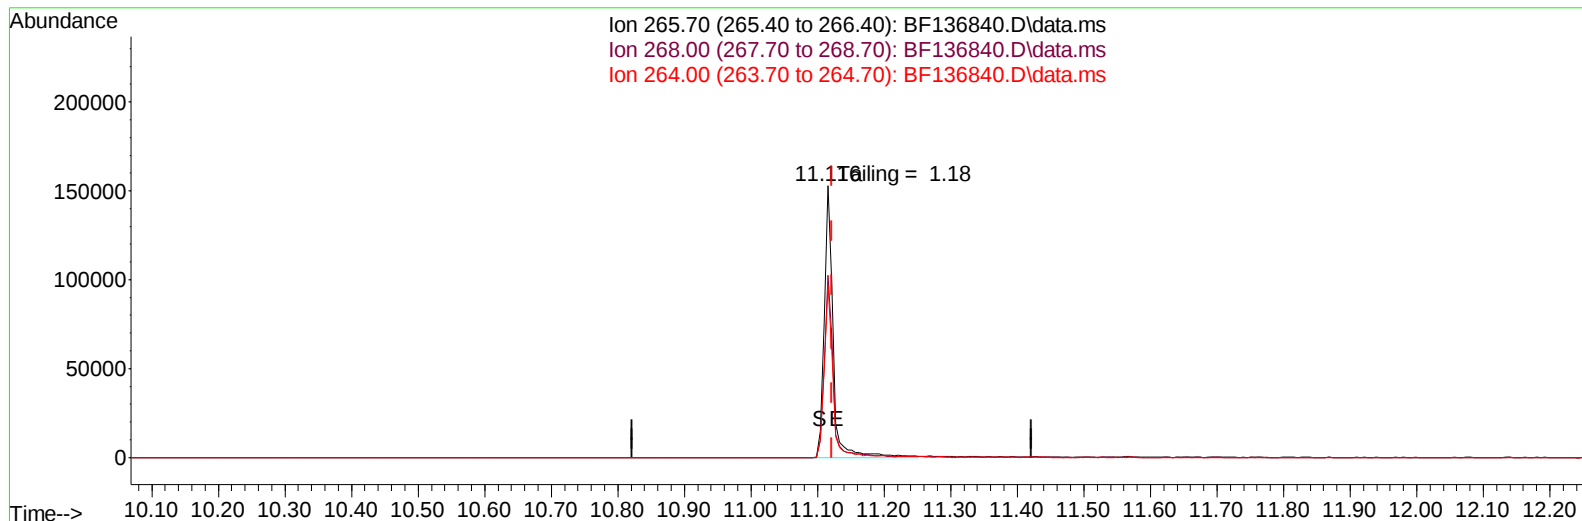




TIC: BF136840.D\data.ms

**(70) Pentachlorophenol (C)****11.116min (-0.006) 32036.35 ng****response 143228**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.70  | 67.07  |
| 264.00 | 61.20  | 63.65  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF122923\  
Data File : BF136840.D  
Acq On : 29 Dec 2023 21:23  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 01:28:36 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF122023.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Dec 21 01:54:25 2023  
Response via : Initial Calibration

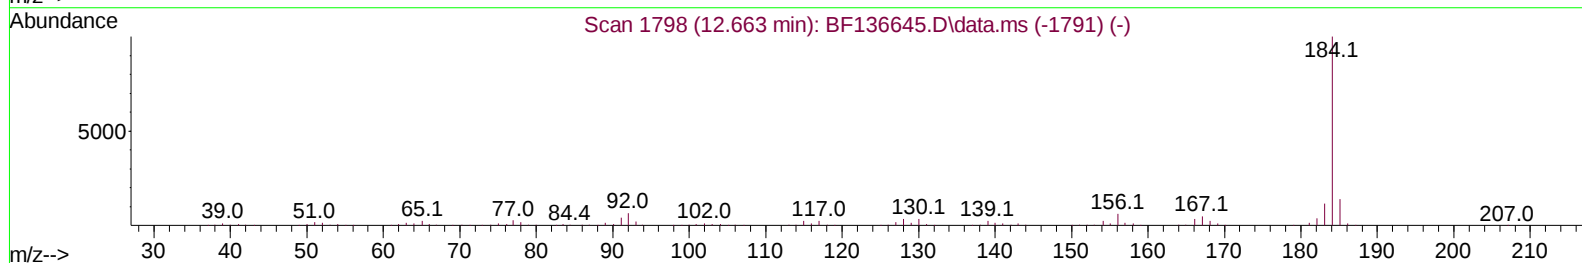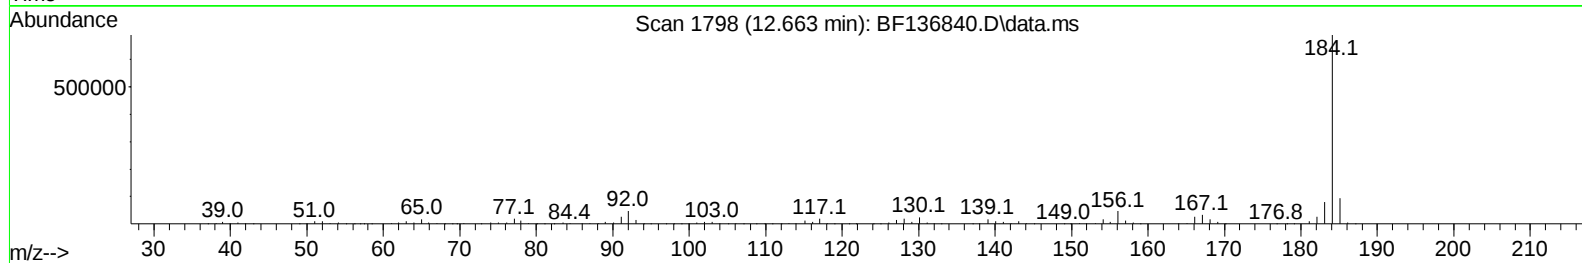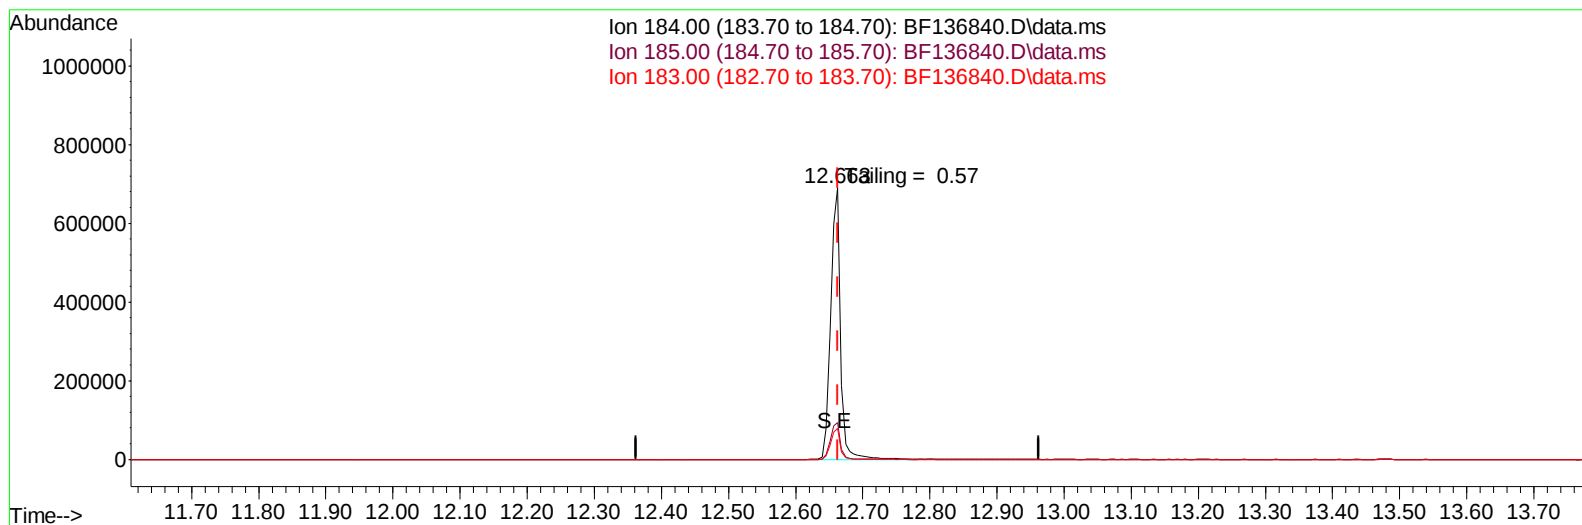

TIC: BF136840.D\data.ms

**(77) Benzidine****12.663min (+ 0.000) 0.00 ng****response 707835**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.00  | 13.68  |
| 183.00 | 11.60  | 11.50  |
| 0.00   | 0.00   | 0.00   |