

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
 Data File : BF136832.D
 Acq On : 29 Dec 2023 16:42
 Operator : CG\JU
 Sample : 05909-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GHL-SS-45

Quant Time: Dec 29 17:08:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.781	152	68789	20.000	ng	-0.01
21) Naphthalene-d8	8.057	136	259412	20.000	ng	-0.01
39) Acenaphthene-d10	9.816	164	134731	20.000	ng	-0.01
64) Phenanthrene-d10	11.304	188	253514	20.000	ng	-0.01
76) Chrysene-d12	13.963	240	143285	20.000	ng	0.00
86) Perylene-d12	15.439	264	136790	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.428	112	550596	124.887	ng	0.00
7) Phenol-d6	6.434	99	695102	121.677	ng	0.00
23) Nitrobenzene-d5	7.346	82	423908	83.619	ng	-0.01
42) 2,4,6-Tribromophenol	10.610	330	188398	118.731	ng	-0.01
45) 2-Fluorobiphenyl	9.140	172	781498	78.015	ng	-0.01
79) Terphenyl-d14	12.904	244	746411	72.798	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136832.D
Acq On : 29 Dec 2023 16:42
Operator : CG\JU
Sample : 05909-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GHL-SS-45

Quant Time: Dec 29 17:08:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration




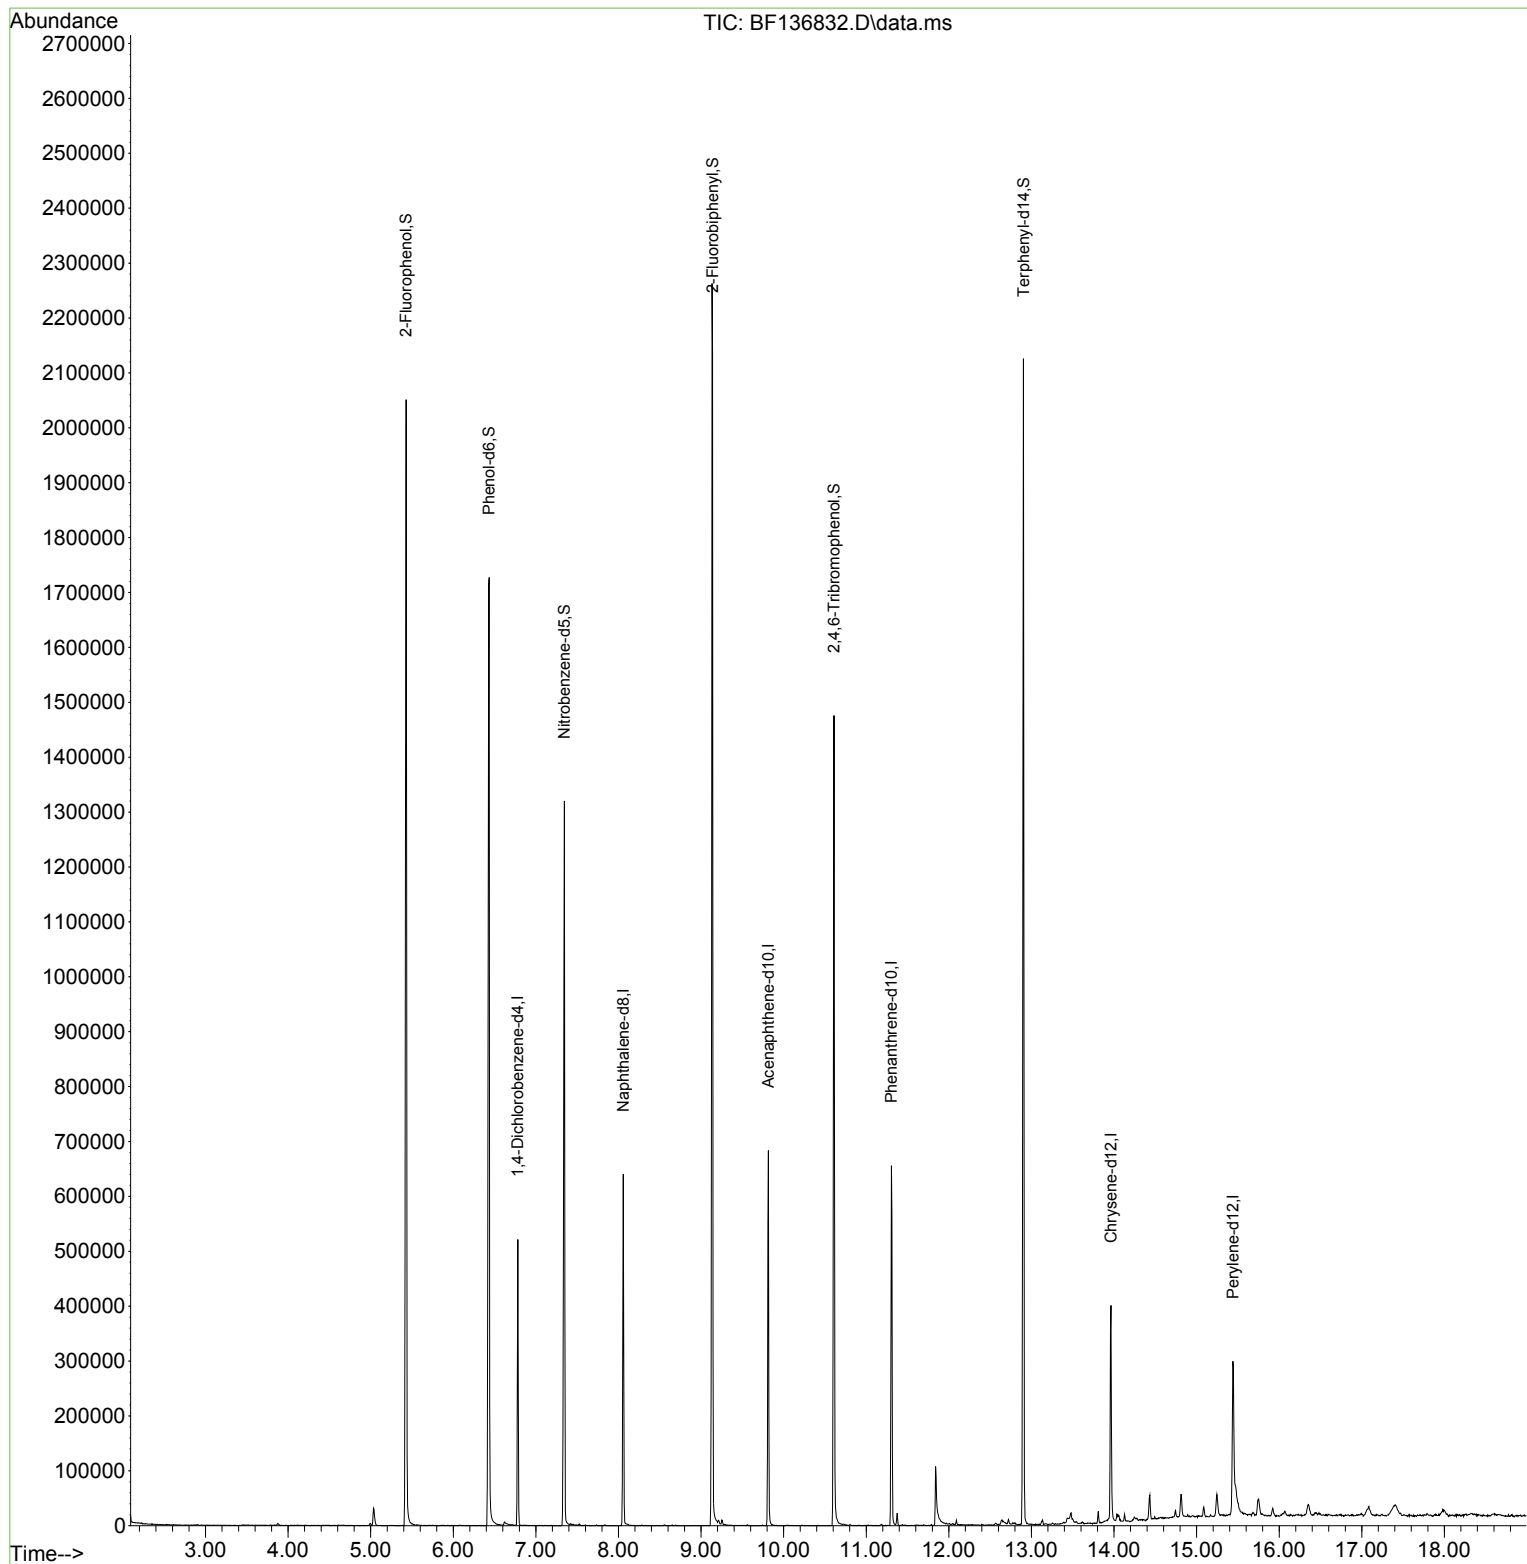


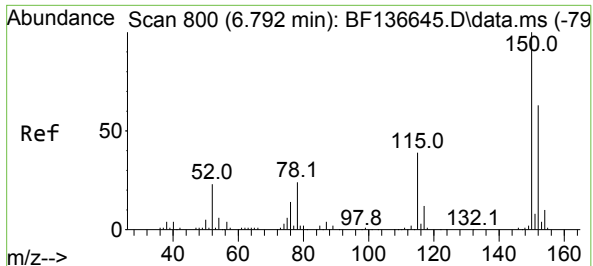

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.781 min Scan# 79
Delta R.T. -0.011 min
Lab File: BF136832.D
Acq: 29 Dec 2023 16:42




Instrument :
BNA_F
ClientSampleId :
GHL-SS-45


Tgt Ion:152 Resp: 68789
Ion Ratio Lower Upper
152 100
150 159.5 127.0 190.6
115 60.3 49.0 73.4

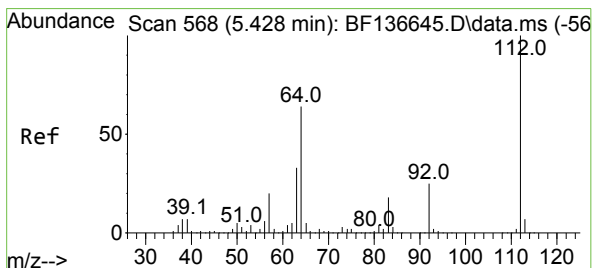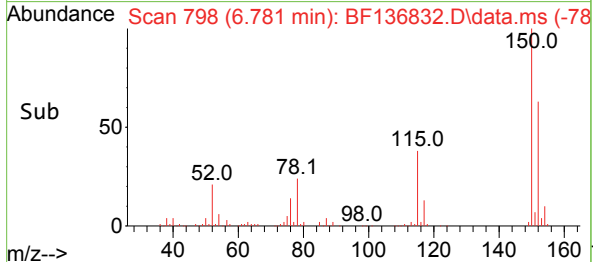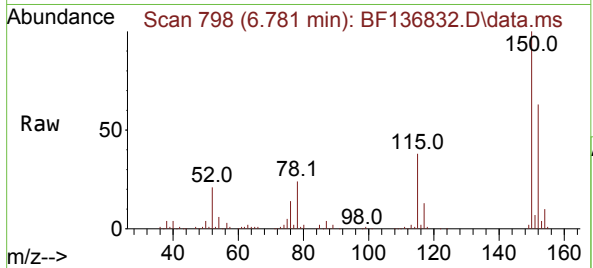

#5
2-Fluorophenol
Concen: 124.887 ng
RT: 5.428 min Scan# 568
Delta R.T. 0.000 min
Lab File: BF136832.D
Acq: 29 Dec 2023 16:42

Tgt Ion:112 Resp: 550596
Ion Ratio Lower Upper
112 100
64 62.2 51.1 76.7
63 31.3 26.1 39.1


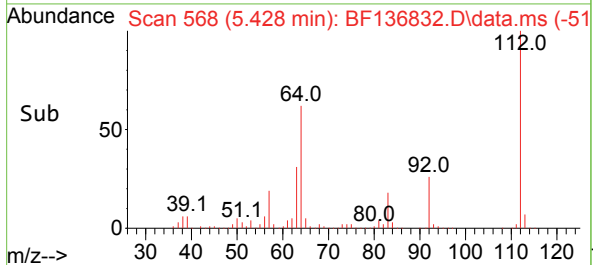

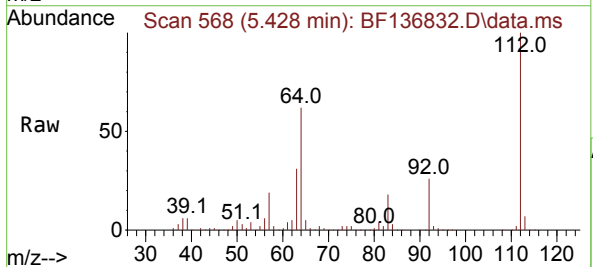


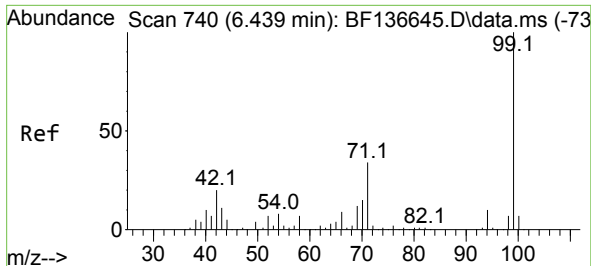

#7
Phenol-d6
Concen: 121.677 ng
RT: 6.434 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF136832.D
Acq: 29 Dec 2023 16:42




Instrument :
BNA_F
ClientSampleId :
GHL-SS-45


Tgt Ion: 99 Resp: 695102
Ion Ratio Lower Upper
99 100
42 18.1 16.1 24.1
71 31.9 27.4 41.2

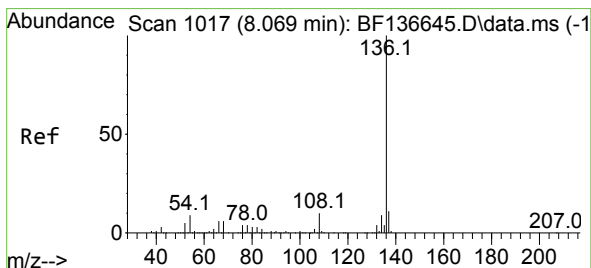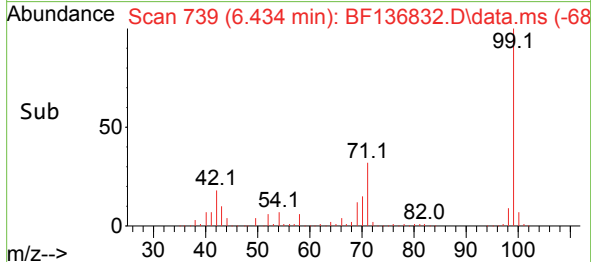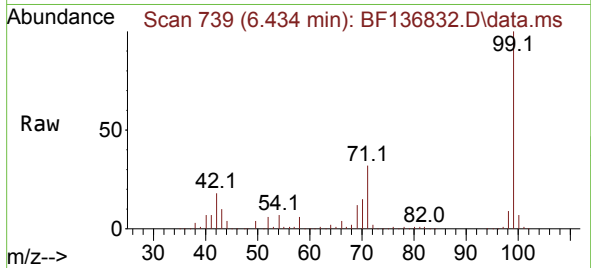

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.057 min Scan# 1015
Delta R.T. -0.011 min
Lab File: BF136832.D
Acq: 29 Dec 2023 16:42

Tgt Ion: 136 Resp: 259412
Ion Ratio Lower Upper
136 100
137 10.7 9.0 13.4
54 8.7 7.2 10.8
68 5.3 4.9 7.3

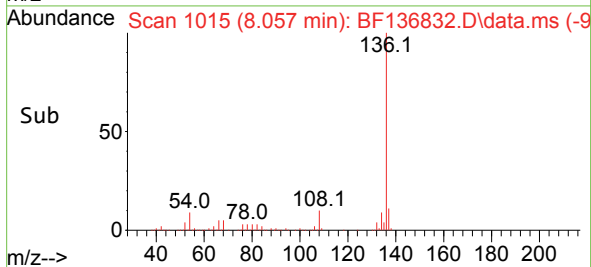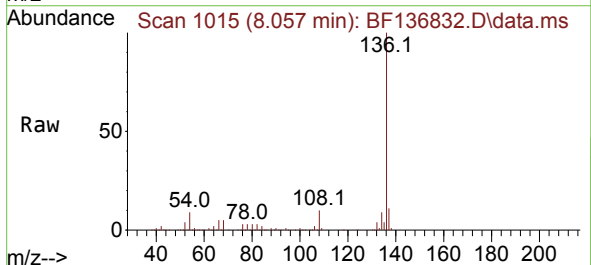




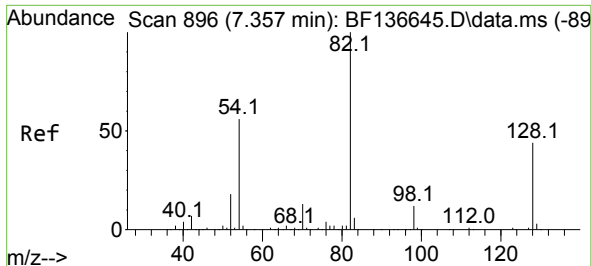


#23
 Nitrobenzene-d5
 Concen: 83.619 ng
 RT: 7.346 min Scan# 896
 Delta R.T. -0.011 min
 Lab File: BF136832.D
 Acq: 29 Dec 2023 16:42

Instrument :
 BNA_F
 ClientSampleId :
 GHL-SS-45

Tgt Ion: 82 Resp: 423908




Ion	Ratio	Lower	Upper
82	100		
128	46.1	35.3	52.9
54	53.2	44.5	66.7

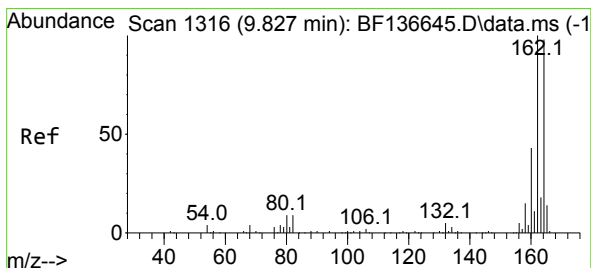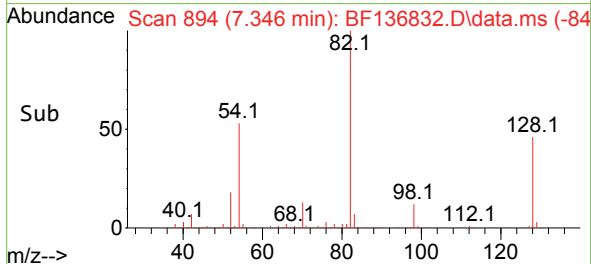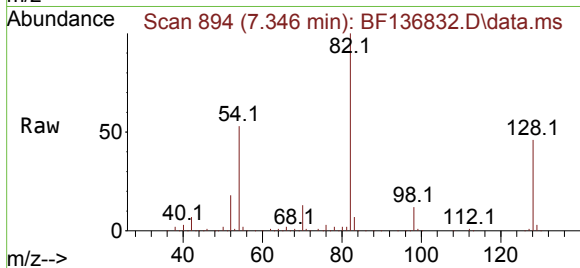


#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.816 min Scan# 1314
 Delta R.T. -0.011 min
 Lab File: BF136832.D
 Acq: 29 Dec 2023 16:42

Tgt Ion:164 Resp: 134731

Ion	Ratio	Lower	Upper
164	100		
162	101.7	81.6	122.4
160	45.2	34.9	52.3


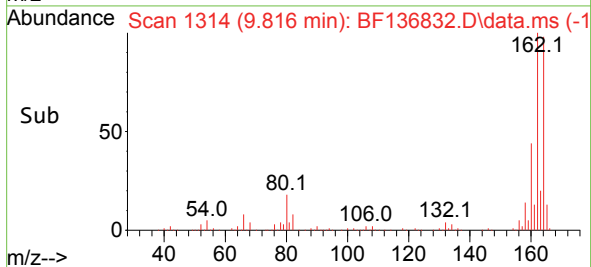

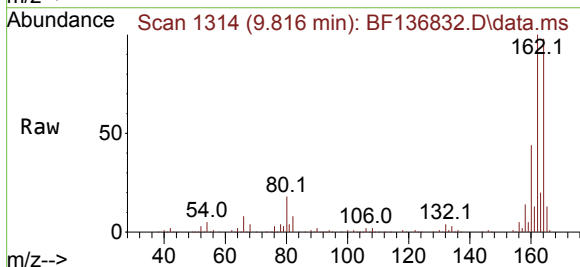


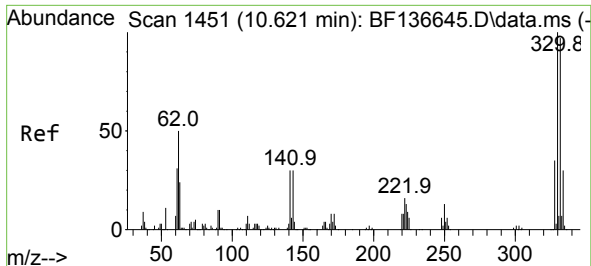

#42
2,4,6-Tribromophenol
Concen: 118.731 ng
RT: 10.610 min Scan# 1449
Delta R.T. -0.011 min
Lab File: BF136832.D
Acq: 29 Dec 2023 16:42




Instrument :
BNA_F
ClientSampleId :
GHL-SS-45


Tgt Ion: 330 Resp: 188398
Ion Ratio Lower Upper
330 100
332 96.9 77.4 116.0
141 28.1 23.4 35.2

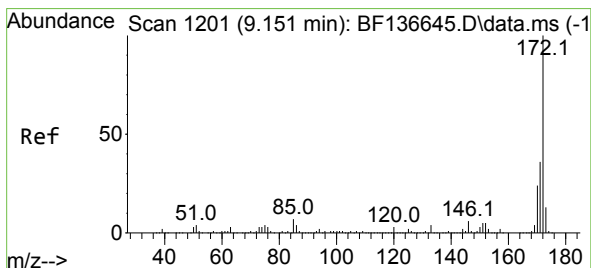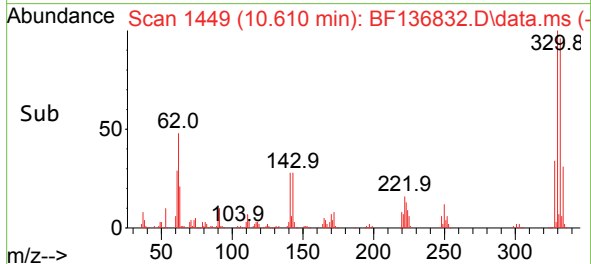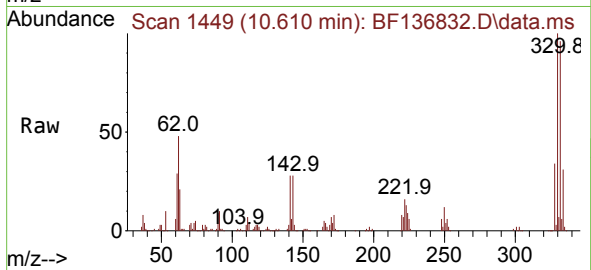

#45
2-Fluorobiphenyl
Concen: 78.015 ng
RT: 9.140 min Scan# 1199
Delta R.T. -0.011 min
Lab File: BF136832.D
Acq: 29 Dec 2023 16:42

Tgt Ion: 172 Resp: 781498
Ion Ratio Lower Upper
172 100
171 35.7 29.0 43.6
170 22.8 19.0 28.4


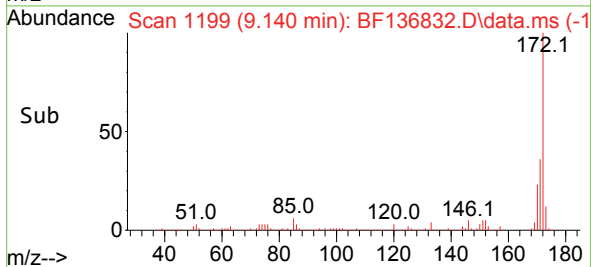

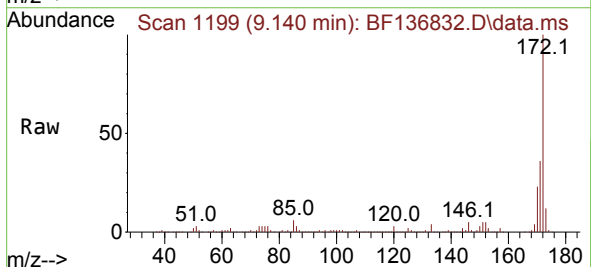


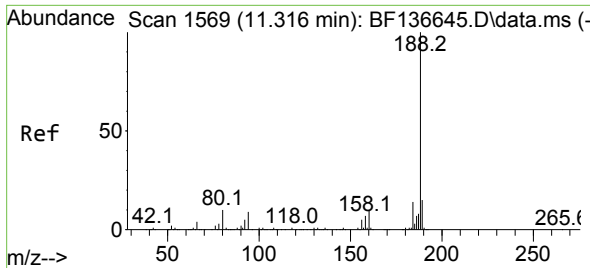

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.304 min Scan# 11
Delta R.T. -0.011 min
Lab File: BF136832.D
Acq: 29 Dec 2023 16:42




Instrument :
BNA_F
ClientSampleId :
GHL-SS-45


Tgt Ion:188 Resp: 253514
Ion Ratio Lower Upper
188 100
94 9.7 7.5 11.3
80 10.6 8.1 12.1

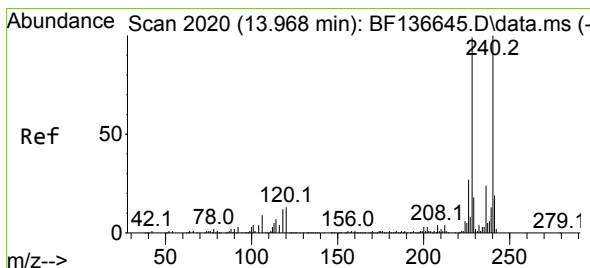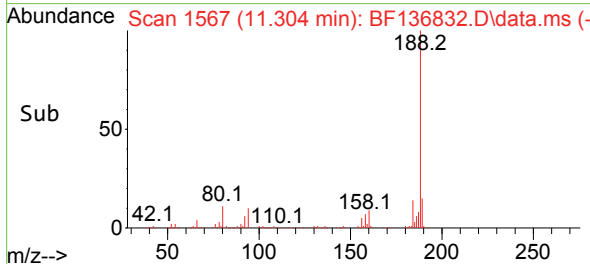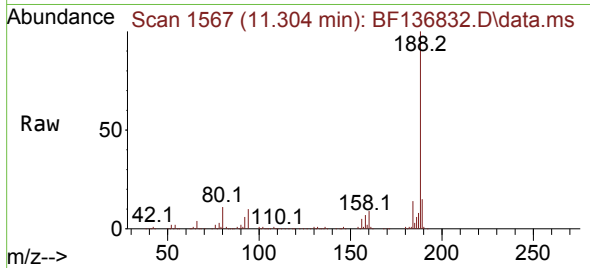

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.963 min Scan# 2019
Delta R.T. -0.006 min
Lab File: BF136832.D
Acq: 29 Dec 2023 16:42


Tgt Ion:240 Resp: 143285
Ion Ratio Lower Upper
240 100
120 10.9 10.3 15.5
236 24.1 19.4 29.2

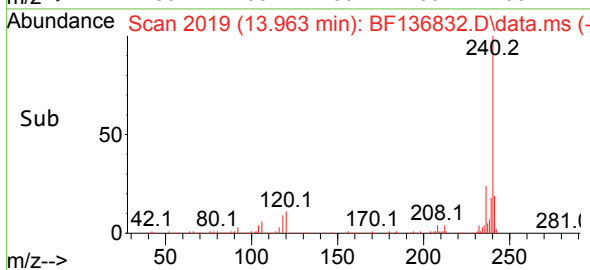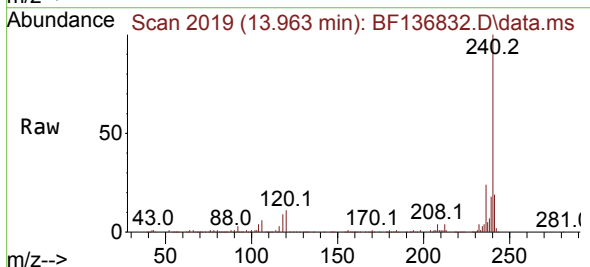



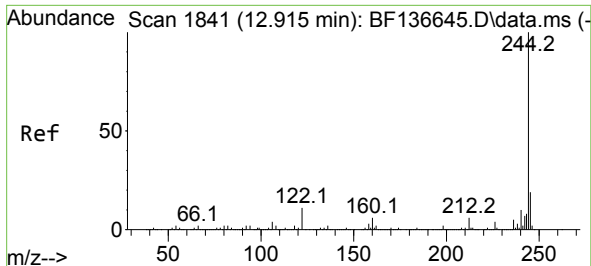


#79
 Terphenyl-d14
 Concen: 72.798 ng
 RT: 12.904 min Scan# 1839
 Delta R.T. -0.011 min
 Lab File: BF136832.D
 Acq: 29 Dec 2023 16:42

Instrument :
 BNA_F
 ClientSampleId :
 GHL-SS-45

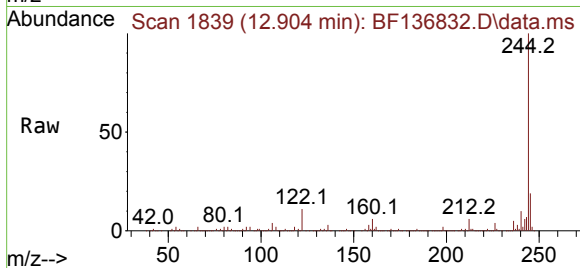

Tgt Ion:244 Resp: 746411
 Ion Ratio Lower Upper
 244 100
 212 6.3 5.0 7.4
 122 11.1 9.0 13.4

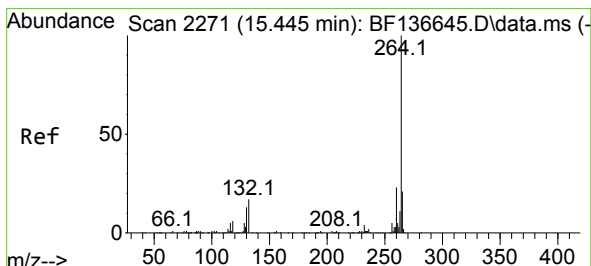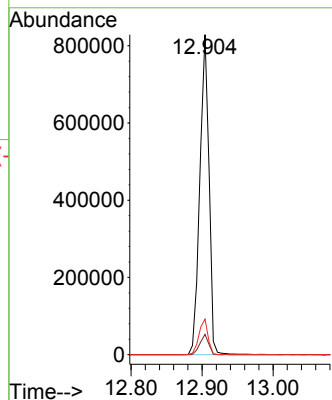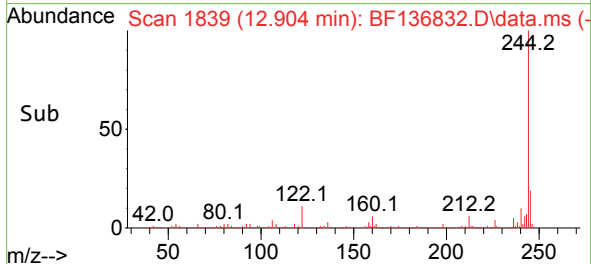

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.439 min Scan# 2270
 Delta R.T. -0.006 min
 Lab File: BF136832.D
 Acq: 29 Dec 2023 16:42

Tgt Ion:264 Resp: 136790
 Ion Ratio Lower Upper
 264 100
 260 22.2 18.3 27.5
 265 21.8 17.0 25.6

