

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
 Data File : BF136856.D
 Acq On : 30 Dec 2023 06:17
 Operator : CG\JU
 Sample : 05897-11
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GHL-SS-40

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136856.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	495	499	506	rVB	23922	27963	1.61%	0.263%
2	5.422	563	567	586	rBV	1579599	1394195	80.03%	13.098%
3	6.428	733	738	754	rBV	1483263	1436973	82.49%	13.500%
4	6.781	794	798	801	rBV	489747	401439	23.04%	3.771%
5	7.339	888	893	896	rBV	962540	935214	53.68%	8.786%
6	8.057	1011	1015	1018	rBV	630970	526336	30.21%	4.945%
7	9.133	1193	1198	1201	rBV	2051626	1742063	100.00%	16.366%
8	9.816	1310	1314	1325	rVB	633001	594555	34.13%	5.586%
9	10.604	1445	1448	1465	rVB	491528	434685	24.95%	4.084%
10	11.304	1563	1567	1571	rBV	725875	611002	35.07%	5.740%
11	12.904	1834	1839	1842	rBV	1758683	1582722	90.85%	14.869%
12	13.110	1870	1874	1876	rBV	24346	20667	1.19%	0.194%
13	13.133	1876	1878	1882	rVB	29913	24129	1.39%	0.227%
14	13.963	2015	2019	2027	rVB	415549	401633	23.06%	3.773%
15	14.815	2161	2164	2170	rVB	25628	27478	1.58%	0.258%
16	15.086	2206	2210	2216	rVB	22977	26067	1.50%	0.245%
17	15.439	2265	2270	2286	rBV	269964	396235	22.75%	3.722%
18	15.921	2347	2352	2357	rBV3	18830	26271	1.51%	0.247%
19	17.098	2548	2552	2558	rVB5	18730	34725	1.99%	0.326%




Sum of corrected areas: 10644352

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136856.D
Acq On : 30 Dec 2023 06:17
Operator : CG\JU
Sample : 05897-11
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GHL-SS-40

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

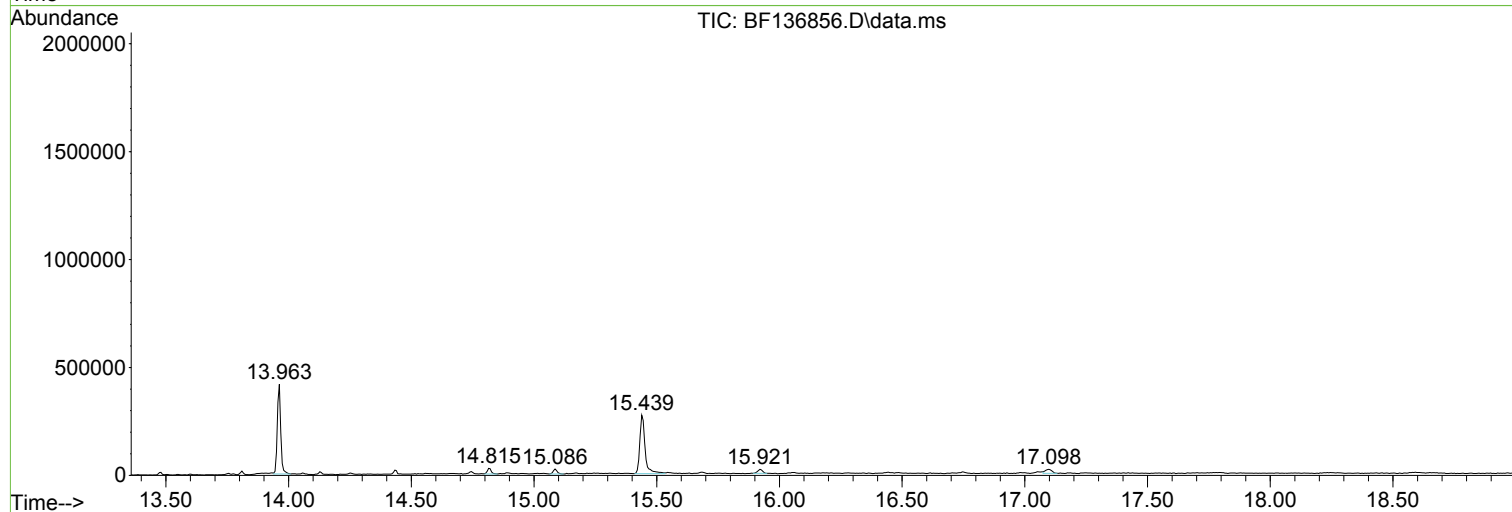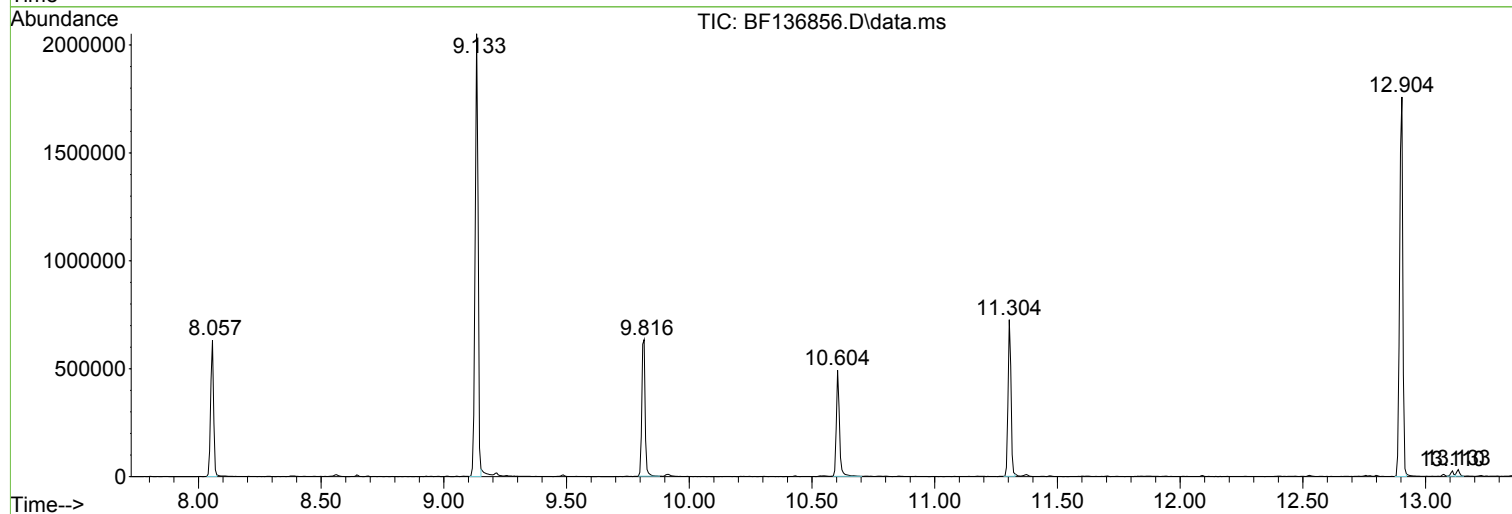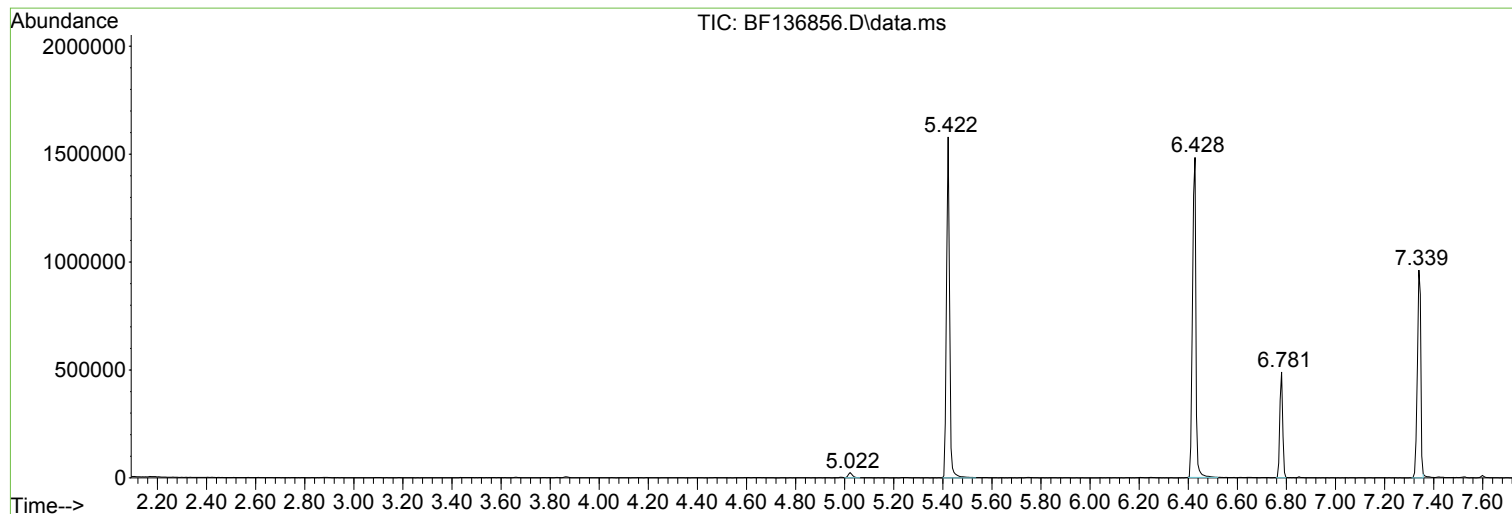

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136856.D
Acq On : 30 Dec 2023 06:17
Operator : CG\JU
Sample : 05897-11
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GHL-SS-40

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136856.D
Acq On : 30 Dec 2023 06:17
Operator : CG\JU
Sample : 05897-11
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GHL-SS-40

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------