

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
 Data File : BF136860.D
 Acq On : 30 Dec 2023 08:23
 Operator : CG\JU
 Sample : 05897-16
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GHL-SS-20

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136860.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	494	498	503	rBV	20418	21332	1.70%	0.242%
2	5.422	563	567	580	rBV	1141911	1101830	87.89%	12.513%
3	6.422	733	737	755	rBV	1290794	1176593	93.85%	13.362%
4	6.781	794	798	801	rBV	502209	411489	32.82%	4.673%
5	7.340	889	893	896	rBV	869283	747175	59.60%	8.485%
6	8.057	1011	1015	1018	rBV	666487	541968	43.23%	6.155%
7	9.134	1194	1198	1201	rBV	1604215	1253690	100.00%	14.237%
8	9.816	1310	1314	1327	rBV	650886	607454	48.45%	6.898%
9	10.604	1445	1448	1462	rBV	338146	303242	24.19%	3.444%
10	11.304	1563	1567	1575	rBV	730526	609771	48.64%	6.925%
11	12.904	1834	1839	1842	rBV	1244027	1198304	95.58%	13.608%
12	13.480	1933	1937	1940	rBV	16668	16014	1.28%	0.182%
13	13.810	1989	1993	1999	rVB	18828	17323	1.38%	0.197%
14	13.963	2015	2019	2025	rVB	386611	374878	29.90%	4.257%
15	14.439	2096	2100	2103	rBV	17852	17837	1.42%	0.203%
16	14.745	2147	2152	2155	rBV2	14980	17185	1.37%	0.195%
17	15.439	2266	2270	2279	rBV	279568	389693	31.08%	4.425%




Sum of corrected areas: 8805778

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136860.D
Acq On : 30 Dec 2023 08:23
Operator : CG\JU
Sample : 05897-16
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GHL-SS-20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

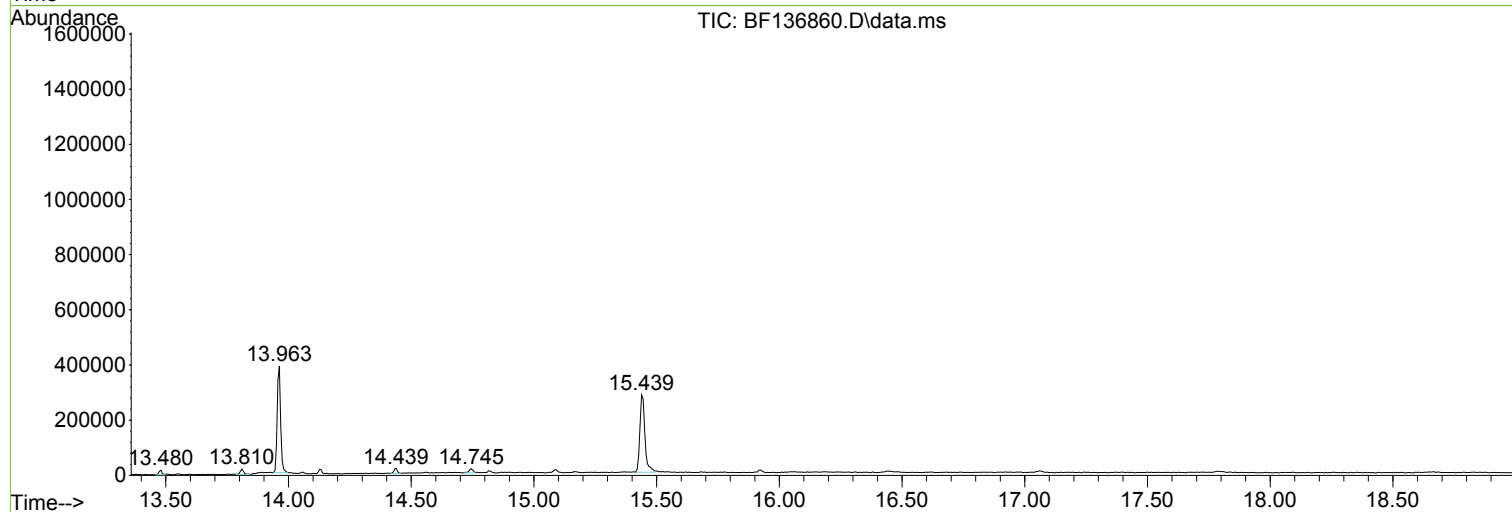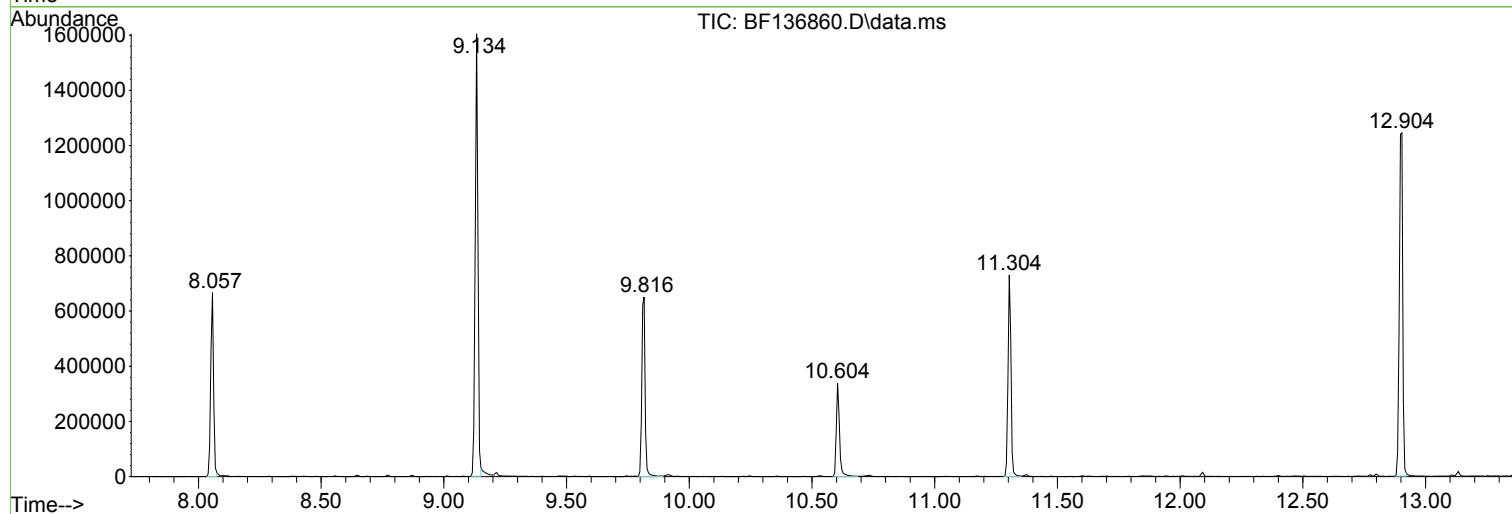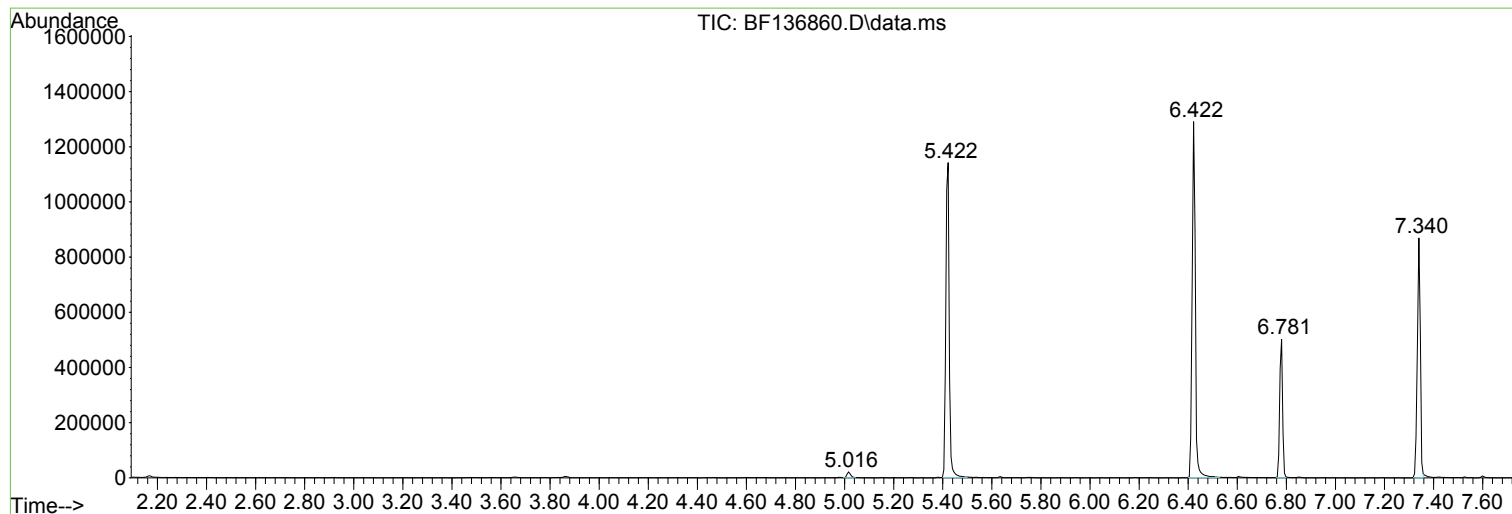

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136860.D
Acq On : 30 Dec 2023 08:23
Operator : CG\JU
Sample : 05897-16
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GHL-SS-20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136860.D
Acq On : 30 Dec 2023 08:23
Operator : CG\JU
Sample : 05897-16
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GHL-SS-20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------