


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136817.D
Acq On : 29 Dec 2023 09:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

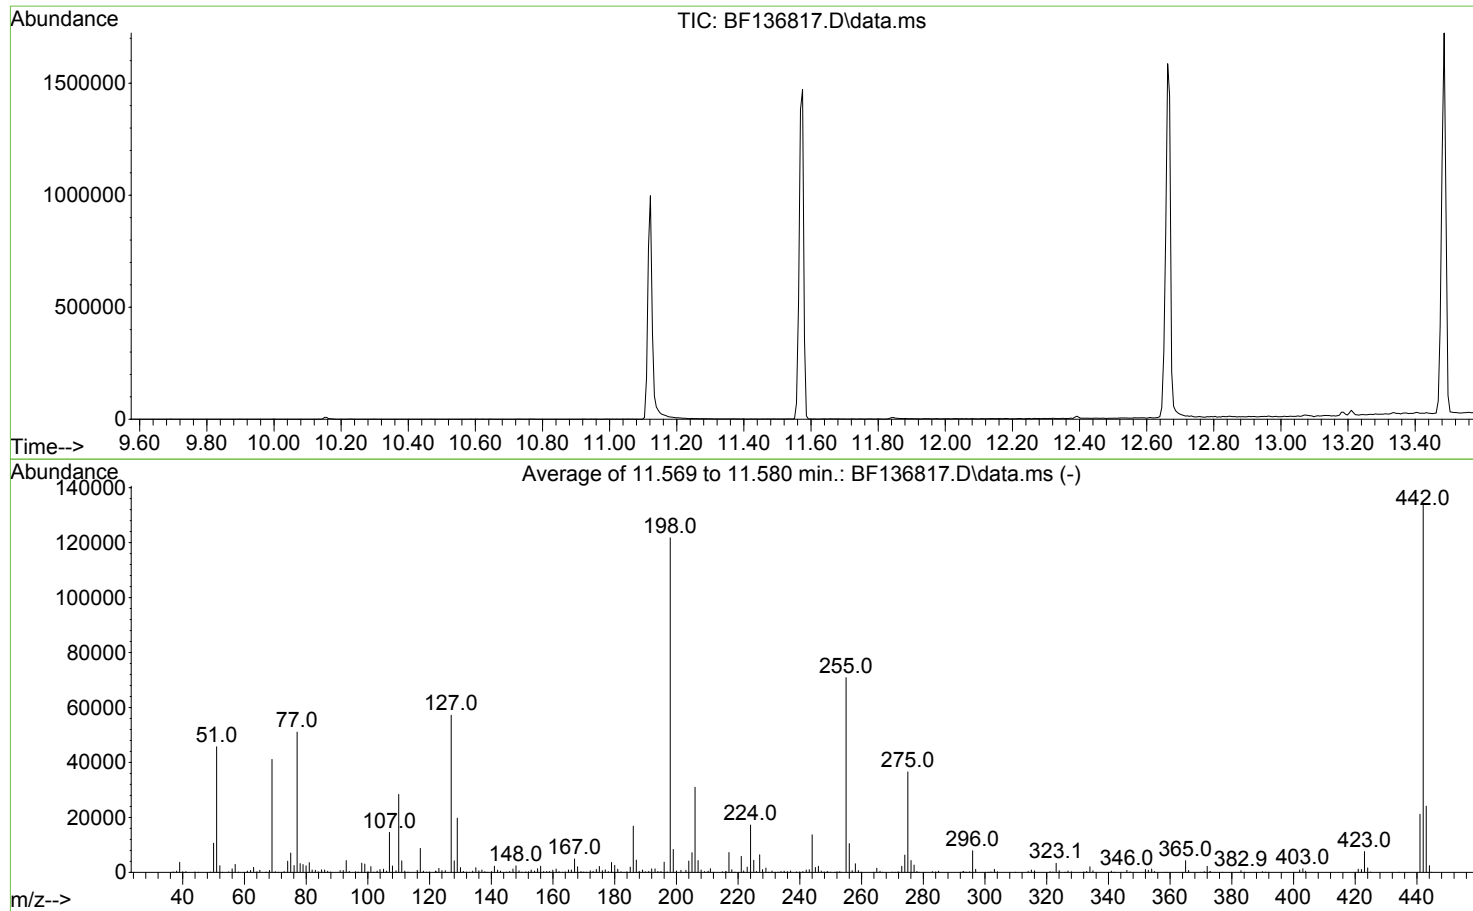

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	45687	PASS
68	69	0.00	2	1.8	733	PASS
69	198	0.00	100	33.8	41123	PASS
70	69	0.00	2	0.6	262	PASS
127	198	10	80	47.0	57178	PASS
197	198	0.00	2	0.1	157	PASS
198	198	100	100	100.0	121768	PASS
199	198	5	9	6.8	8320	PASS
275	198	10	60	30.0	36557	PASS
365	198	1	100	3.5	4228	PASS
441	198	0.01	100	17.4	21127	PASS
442	442	50	100	100.0	133859	PASS
443	442	15	24	18.0	24087	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/29/2023	BNA_F	<u>BF136817.D</u>
Compound Name	Response	Retention Time
DDT	313151	13.486
DDD	6811	13.21
DDE	465	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7276	320427	2.27

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136817.D
Acq On : 29 Dec 2023 09:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 29 10:08:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

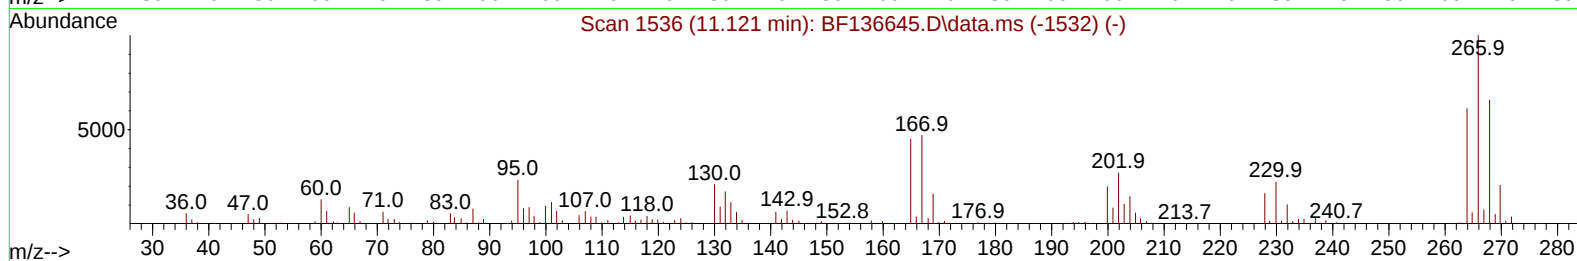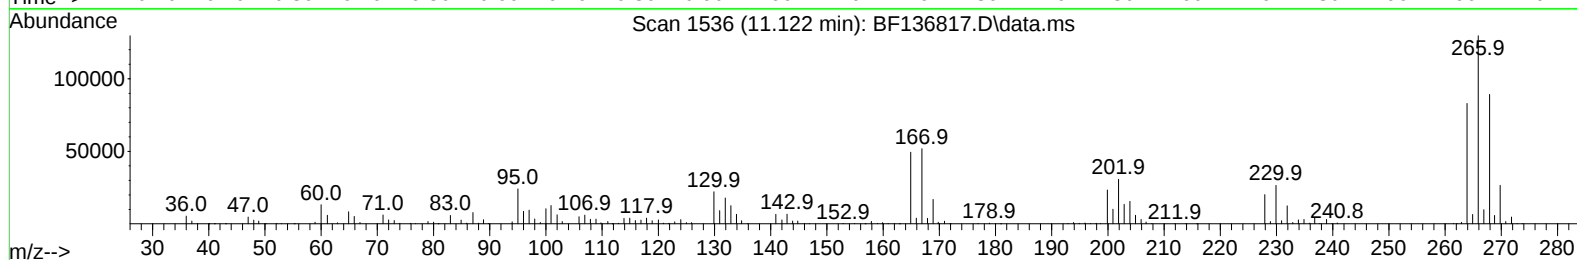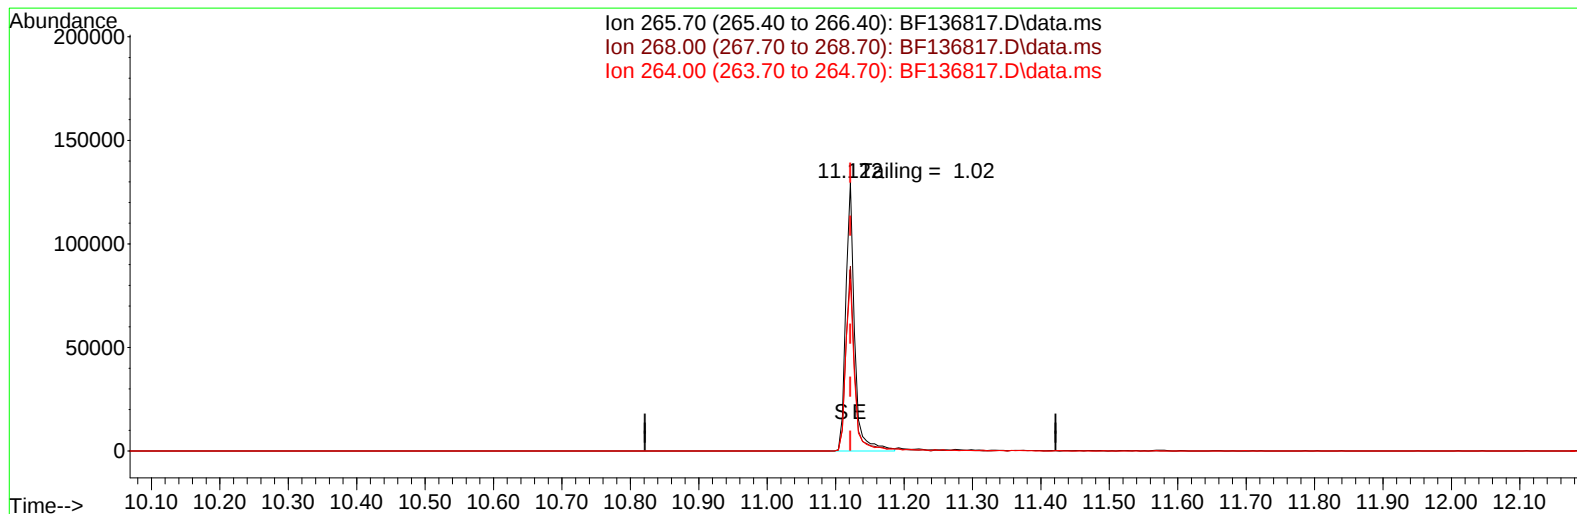

TIC: BF136817.D\data.ms

(70) Pentachlorophenol (C)

11.122min (+ 0.000) 39770.90 ng




response 116550

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	68.78
264.00	61.20	64.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136817.D
Acq On : 29 Dec 2023 09:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 29 10:08:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

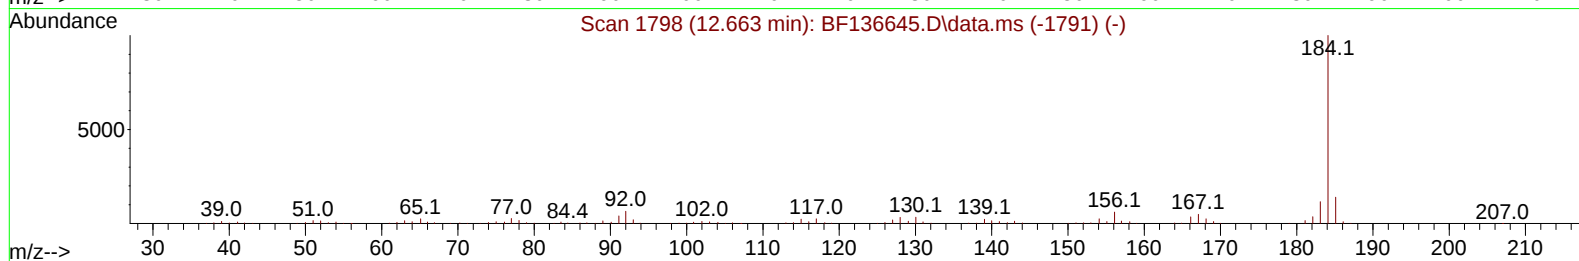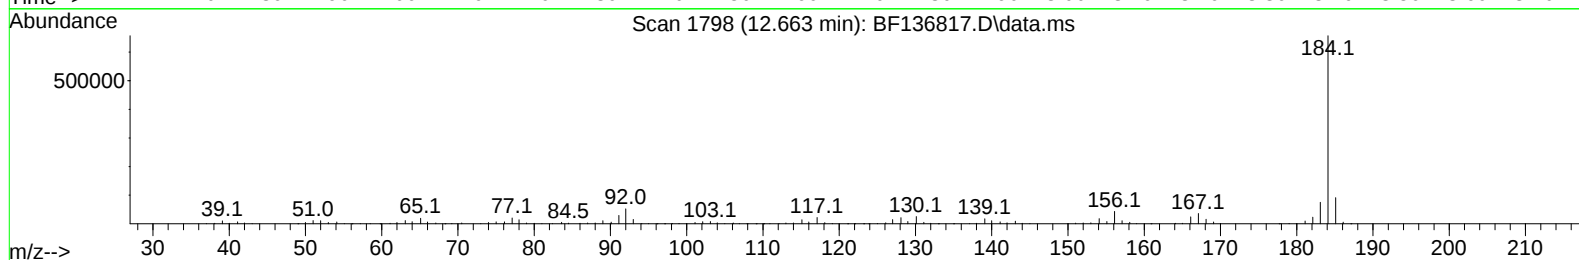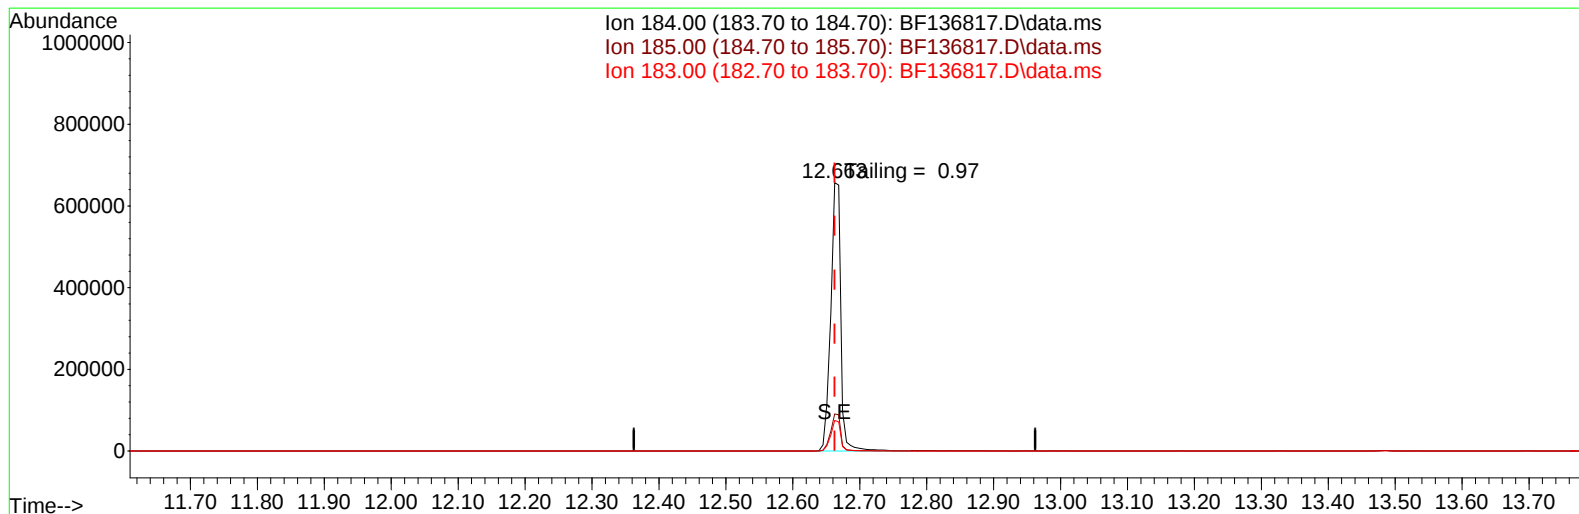

TIC: BF136817.D\data.ms

(77) Benzidine

12.663min (+ 0.000) 374275.79 ng

response 684219

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.86
183.00	11.60	11.42
0.00	0.00	0.00