
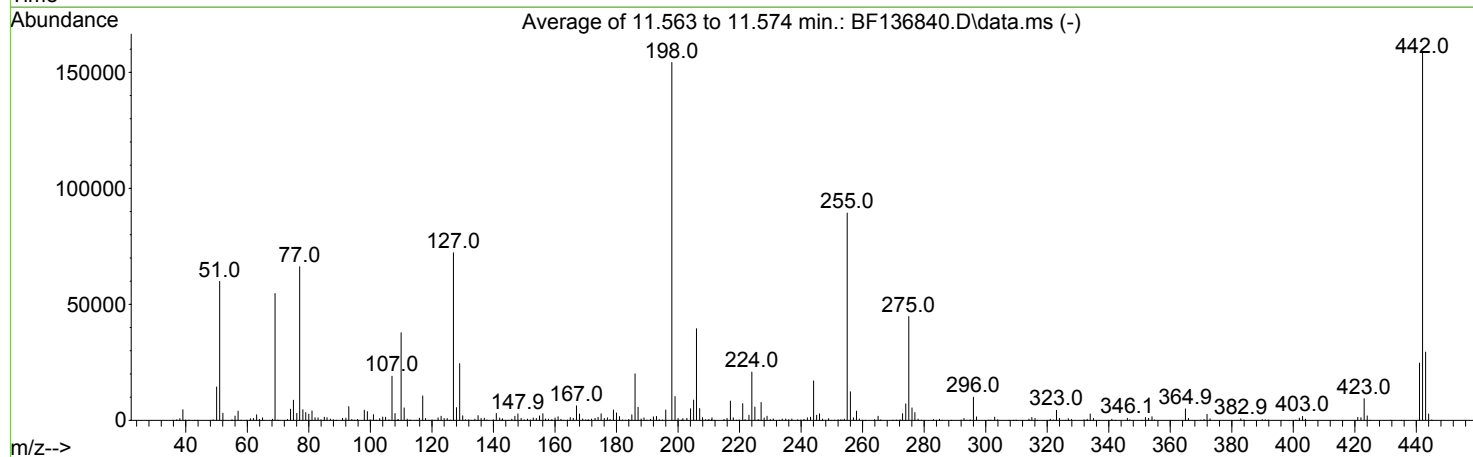


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136840.D
Acq On : 29 Dec 2023 21:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

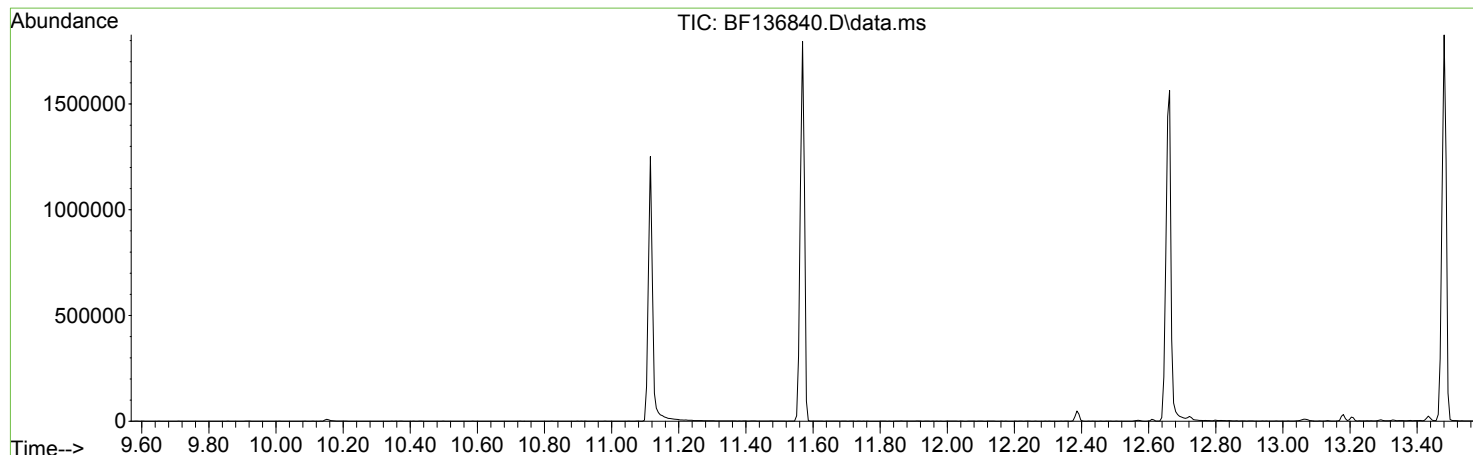

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	59915	PASS
68	69	0.00	2	0.9	514	PASS
69	198	0.00	100	35.4	54675	PASS
70	69	0.00	2	0.4	220	PASS
127	198	10	80	46.9	72299	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	154293	PASS
199	198	5	9	6.7	10295	PASS
275	198	10	60	29.0	44747	PASS
365	198	1	100	3.2	4938	PASS
441	198	0.01	100	16.0	24716	PASS
442	442	50	100	100.0	158581	PASS
443	442	15	24	18.6	29449	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/29/2023	BNA_F	<u>BF136840.D</u>
Compound Name	Response	Retention Time
DDT	344489	13.48
DDD	9716	13.18
DDE	321	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10037	354526	2.83

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136840.D
Acq On : 29 Dec 2023 21:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 30 01:28:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

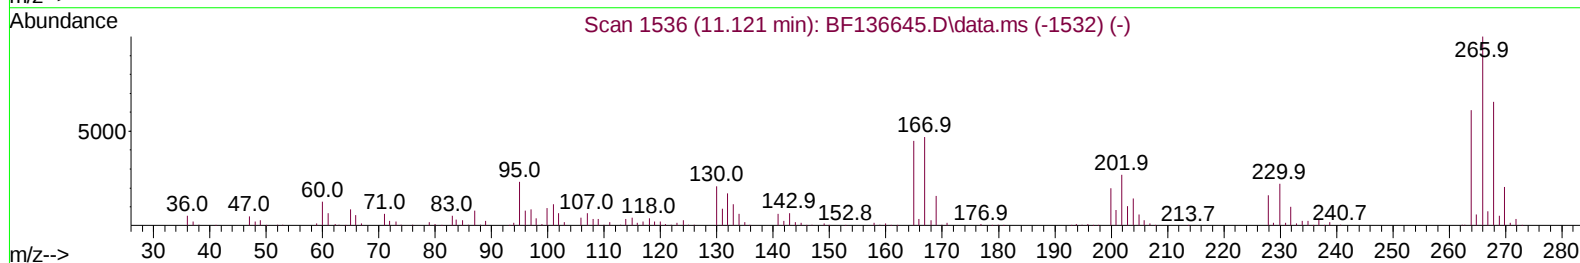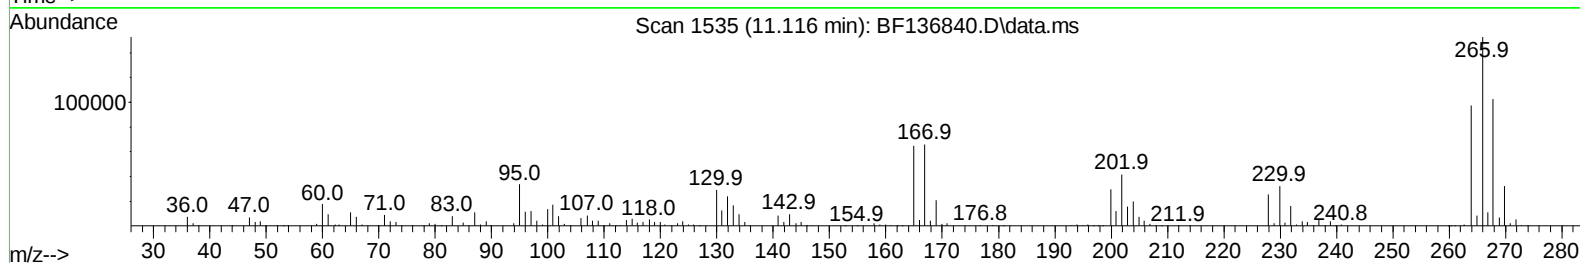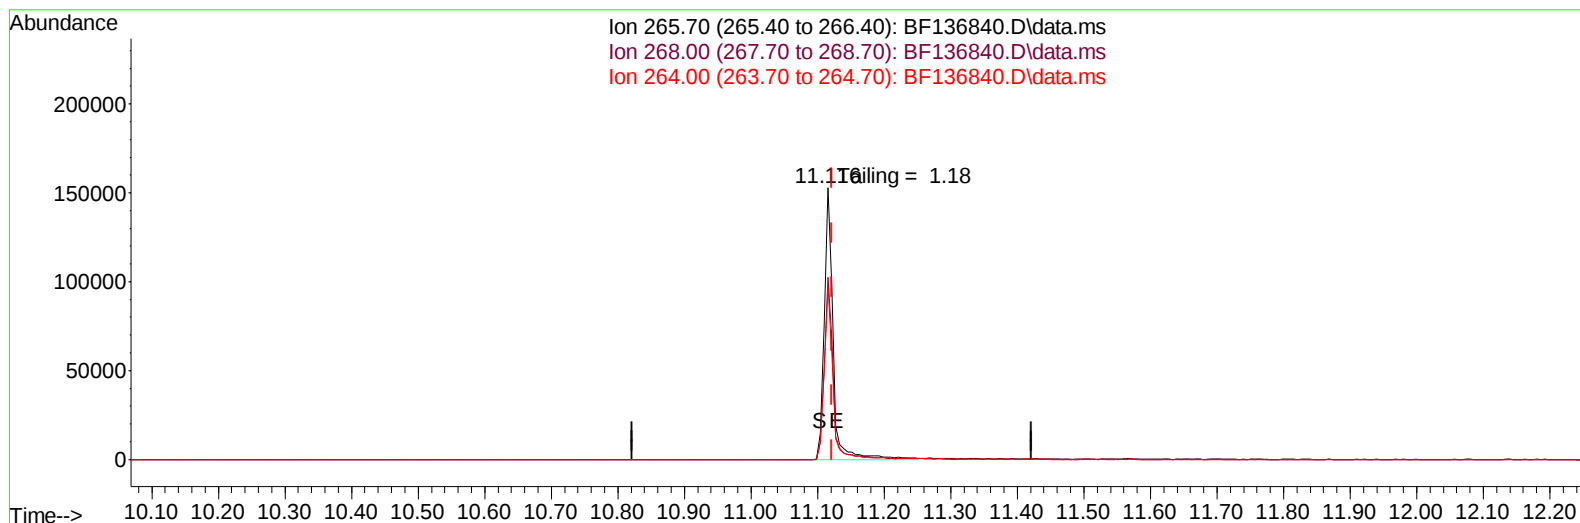

TIC: BF136840.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.006) 32036.35 ng




response 143228

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	67.07
264.00	61.20	63.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122923\
Data File : BF136840.D
Acq On : 29 Dec 2023 21:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 30 01:28:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

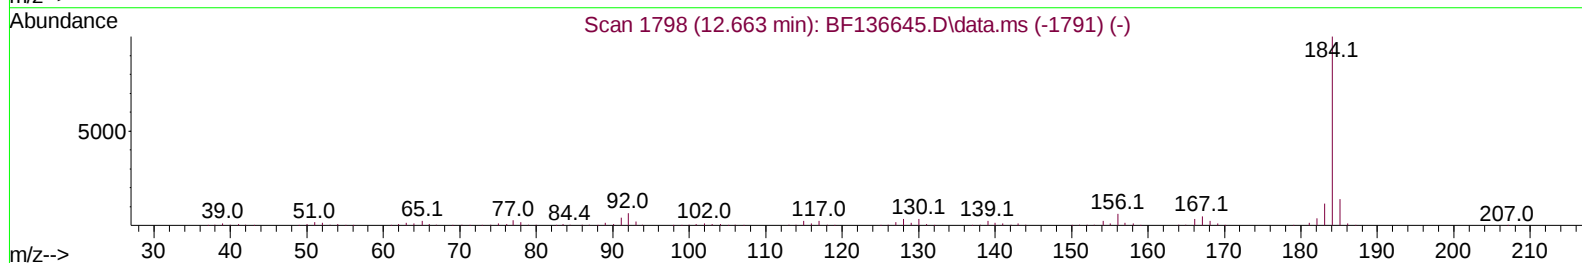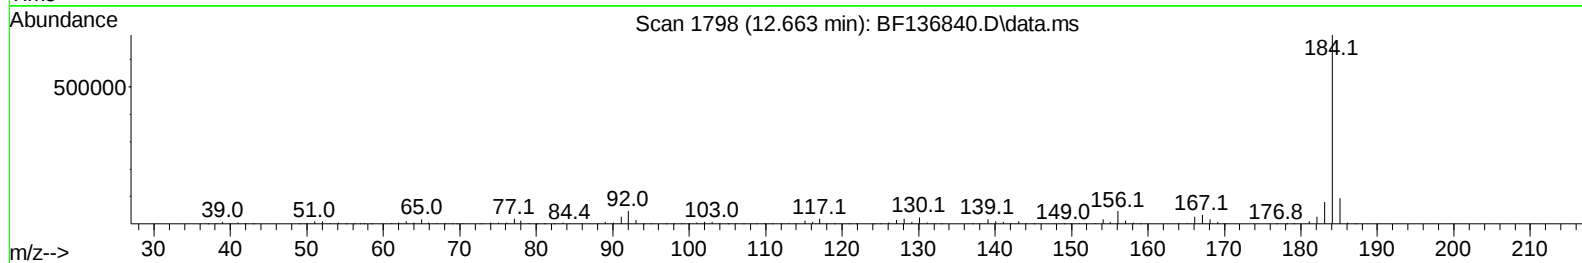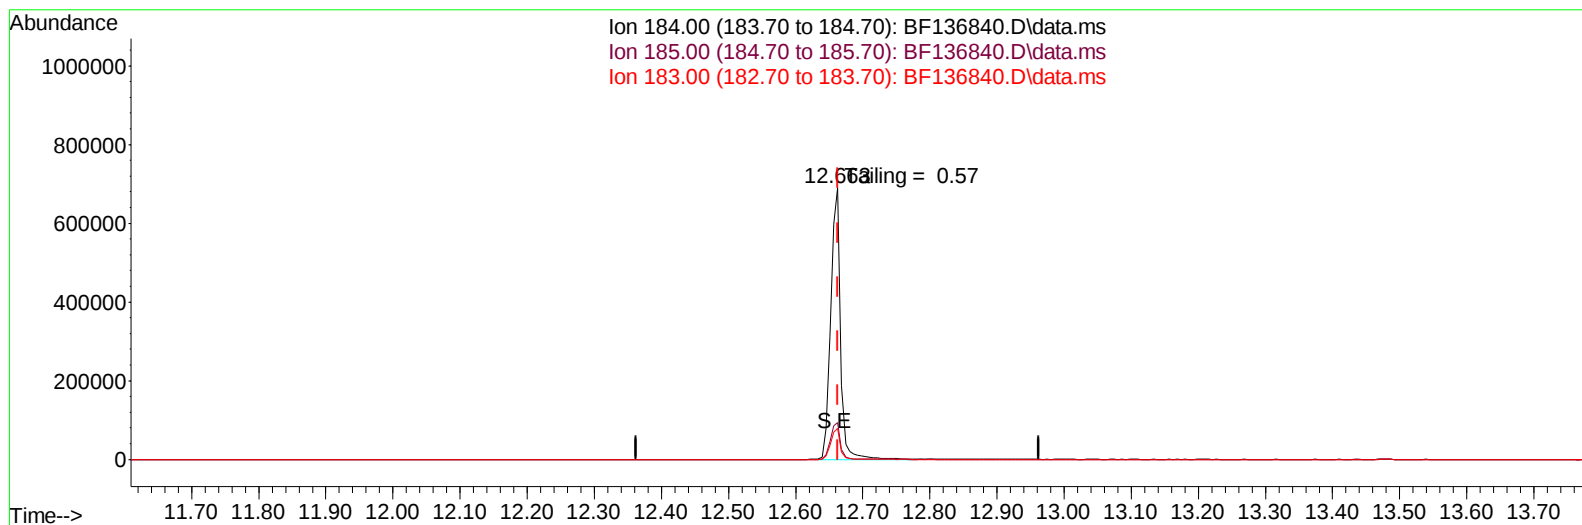

TIC: BF136840.D\data.ms

(77) Benzidine

12.663min (+ 0.000) 0.00 ng

response 707835

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.68
183.00	11.60	11.50
0.00	0.00	0.00