


Data Path : Z:\HPCHEM1\BNA F\DATA\BF123015\
 Data File : BF084163.D
 Acq On : 30 Dec 2015 23:04
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 31 04:29:55 2015

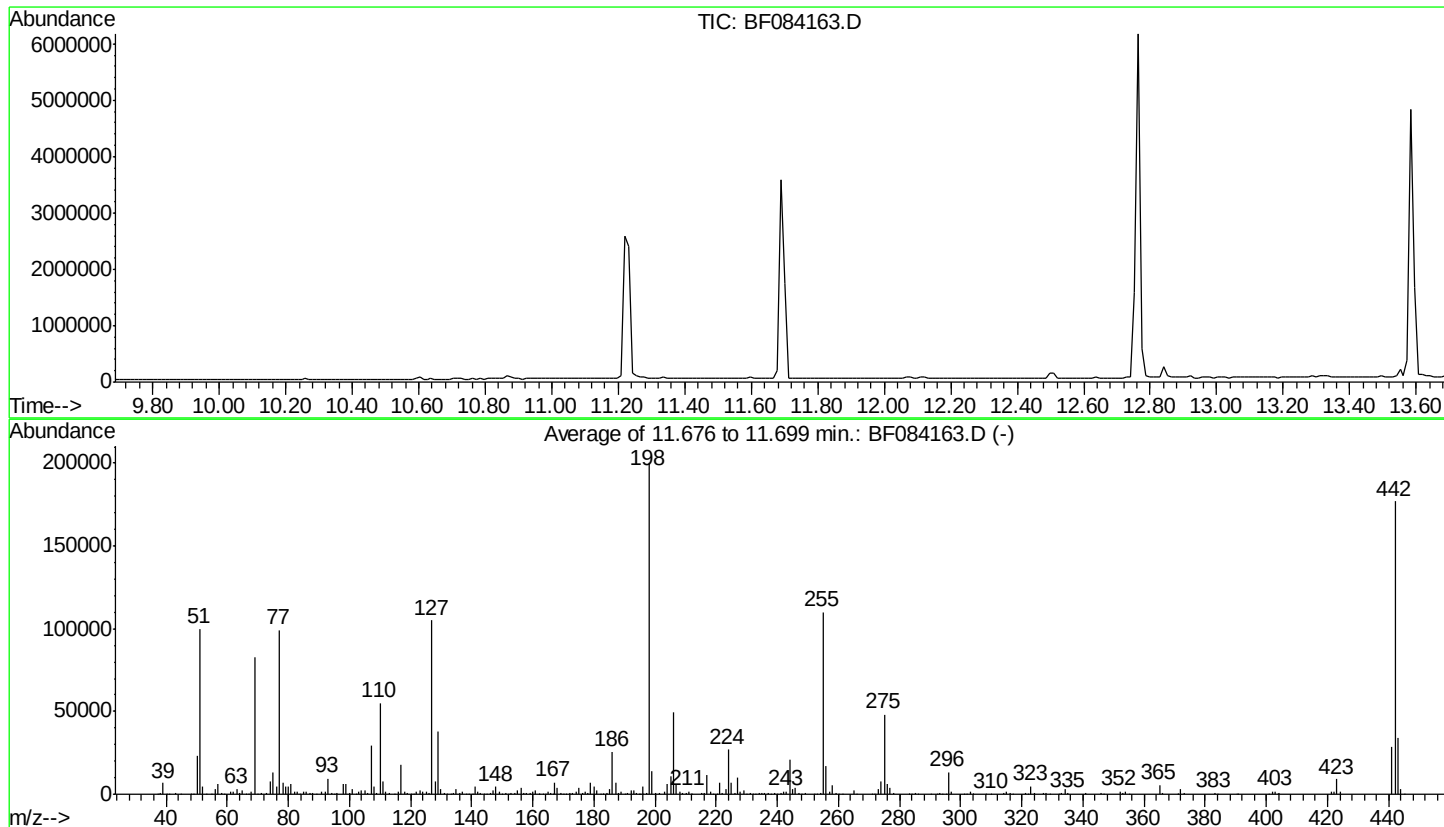

AutoFind: Scans 839, 840, 841; Background Corrected with Scan 836

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.9	99921	PASS
68	69	0.00	2	1.9	1595	PASS
69	198	0.00	100	41.4	82919	PASS
70	69	0.00	2	0.4	323	PASS
127	198	10	80	52.4	105031	PASS
197	198	0.00	2	0.5	1059	PASS
198	198	100	100	100.0	200374	PASS
199	198	5	9	6.9	13738	PASS
275	198	10	60	24.1	48256	PASS
365	198	1	100	2.9	5731	PASS
441	442	0.01	24	16.1	28562	PASS
442	198	50	100	88.4	177061	PASS
443	442	15	24	19.1	33832	PASS