


Data Path : Z:\HPCHEM1\BNA F\DATA\BF123015\
Data File : BF084172.D
Acq On : 31 Dec 2015 3:12
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123015.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 31 04:29:55 2015

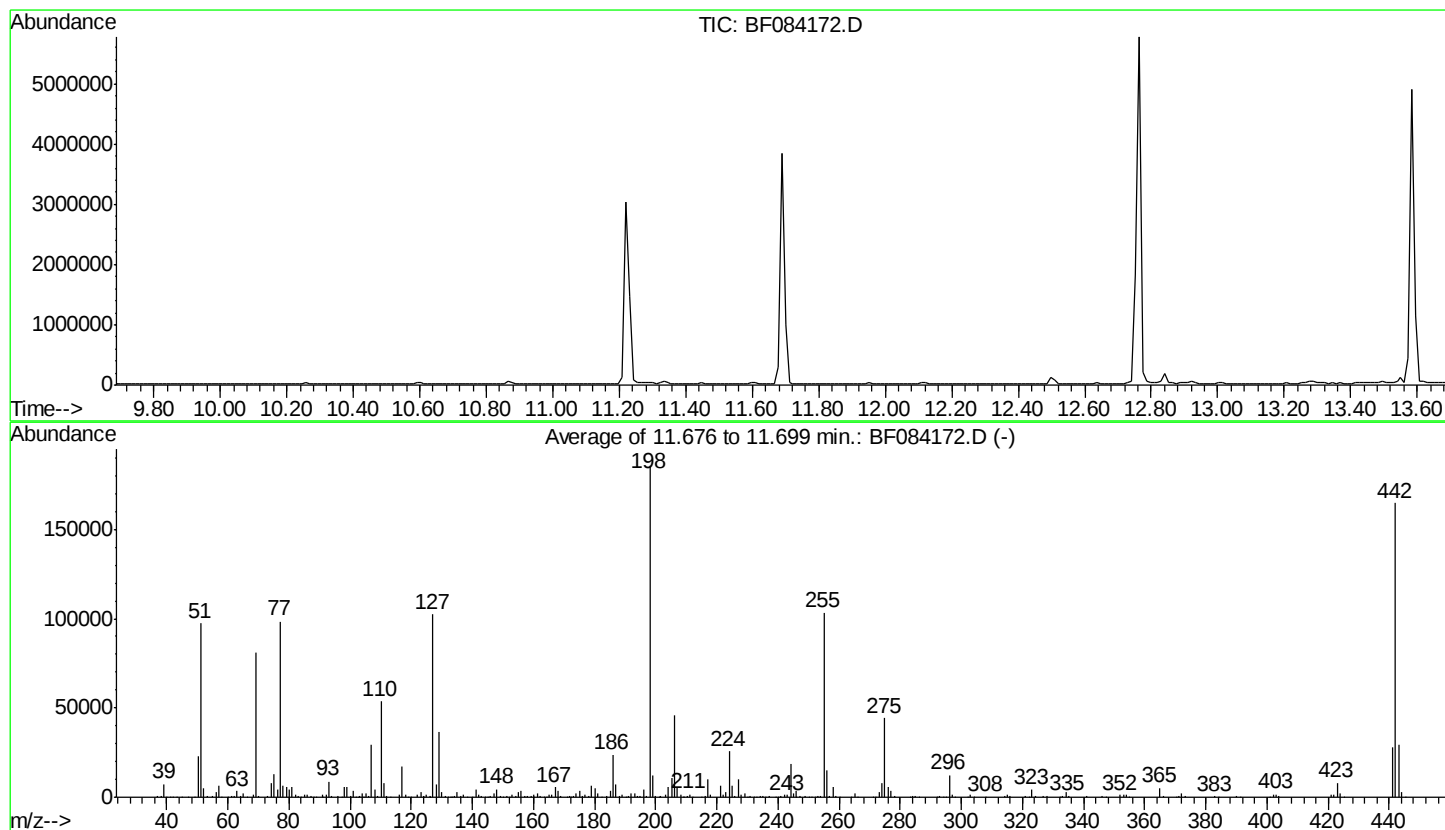

AutoFind: Scans 839, 840, 841; Background Corrected with Scan 836

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.3	97181	PASS
68	69	0.00	2	1.8	1464	PASS
69	198	0.00	100	43.7	81255	PASS
70	69	0.00	2	0.9	754	PASS
127	198	10	80	55.1	102314	PASS
197	198	0.00	2	0.6	1052	PASS
198	198	100	100	100.0	185728	PASS
199	198	5	9	6.7	12522	PASS
275	198	10	60	23.8	44274	PASS
365	198	1	100	2.9	5313	PASS
441	442	0.01	24	16.8	27733	PASS
442	198	50	100	88.7	164813	PASS
443	442	15	24	18.0	29736	PASS