
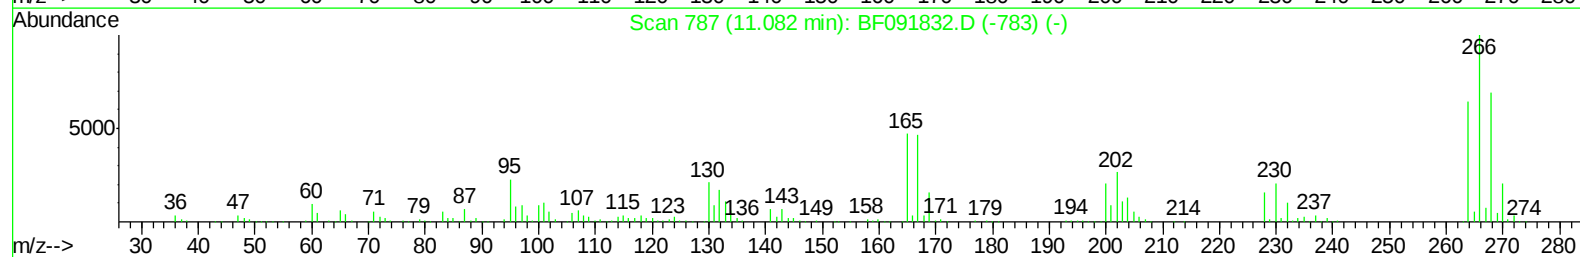
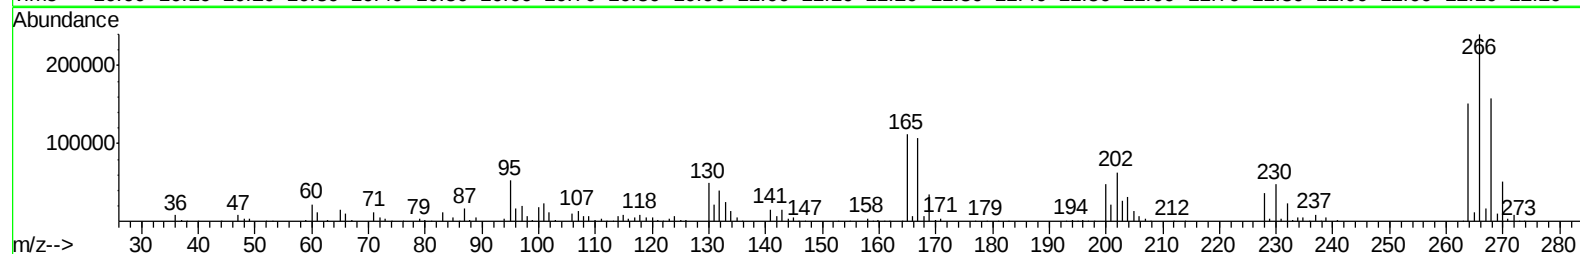


Data Path : Z:\HPCHEM1\BNA F\Data\BF123016\
Data File : BF092039.D
Acq On : 30 Dec 2016 10:19
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 03:54:30 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 17:32:10 2016
Response via : Initial Calibration

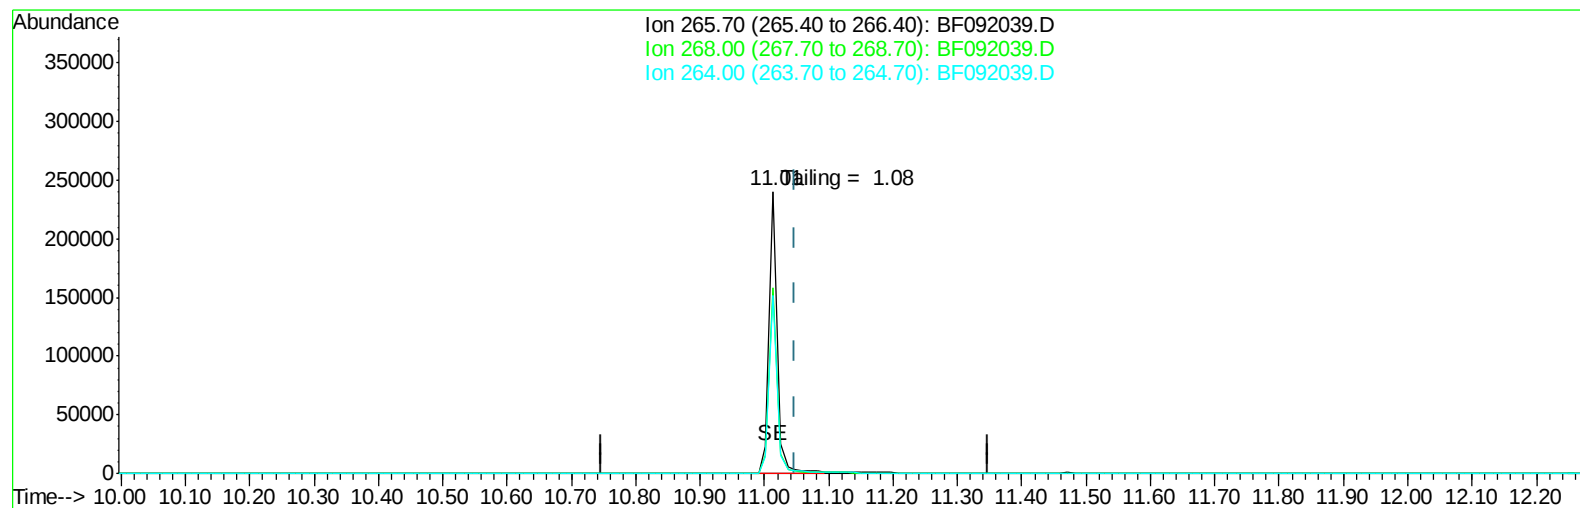

TIC: BF092039.D

(69) Pentachlorophenol (C)




11.013min (-0.034) 44917.61ng

response 194823

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	66.00
264.00	62.90	62.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF123016\
Data File : BF092039.D
Acq On : 30 Dec 2016 10:19
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 03:54:30 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 17:32:10 2016
Response via : Initial Calibration

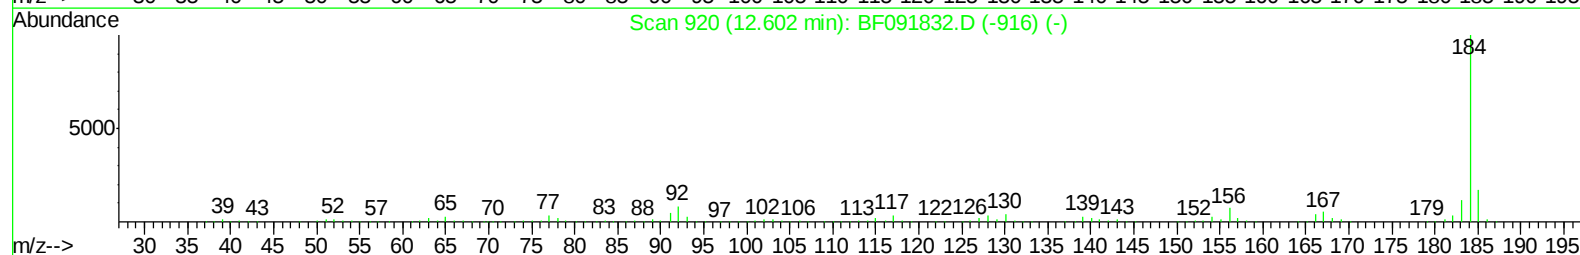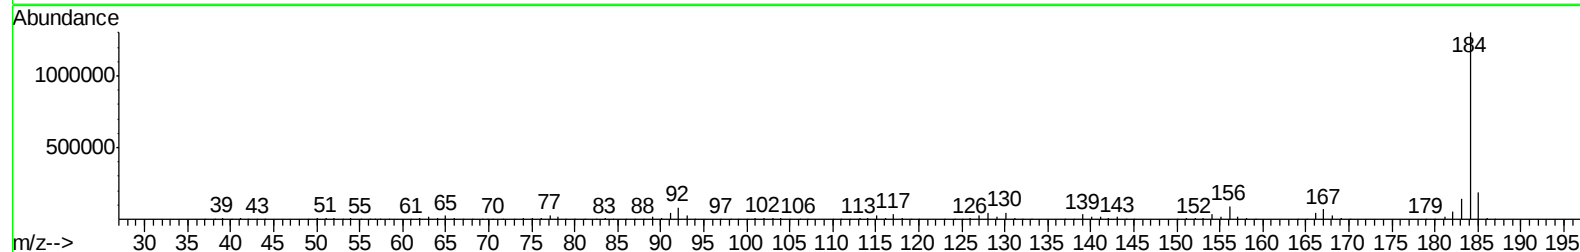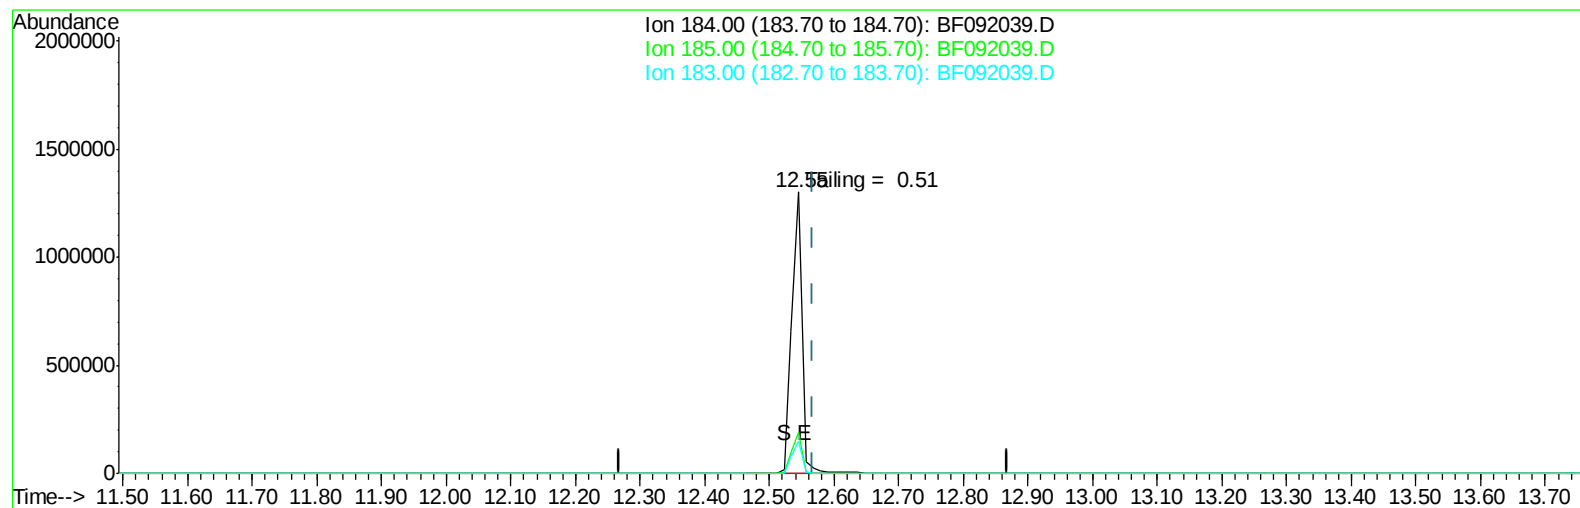

TIC: BF092039.D

(76) Benzidine

12.545min (-0.023) 0.00ng

response 1451278

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.44
183.00	11.50	11.29
0.00	0.00	0.00