


Data Path : Z:\HPCHEM1\BNA F\Data\BF123016\
 Data File : BF092039.D
 Acq On : 30 Dec 2016 10:19
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 28 17:32:10 2016

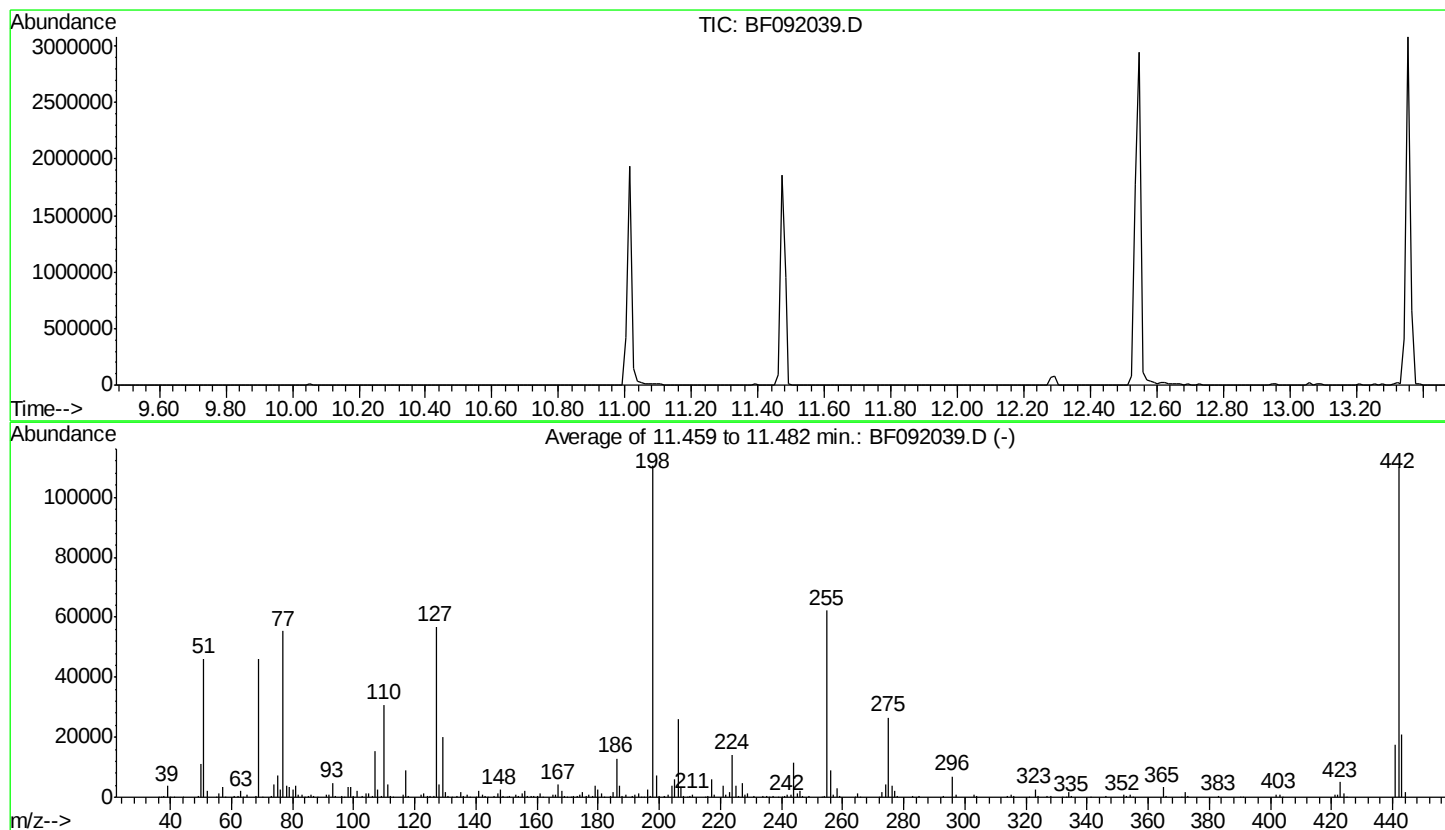

AutoFind: Scans 820, 821, 822; Background Corrected with Scan 817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	46084	PASS
68	69	0.00	2	1.3	606	PASS
69	198	0.00	100	41.8	46184	PASS
70	69	0.00	2	0.3	141	PASS
127	198	10	80	51.5	56917	PASS
197	198	0.00	2	0.6	635	PASS
198	198	100	100	100.0	110510	PASS
199	198	5	9	6.7	7422	PASS
275	198	10	60	24.0	26476	PASS
365	198	1	100	3.0	3346	PASS
441	442	0.01	24	15.7	17349	PASS
442	198	50	100	99.8	110240	PASS
443	442	15	24	18.9	20888	PASS