
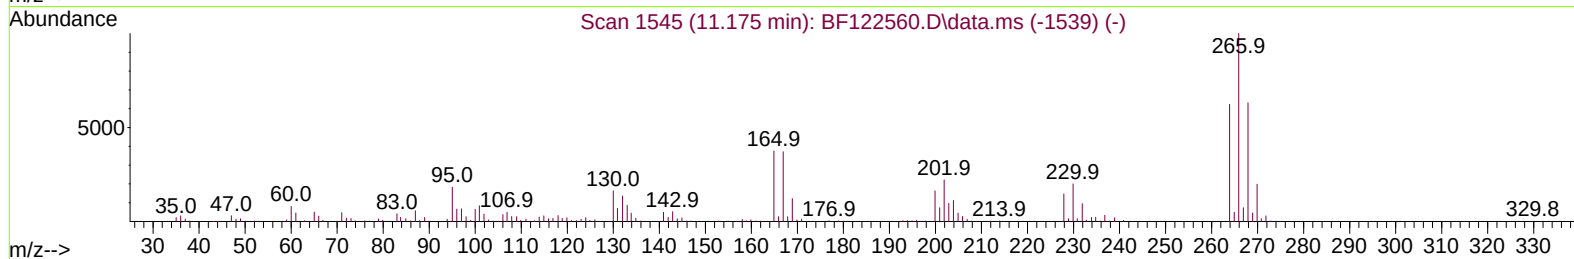
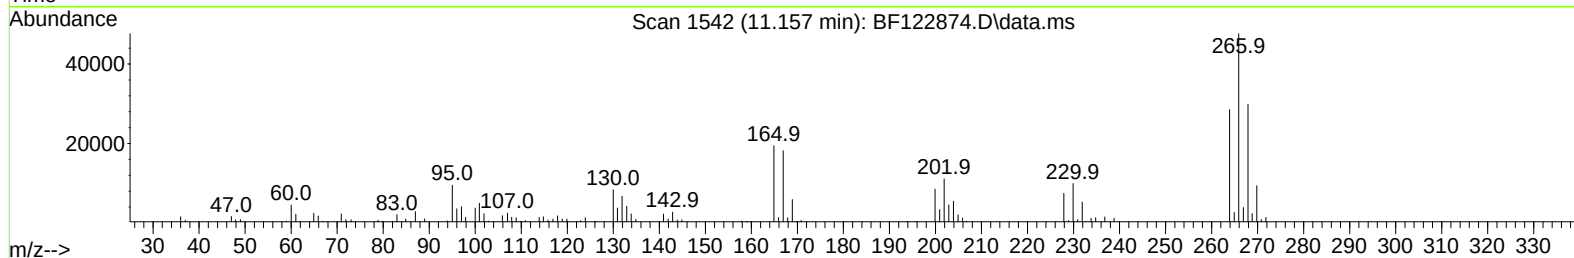


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123020\
Data File : BF122874.D
Acq On : 30 Dec 2020 12:27
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 02:54:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 18:14:23 2020
Response via : Initial Calibration

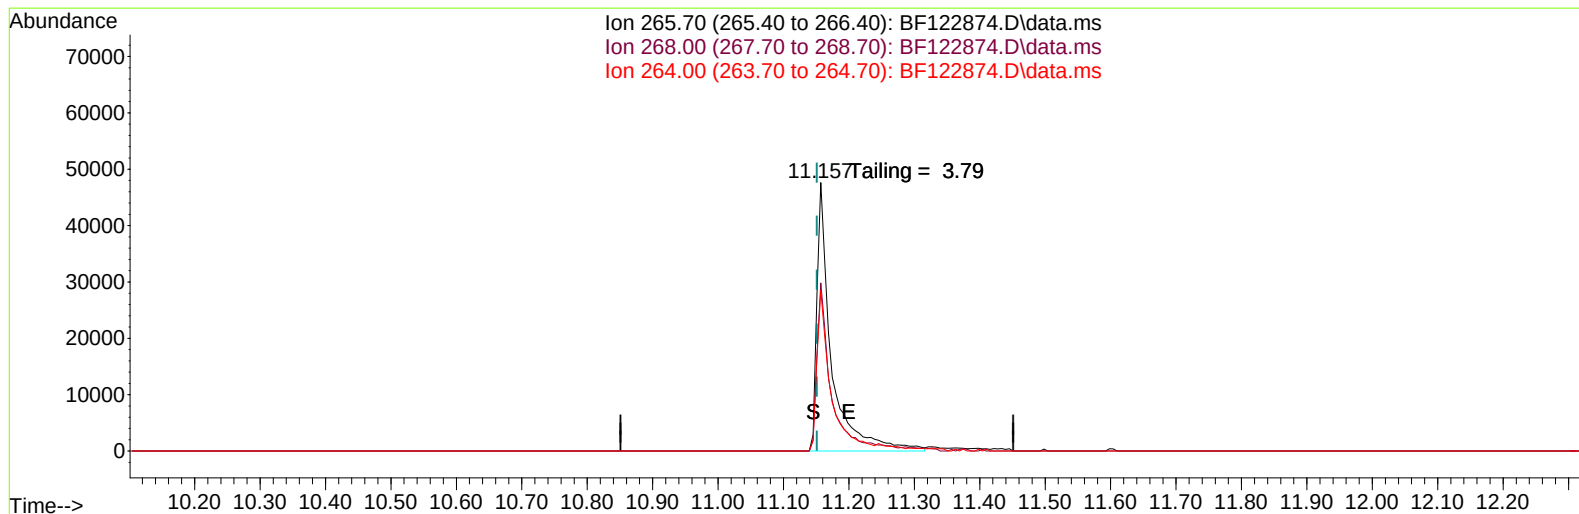

TIC: BF122874.D\data.ms

(70) Pentachlorophenol (C)




11.157min (+ 0.006) 23134.12 ng

response 74178

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.59
264.00	62.30	59.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123020\
 Data File : BF122874.D
 Acq On : 30 Dec 2020 12:27
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 02:54:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 15 18:14:23 2020
 Response via : Initial Calibration

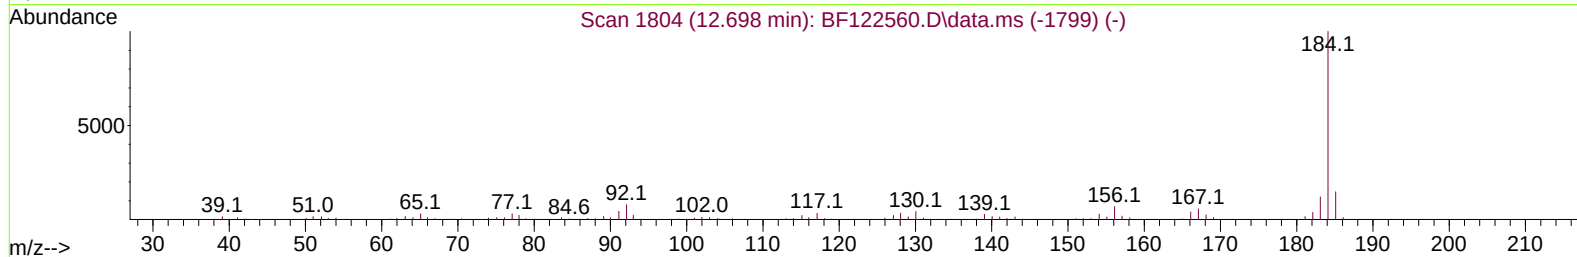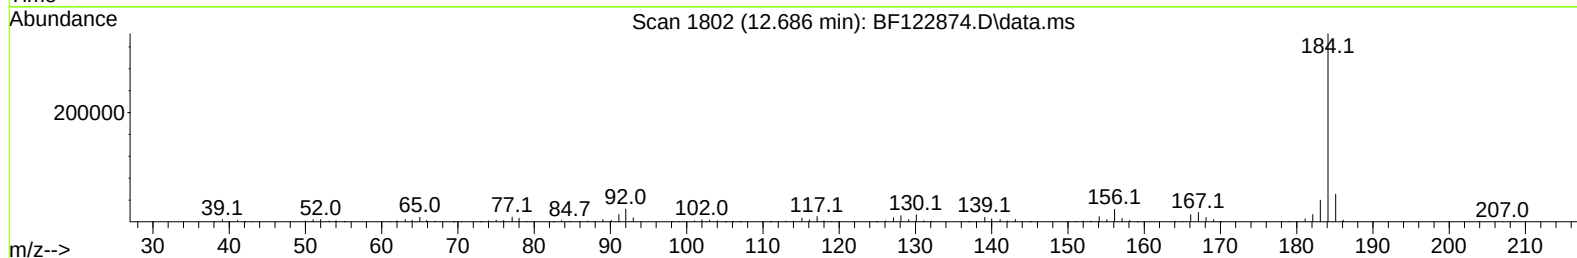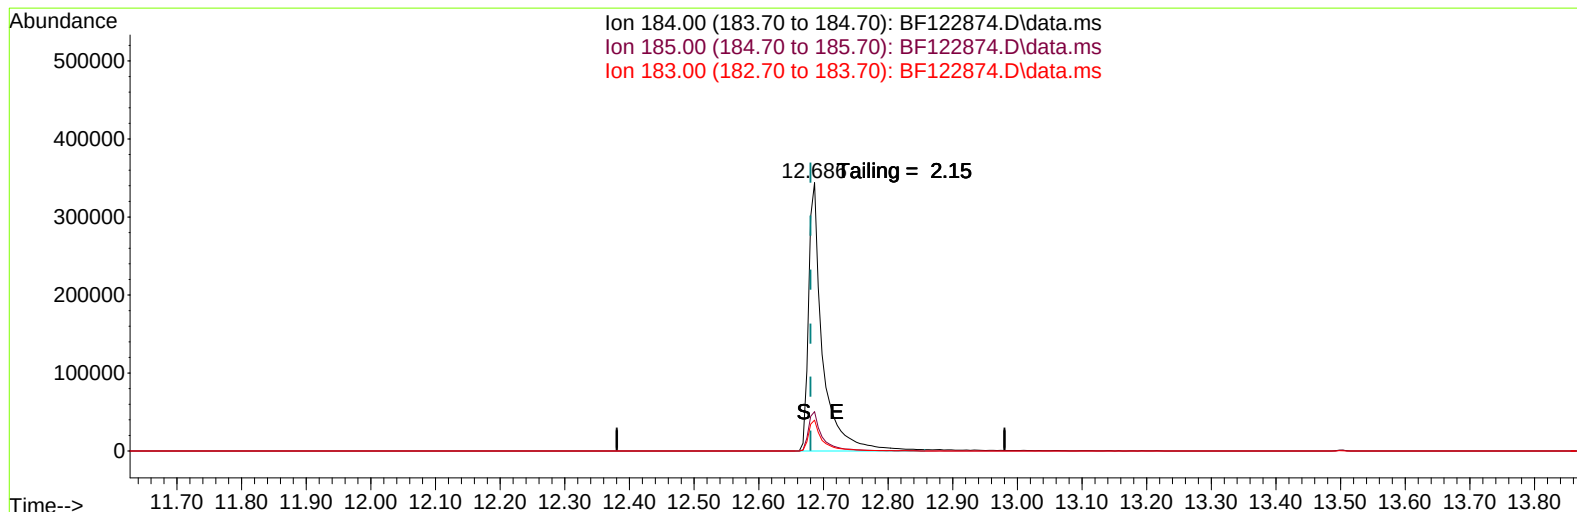

TIC: BF122874.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 0.00 ng

response 522890

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.70
183.00	12.10	11.55
0.00	0.00	0.00