
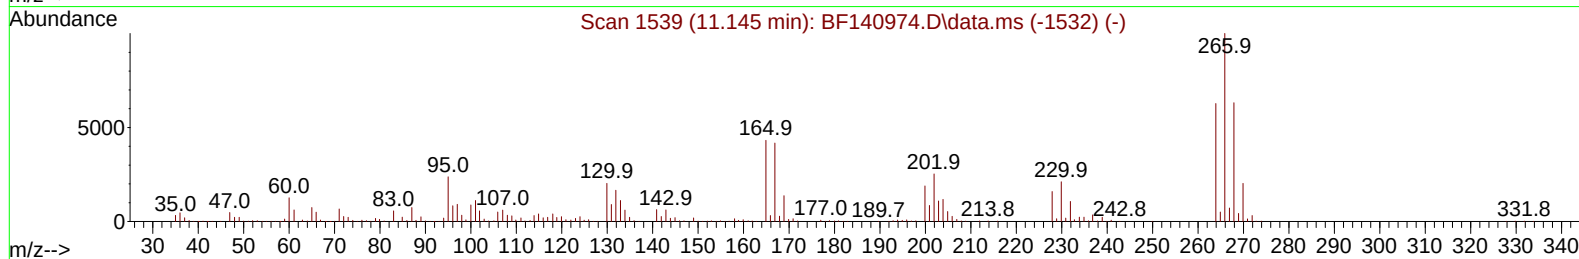
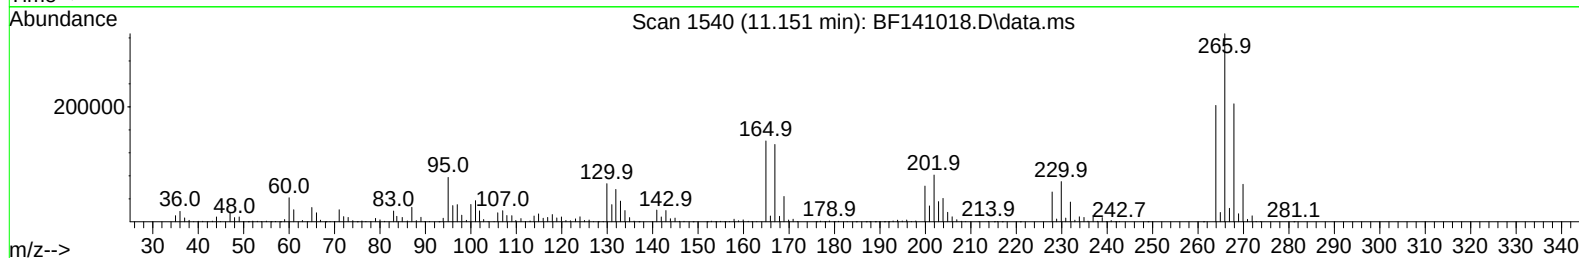


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141018.D
Acq On : 30 Dec 2024 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 10:08:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

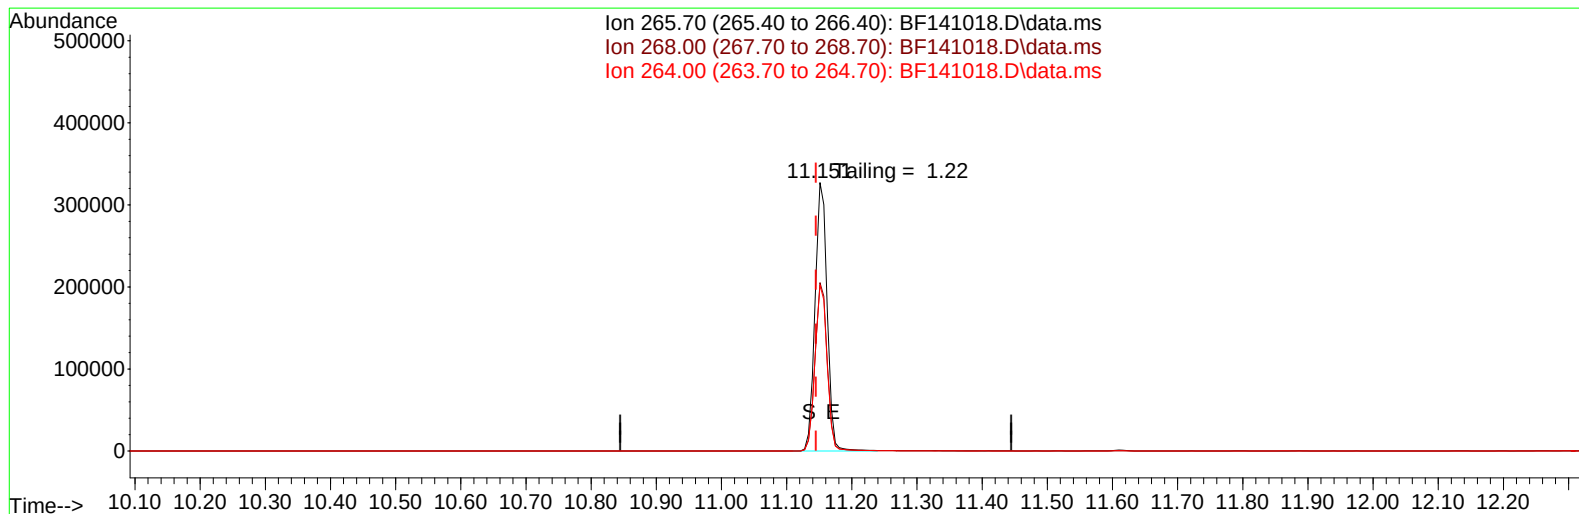

TIC: BF141018.D\data.ms

(70) Pentachlorophenol (C)




11.151min (+ 0.006) 118641.00 ng

response 426155

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.72
264.00	62.80	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141018.D
Acq On : 30 Dec 2024 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 10:08:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

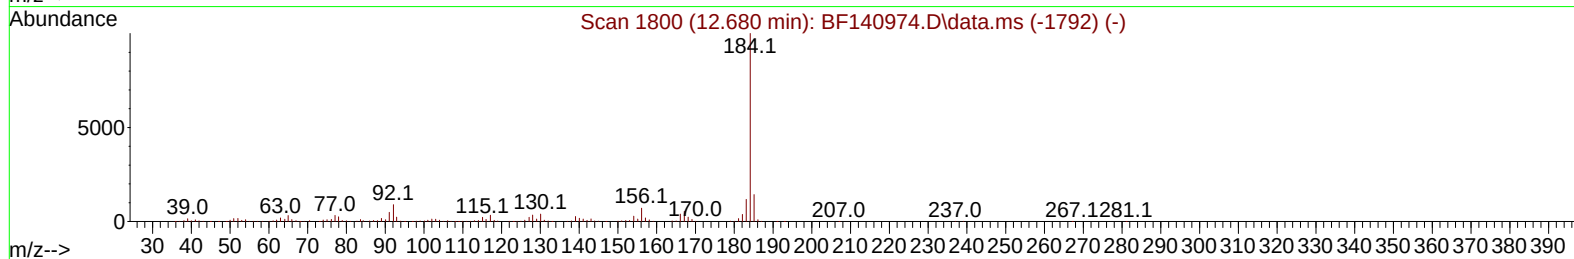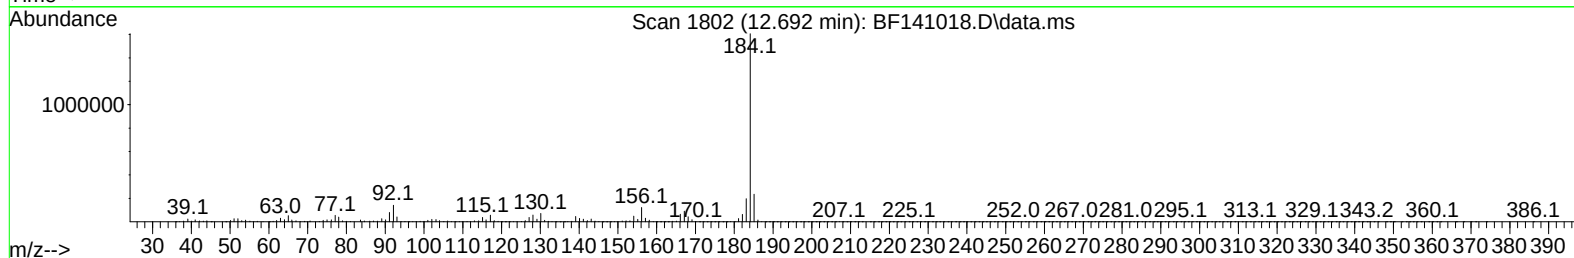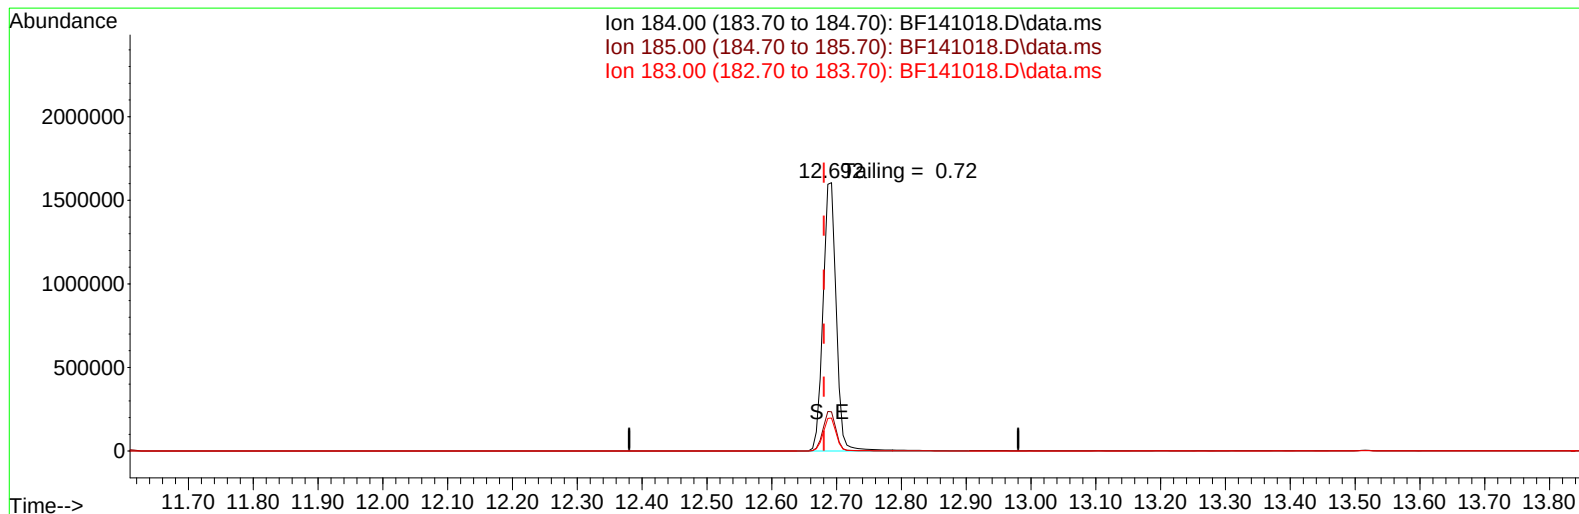

TIC: BF141018.D\data.ms

(77) Benzidine**12.692min (+ 0.012) 182948.18 ng****response 2285059**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.65
183.00	11.70	12.30
0.00	0.00	0.00