

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141020.D
Acq On : 30 Dec 2024 09:50
Operator : RC/JU
Sample : PB165894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165894BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141020.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.451	564	571	576	rBV	6243968	8870126	78.64%	13.541%
2	6.451	734	741	747	rBV	5806241	8856485	78.52%	13.520%
3	6.828	800	805	811	rVB	1428598	1771293	15.70%	2.704%
4	7.392	893	901	906	rBV	3887113	5655334	50.14%	8.633%
5	8.110	1016	1023	1028	rBV	1866116	2400169	21.28%	3.664%
6	9.186	1198	1206	1211	rBV	7689315	10671476	94.61%	16.291%
7	9.863	1314	1321	1326	rBV	2185736	2761094	24.48%	4.215%
8	10.651	1448	1455	1460	rBV	4887257	6484667	57.49%	9.899%
9	11.345	1568	1573	1579	rBV	2152197	2799629	24.82%	4.274%
10	12.939	1838	1844	1849	rBV	8170957	11279257	100.00%	17.218%
11	13.986	2017	2022	2028	rBV	1719879	2215343	19.64%	3.382%
12	15.451	2265	2271	2277	rBV	1080550	1742306	15.45%	2.660%




Sum of corrected areas: 65507179

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141020.D
Acq On : 30 Dec 2024 09:50
Operator : RC/JU
Sample : PB165894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165894BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

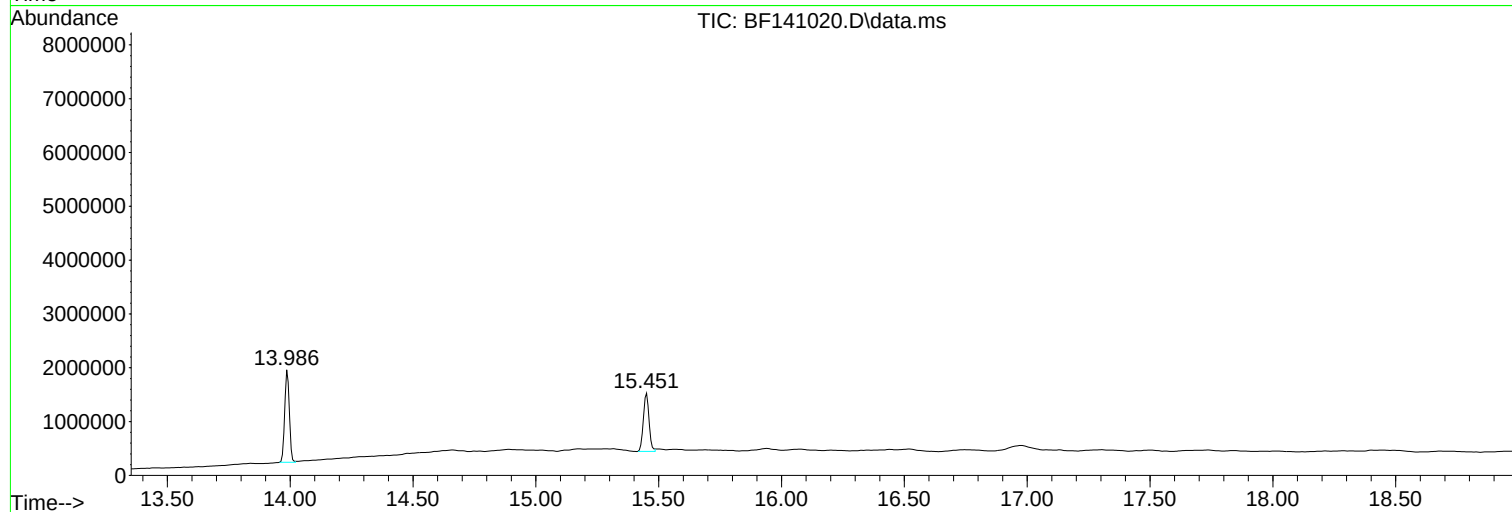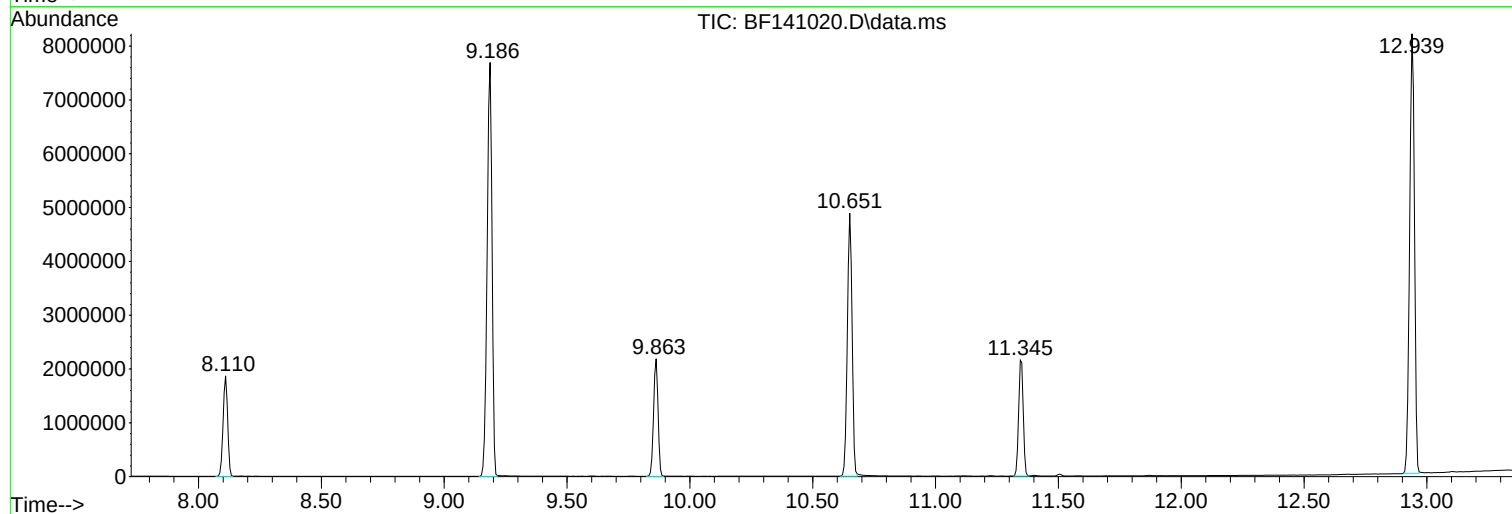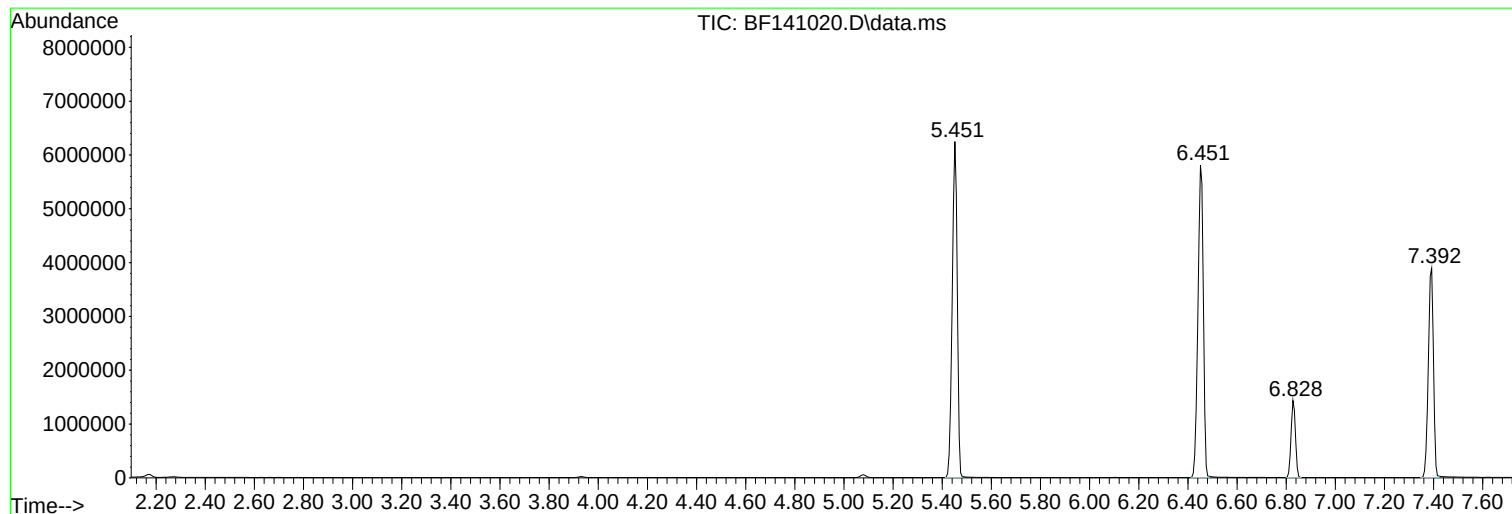

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141020.D
Acq On : 30 Dec 2024 09:50
Operator : RC/JU
Sample : PB165894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165894BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141020.D
Acq On : 30 Dec 2024 09:50
Operator : RC/JU
Sample : PB165894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165894BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------