

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141026.D
Acq On : 30 Dec 2024 12:30
Operator : RC/JU
Sample : PB165875BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165875BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.152	6	10	18	rVB	84720	149124	1.42%	0.241%
2	5.446	563	570	576	rBV	5922986	8545928	81.32%	13.790%
3	6.451	733	741	746	rBV	5756301	8695035	82.74%	14.031%
4	6.828	799	805	810	rBV	1221634	1493966	14.22%	2.411%
5	7.387	893	900	905	rBV	4077505	5696602	54.21%	9.192%
6	8.104	1016	1022	1028	rBV	1516039	2031529	19.33%	3.278%
7	9.181	1198	1205	1211	rBV	7308648	10263952	97.67%	16.562%
8	9.857	1314	1320	1331	rBV	1829047	2325002	22.12%	3.752%
9	10.645	1447	1454	1476	rBV	4678191	6521206	62.06%	10.523%
10	11.345	1567	1573	1578	rBV	1862480	2337186	22.24%	3.771%
11	12.933	1837	1843	1849	rBV	7696498	10508694	100.00%	16.957%
12	13.980	2016	2021	2031	rBV	1381904	1801058	17.14%	2.906%
13	15.445	2264	2270	2292	rVB	967131	1602635	15.25%	2.586%




Sum of corrected areas: 61971917

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141026.D
Acq On : 30 Dec 2024 12:30
Operator : RC/JU
Sample : PB165875BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165875BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

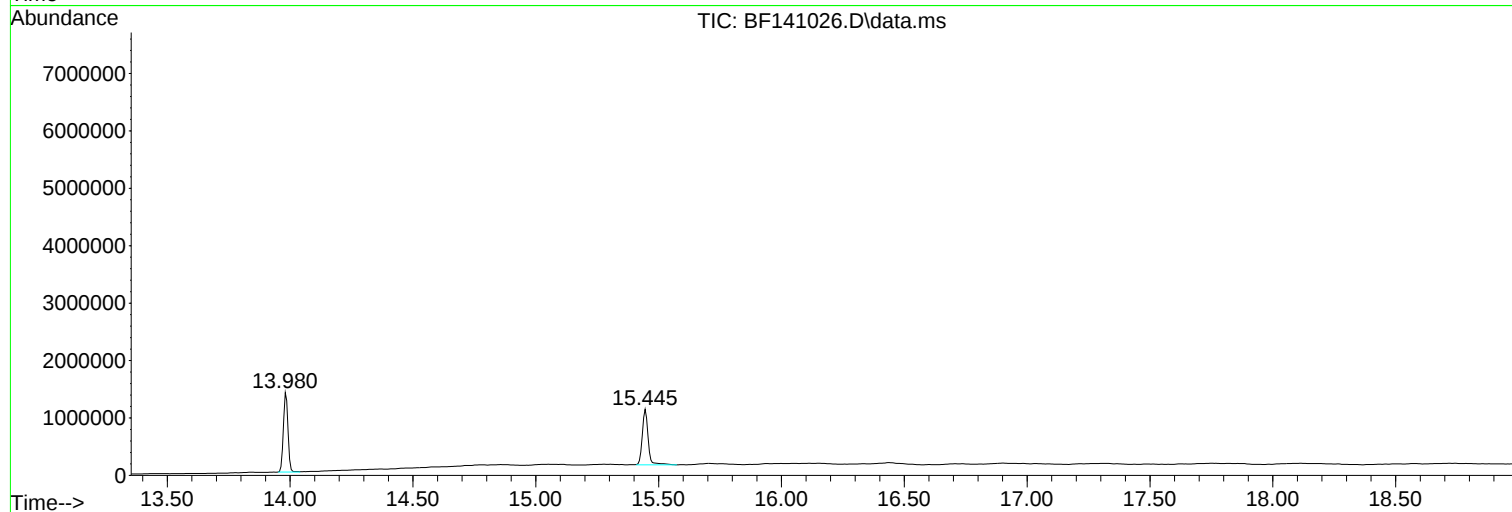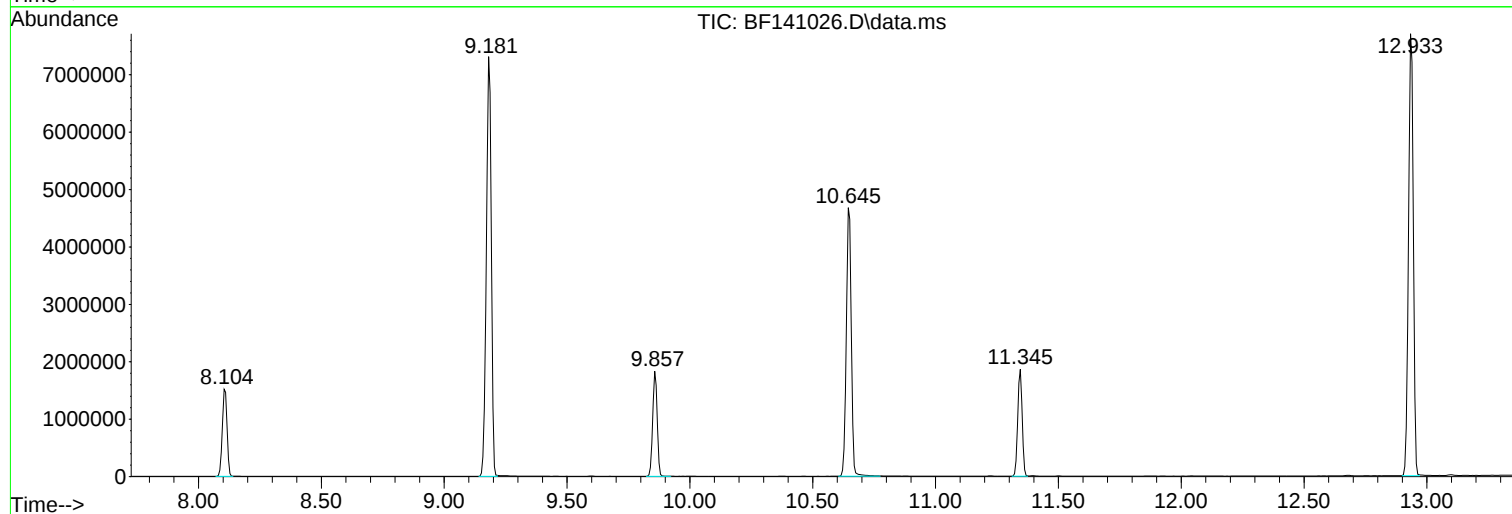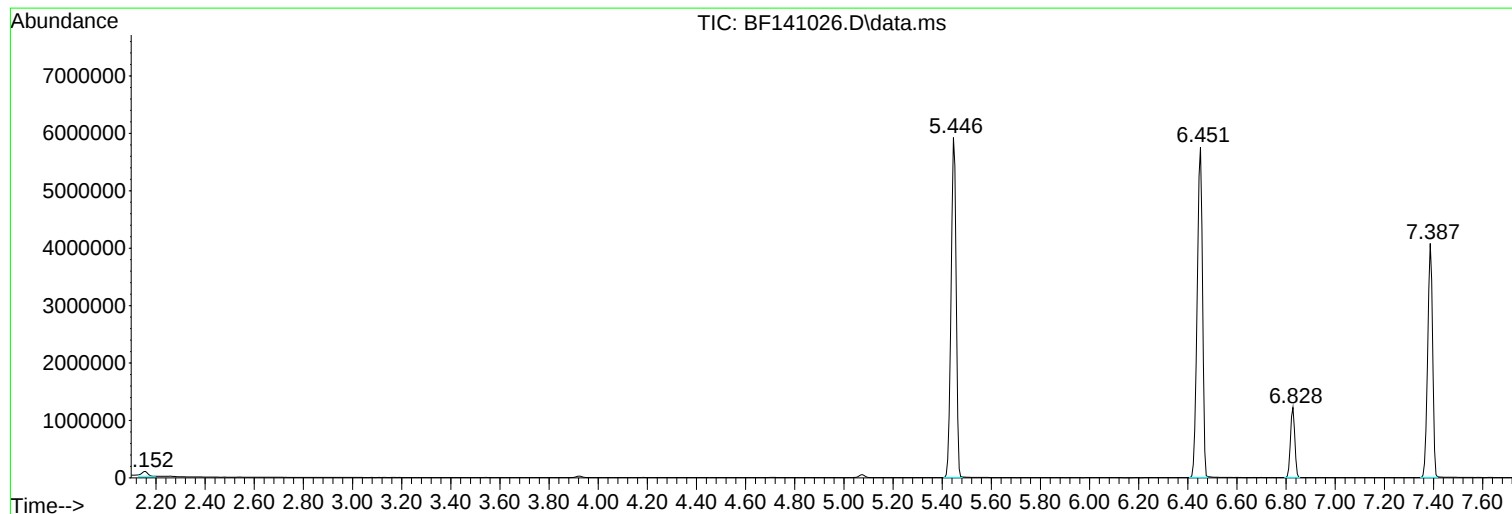

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141026.D
Acq On : 30 Dec 2024 12:30
Operator : RC/JU
Sample : PB165875BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165875BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141026.D
Acq On : 30 Dec 2024 12:30
Operator : RC/JU
Sample : PB165875BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165875BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------