

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
 Data File : BF141032.D
 Acq On : 30 Dec 2024 15:47
 Operator : RC/JU
 Sample : PB165900BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB165900BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	6	12	24	rVB	108695	197632	1.83%	0.319%
2	5.445	563	570	575	rBV	5805100	8218545	76.27%	13.271%
3	6.445	733	740	746	rBV	5409778	8196688	76.07%	13.235%
4	6.828	799	805	810	rBV	1230533	1591730	14.77%	2.570%
5	7.387	893	900	905	rBV	3843663	5467384	50.74%	8.828%
6	8.104	1016	1022	1028	rBV	1673670	2163812	20.08%	3.494%
7	9.181	1198	1205	1210	rBV	7148202	9881553	91.70%	15.956%
8	9.857	1313	1320	1325	rBV	1953582	2496098	23.16%	4.031%
9	10.645	1447	1454	1480	rBV	4787540	6544417	60.73%	10.567%
10	11.345	1567	1573	1578	rBV	1943457	2555057	23.71%	4.126%
11	12.933	1837	1843	1848	rBV	7919846	10775431	100.00%	17.399%
12	13.980	2015	2021	2035	rBV	1656083	2146828	19.92%	3.467%
13	15.439	2263	2269	2287	rBV	1004388	1694768	15.73%	2.737%




Sum of corrected areas: 61929943

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141032.D
Acq On : 30 Dec 2024 15:47
Operator : RC/JU
Sample : PB165900BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165900BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

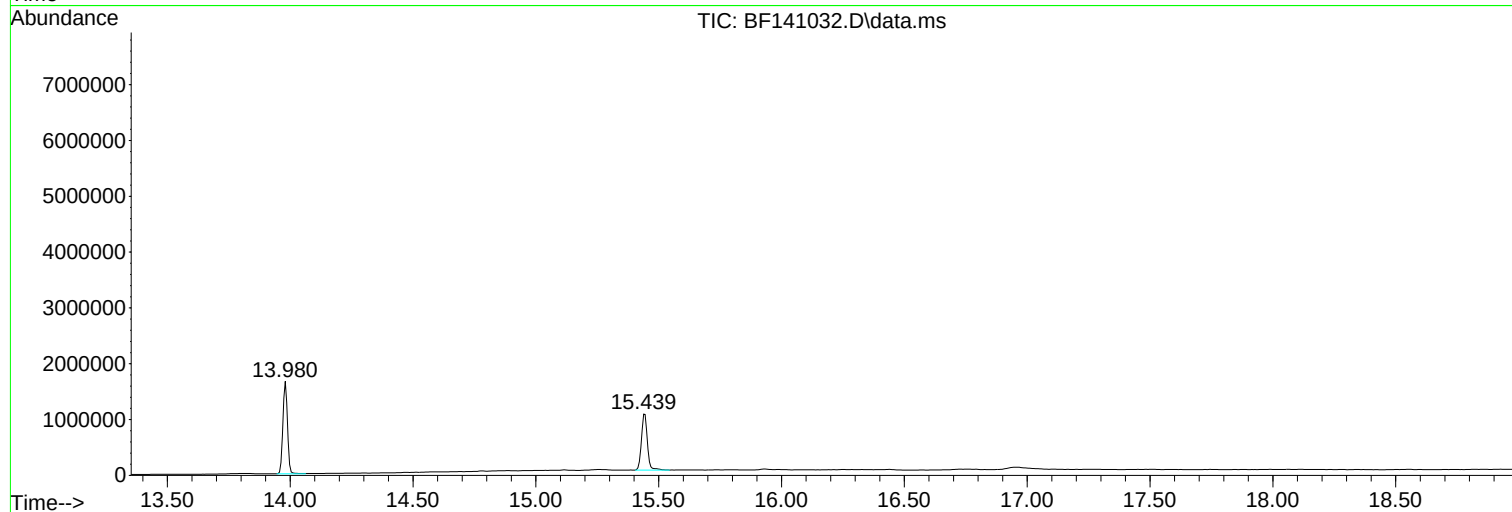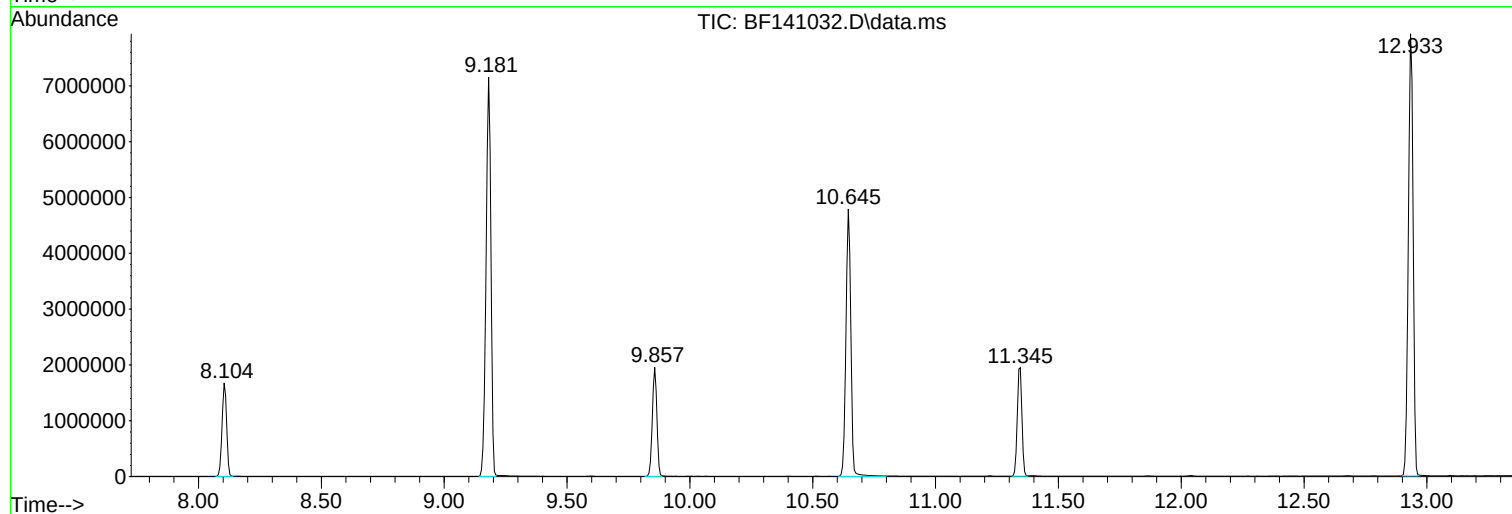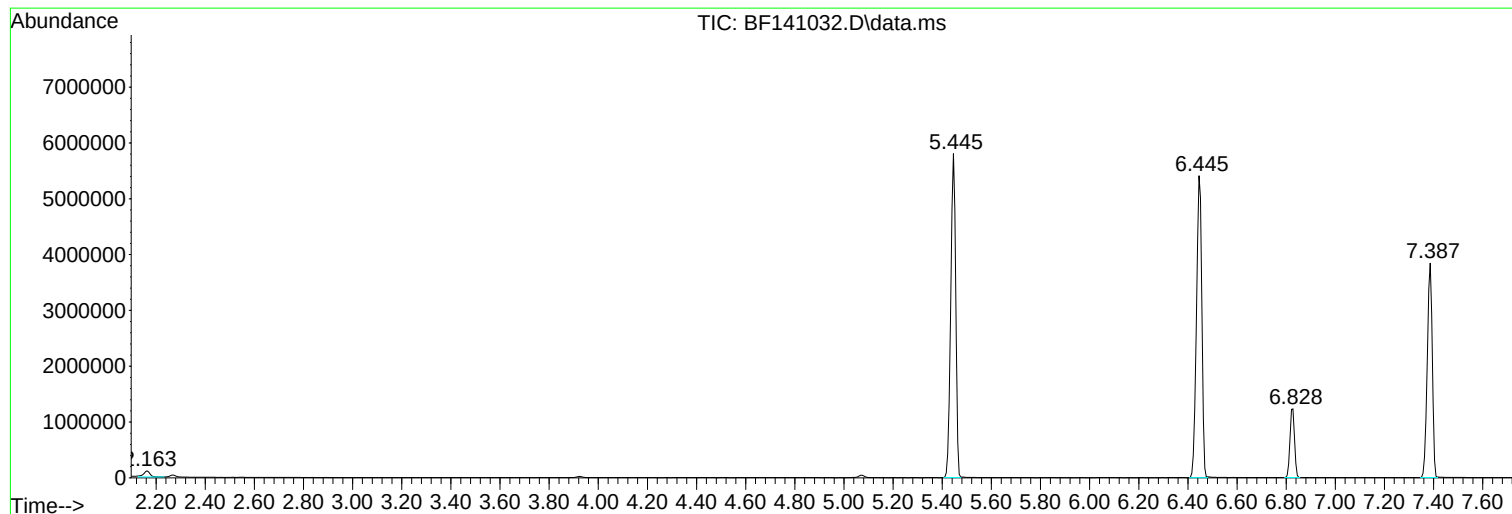

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141032.D
Acq On : 30 Dec 2024 15:47
Operator : RC/JU
Sample : PB165900BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165900BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.163	2.48 ng	197632	1,4-Dichlorobenzene-d4	6.828

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
2			Silane, tetramethyl-	88	C4H12Si	000075-76-3	35
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
4			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

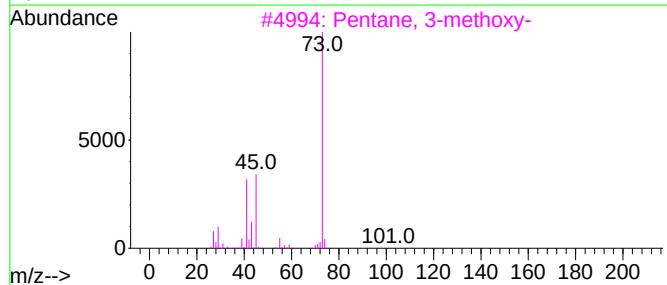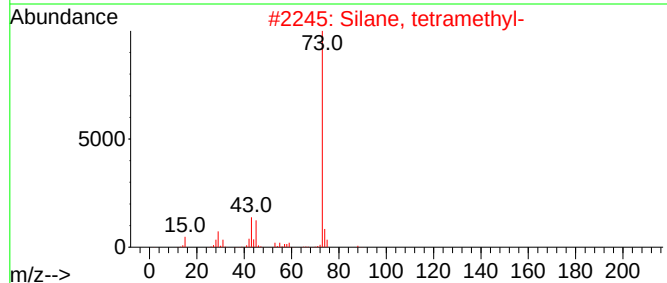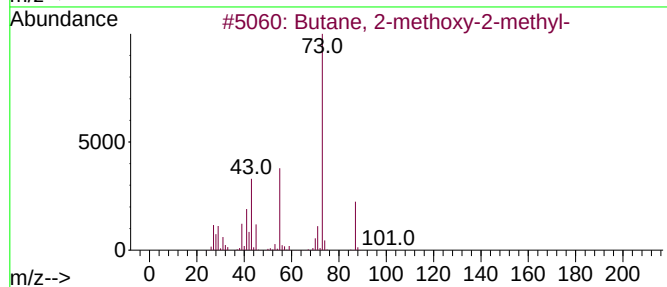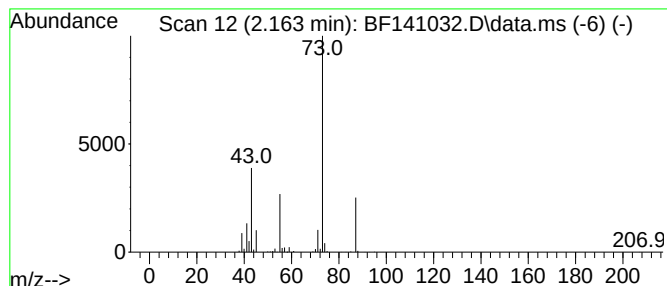

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141032.D
Acq On : 30 Dec 2024 15:47
Operator : RC/JU
Sample : PB165900BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165900BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.163	2.5	ng	197632	1	6.828	1591730	20.0