


Data Path : Z:\HPCHEM1\BNA_F\Data\BF123114\
 Data File : BF076715.D
 Acq On : 31 Dec 2014 21:44
 Operator : IZ / TP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121714.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 01 04:58:19 2015

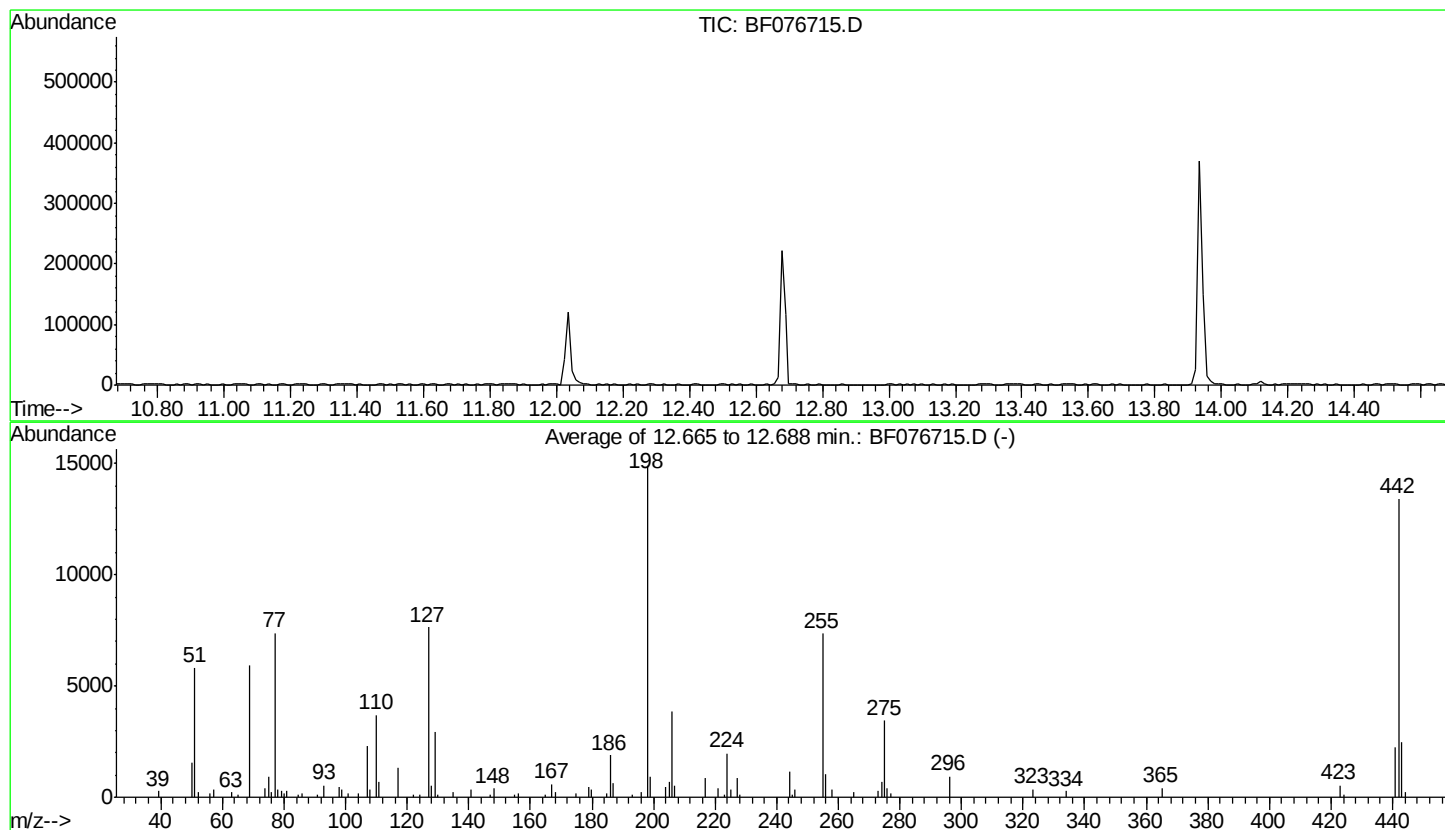

AutoFind: Scans 1013, 1014, 1015; Background Corrected with Scan 1010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	5842	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.6	5903	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.3	7645	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14907	PASS
199	198	5	9	6.4	951	PASS
275	198	10	60	23.1	3438	PASS
365	198	1	100	2.8	412	PASS
441	442	0.01	24	16.7	2245	PASS
442	198	50	100	90.1	13427	PASS
443	442	15	24	18.5	2483	PASS