

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF123114\
 Data File : BF076708.D
 Acq On : 31 Dec 2014 18:24
 Operator : IZ / TP
 Sample : PB81132BL
 Misc : W
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB81132BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121714.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.144	3	5	7	rVB	14453	18918	1.27%	0.176%
2	1.418	28	29	35	rBV	58997	100326	6.75%	0.932%
3	1.510	35	37	50	rVB	115023	261515	17.59%	2.428%
4	4.241	273	276	284	rBV	183486	314193	21.13%	2.917%
5	4.904	331	334	344	rVB	748092	1035357	69.64%	9.613%
6	6.322	455	458	460	rBV	939475	1029965	69.28%	9.563%
7	6.424	464	467	469	rBV	1068306	1083999	72.91%	10.065%
8	6.722	490	493	495	rBV	170882	211269	14.21%	1.962%
9	6.904	506	509	511	rBV	858390	822865	55.35%	7.640%
10	7.430	552	555	557	rBV	646162	658280	44.28%	6.112%
11	8.299	629	631	634	rBV	320557	290549	19.54%	2.698%
12	9.648	747	749	752	rBV	1305217	1243438	83.63%	11.545%
13	10.448	816	819	821	rBV	364439	321800	21.64%	2.988%
14	11.408	901	903	906	rBV2	576407	826872	55.62%	7.677%
15	12.254	975	977	980	rBV	353393	343514	23.10%	3.190%
16	14.242	1148	1151	1154	rBV	1423640	1486756	100.00%	13.804%
17	15.488	1258	1260	1263	rBV	358069	369981	24.89%	3.435%
18	17.180	1405	1408	1411	rBV	299315	350486	23.57%	3.254%


Sum of corrected areas: 10770083

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF123114\
Data File : BF076708.D
Acq On : 31 Dec 2014 18:24
Operator : IZ / TP
Sample : PB81132BL
Misc : W
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81132BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121714.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

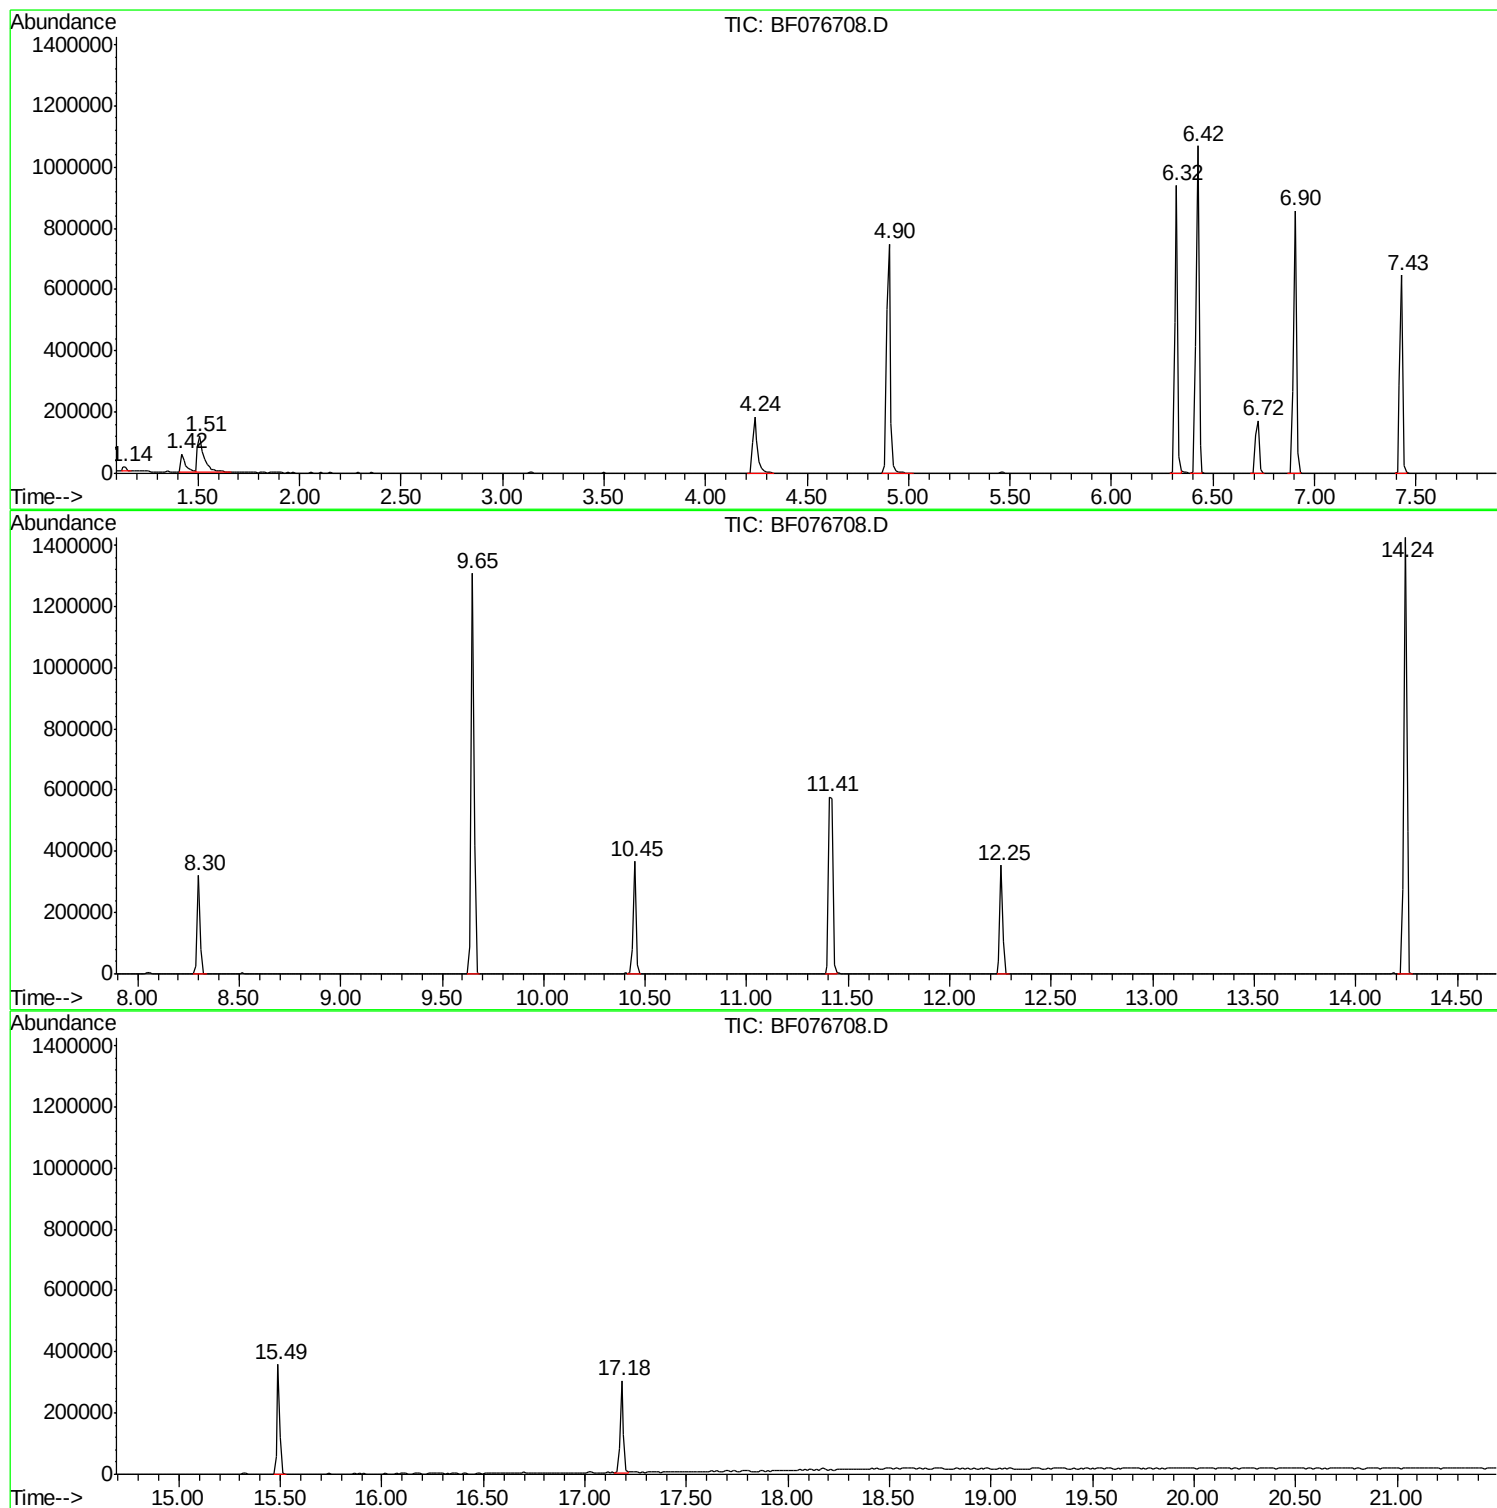

Data Path : Z:\HPCHEM1\BNA F\DATA\BF123114\
Data File : BF076708.D
Acq On : 31 Dec 2014 18:24
Operator : IZ / TP
Sample : PB81132BL
Misc : W
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
PB81132BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121714.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.24	29.74 ng	314193	1,4-Dichlorobenzene-d4	6.72

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	40
2			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	36
3			1,8-Nonanediol, 8-methyl-	174	C10H22O2	054725-73-4	33
4			Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	28
5			4-Penten-2-one, 4-methyl-	98	C6H10O	003744-02-3	9

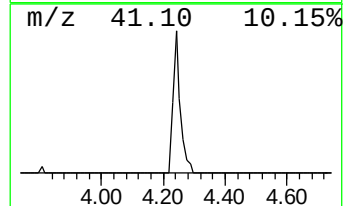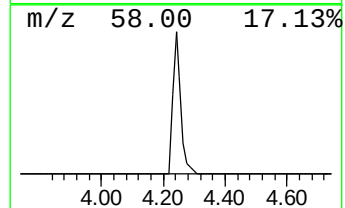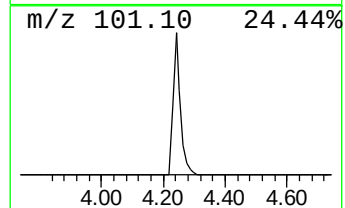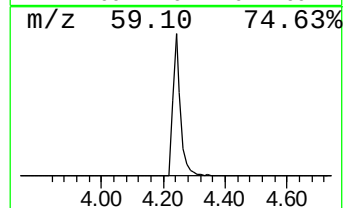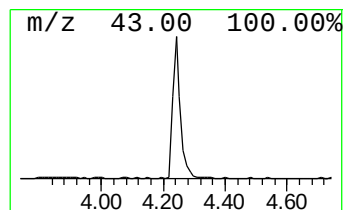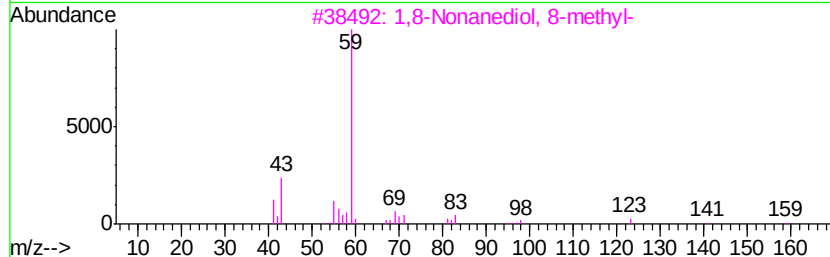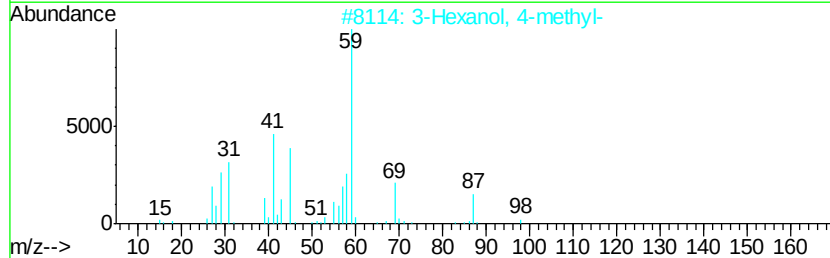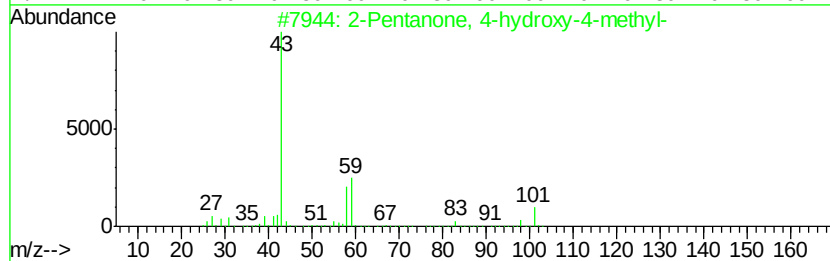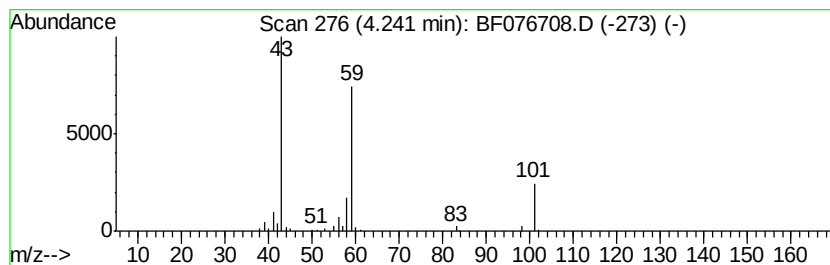

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF123114\
Data File : BF076708.D
Acq On : 31 Dec 2014 18:24
Operator : IZ / TP
Sample : PB81132BL
Misc : W
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81132BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121714.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown6.42 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.42	102.62 ng	1084000	1,4-Dichlorobenzene-d4	6.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

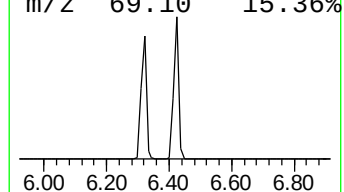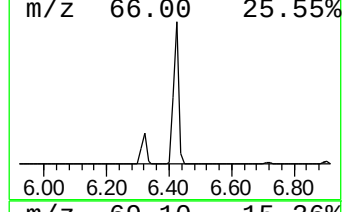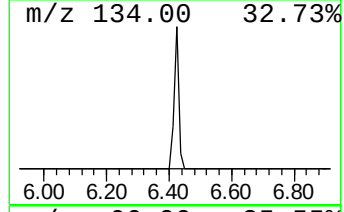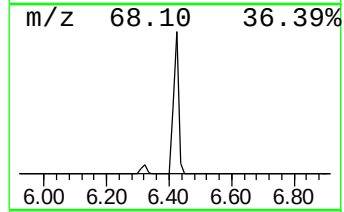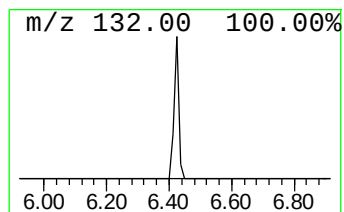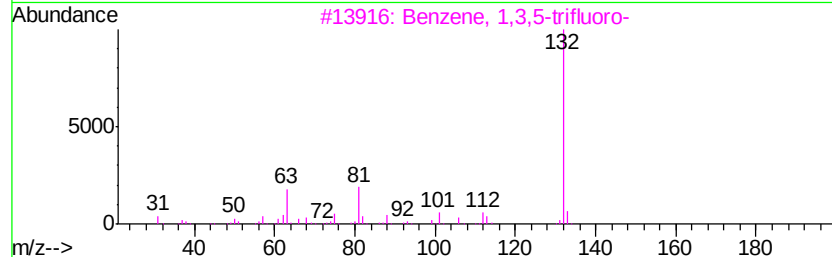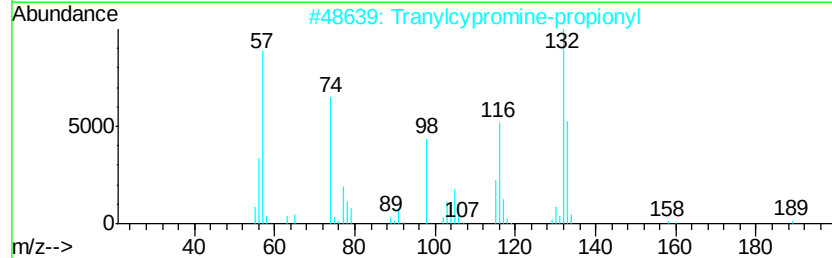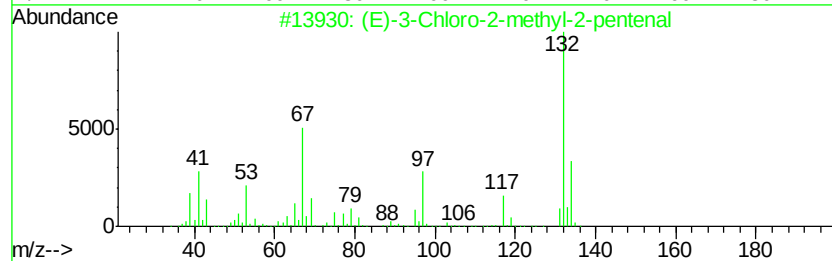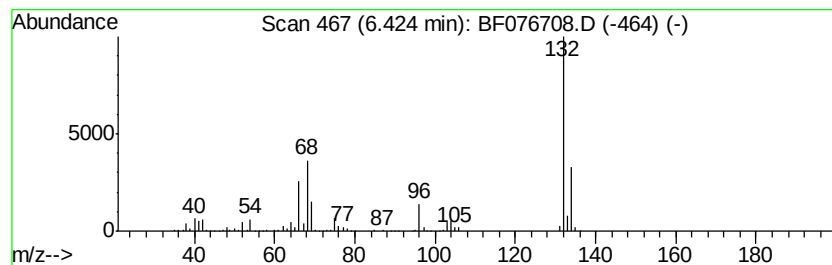

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF123114\
Data File : BF076708.D
Acq On : 31 Dec 2014 18:24
Operator : IZ / TP
Sample : PB81132BL
Misc : W
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81132BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121714.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.24	29.7	ng	314193	1	6.72	211269	20.0
unknown6.42	6.42	102.6	ng	1084000	1	6.72	211269	20.0