

Data Path : Z:\HPCHEM1\BNA F\DATA\BF123114\
 Data File : BF076717.D
 Acq On : 31 Dec 2014 23:37
 Operator : IZ / TP
 Sample : F5249-01
 Misc : W
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RWB4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121714.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.418	28	29	35	rBV	224096	383014	11.99%	1.141%
2	1.510	35	37	55	rVB	447789	1099354	34.40%	3.274%
3	3.270	188	191	195	rVB	25433	57027	1.78%	0.170%
4	4.241	273	276	283	rBV	513600	926036	28.98%	2.758%
5	4.904	331	334	340	rVB	226204	337758	10.57%	1.006%
6	6.310	455	457	464	rVB2	164302	208797	6.53%	0.622%
7	6.424	464	467	469	rBV	557430	714894	22.37%	2.129%
8	6.504	472	474	476	rVB	27953	35384	1.11%	0.105%
9	6.722	490	493	495	rBV	162743	219707	6.88%	0.654%
10	6.905	506	509	511	rBV	807944	861992	26.97%	2.567%
11	6.939	511	512	514	rVB	77419	56635	1.77%	0.169%
12	7.430	552	555	557	rBV	599563	695132	21.75%	2.070%
13	7.990	602	604	607	rVB2	61802	74026	2.32%	0.220%
14	8.299	629	631	632	rBV	369646	338873	10.60%	1.009%
15	8.322	632	633	636	rVB	451025	430685	13.48%	1.283%
16	8.756	669	671	673	rBV	49303	61063	1.91%	0.182%
17	8.905	681	684	686	rBV	35071	47926	1.50%	0.143%
18	9.019	693	694	699	rVB2	33844	57893	1.81%	0.172%
19	9.179	706	708	712	rVV	860729	924559	28.93%	2.753%
20	9.293	716	718	721	rVB	609841	767672	24.02%	2.286%
21	9.648	747	749	751	rBV	1459546	1303960	40.81%	3.883%
22	9.762	757	759	761	rVB	265590	237178	7.42%	0.706%
23	9.865	766	768	771	rVV2	364722	473644	14.82%	1.411%
24	9.956	774	776	778	rVV	134600	221011	6.92%	0.658%
25	10.048	781	784	785	rBV	242581	309190	9.68%	0.921%
26	10.071	785	786	788	rVV	153614	158953	4.97%	0.473%
27	10.185	792	796	799	rBV2	100454	213074	6.67%	0.635%
28	10.242	799	801	803	rBV	136179	155139	4.85%	0.462%
29	10.276	803	804	807	rVB	84362	81333	2.55%	0.242%
30	10.448	816	819	821	rBV2	372852	474899	14.86%	1.414%
31	10.493	821	823	825	rVV	3047352	3195558	100.00%	9.516%
32	10.539	825	827	828	rVB	152731	123815	3.87%	0.369%
33	10.642	834	836	838	rVB2	89143	144761	4.53%	0.431%
34	10.699	838	841	845	rVB	1297888	1319543	41.29%	3.930%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF123114\
 Data File : BF076717.D
 Acq On : 31 Dec 2014 23:37
 Operator : IZ / TP
 Sample : F5249-01
 Misc : W
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RWB4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121714.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.802	848	850	852 rBV2	27053	42014	1.31%	0.125%
36	10.836	852	853	856 rVB2	32414	54934	1.72%	0.164%
37	11.019	866	869	871 rVB2	64172	63574	1.99%	0.189%
38	11.122	875	878	880 rVV	2096444	1976106	61.84%	5.885%
39	11.191	882	884	886 rVV	75444	149398	4.68%	0.445%
40	11.236	886	888	891 rVV2	349805	535747	16.77%	1.595%
41	11.282	891	892	893 rVV	53351	38834	1.22%	0.116%
42	11.316	893	895	897 rVV	102152	143929	4.50%	0.429%
43	11.351	897	898	900 rVV	136341	112305	3.51%	0.334%
44	11.419	901	904	907 rVV3	587846	942941	29.51%	2.808%
45	11.488	907	910	912 rVV	23941	55597	1.74%	0.166%
46	11.568	915	917	921 rVB	107400	127407	3.99%	0.379%
47	11.796	931	937	938 rBV3	68209	130384	4.08%	0.388%
48	11.968	950	952	955 rBV4	25856	36775	1.15%	0.110%
49	12.036	955	958	961 rVV2	1307835	1719107	53.80%	5.120%
50	12.128	964	966	968 rVB	235433	221586	6.93%	0.660%
51	12.254	975	977	978 rBV	281165	343483	10.75%	1.023%
52	12.288	978	980	982 rVV	2531718	2703785	84.61%	8.052%
53	12.345	982	985	987 rVB2	141742	271537	8.50%	0.809%
54	12.517	998	1000	1002 rVB2	48238	51114	1.60%	0.152%
55	12.562	1002	1004	1007 rBV	370804	376228	11.77%	1.120%
56	12.642	1007	1011	1013 rVV3	31621	56685	1.77%	0.169%
57	12.734	1017	1019	1023 rVV3	64267	108227	3.39%	0.322%
58	12.802	1023	1025	1029 rVV4	84408	117781	3.69%	0.351%
59	12.882	1029	1032	1033 rVV	80367	93330	2.92%	0.278%
60	12.928	1033	1036	1038 rVV2	96745	190646	5.97%	0.568%
61	13.008	1041	1043	1044 rVV	216386	302802	9.48%	0.902%
62	13.031	1044	1045	1048 rVV2	120867	183058	5.73%	0.545%
63	13.122	1051	1053	1054 rVV	35441	45485	1.42%	0.135%
64	13.145	1054	1055	1059 rVV2	62250	81372	2.55%	0.242%
65	13.214	1059	1061	1063 rVV	49641	60475	1.89%	0.180%
66	13.271	1063	1066	1069 rVB2	276047	316706	9.91%	0.943%
67	13.557	1088	1091	1093 rVB	37467	43055	1.35%	0.128%
68	13.637	1096	1098	1104 rBV	66381	123925	3.88%	0.369%
69	13.739	1104	1107	1109 rVV	572513	639125	20.00%	1.903%
70	13.911	1116	1122	1124 rBV3	50389	111871	3.50%	0.333%
71	13.957	1124	1126	1128 rVV2	28511	36345	1.14%	0.108%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF123114\
 Data File : BF076717.D
 Acq On : 31 Dec 2014 23:37
 Operator : IZ / TP
 Sample : F5249-01
 Misc : W
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RWB4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121714.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	14.002	1128	1130	1133	rVV	376167	407504	12.75%	1.214%
73	14.082	1135	1137	1143	rVB2	15484	39650	1.24%	0.118%
74	14.208	1143	1148	1149	rBV4	35827	89747	2.81%	0.267%
75	14.242	1149	1151	1153	rVV	1391963	1355109	42.41%	4.036%
76	14.334	1157	1159	1161	rVB	80521	81577	2.55%	0.243%
77	14.402	1161	1165	1169	rVB2	21563	42255	1.32%	0.126%
78	14.905	1202	1209	1211	rBV4	19393	58664	1.84%	0.175%
79	15.042	1219	1221	1223	rBV	26737	34211	1.07%	0.102%
80	15.443	1253	1256	1258	rBV2	157928	286217	8.96%	0.852%
81	15.488	1258	1260	1265	rVB	368079	441029	13.80%	1.313%
82	15.854	1289	1292	1294	rVB	49816	71002	2.22%	0.211%
83	15.900	1294	1296	1301	rBV	29005	36695	1.15%	0.109%
84	16.231	1322	1325	1330	rBV	67488	84221	2.64%	0.251%
85	16.608	1355	1358	1361	rVV	56073	65634	2.05%	0.195%
86	16.665	1361	1363	1366	rVB	61348	80755	2.53%	0.240%
87	16.974	1387	1390	1392	rBV	53876	70559	2.21%	0.210%
88	17.134	1401	1404	1407	rBV	325725	356419	11.15%	1.061%
89	17.340	1419	1422	1426	rBV	50796	69857	2.19%	0.208%
90	17.706	1451	1454	1456	rBV	41009	66173	2.07%	0.197%
91	18.014	1478	1481	1483	rBV	32238	49826	1.56%	0.148%
92	18.071	1483	1486	1491	rVB2	27526	55545	1.74%	0.165%
93	18.734	1537	1544	1549	rBV6	51194	134809	4.22%	0.401%
94	18.814	1549	1551	1555	rVB4	18638	41896	1.31%	0.125%
95	19.157	1577	1581	1586	rVB6	20999	54608	1.71%	0.163%
96	20.403	1687	1690	1694	rBV5	14365	34369	1.08%	0.102%
97	21.134	1748	1754	1759	rVB3	50578	152757	4.78%	0.455%


Sum of corrected areas: 33579246

Data Path : Z:\HPCHEM1\BNA F\DATA\BF123114\
Data File : BF076717.D
Acq On : 31 Dec 2014 23:37
Operator : IZ / TP
Sample : F5249-01
Misc : W
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RWB4

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121714.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

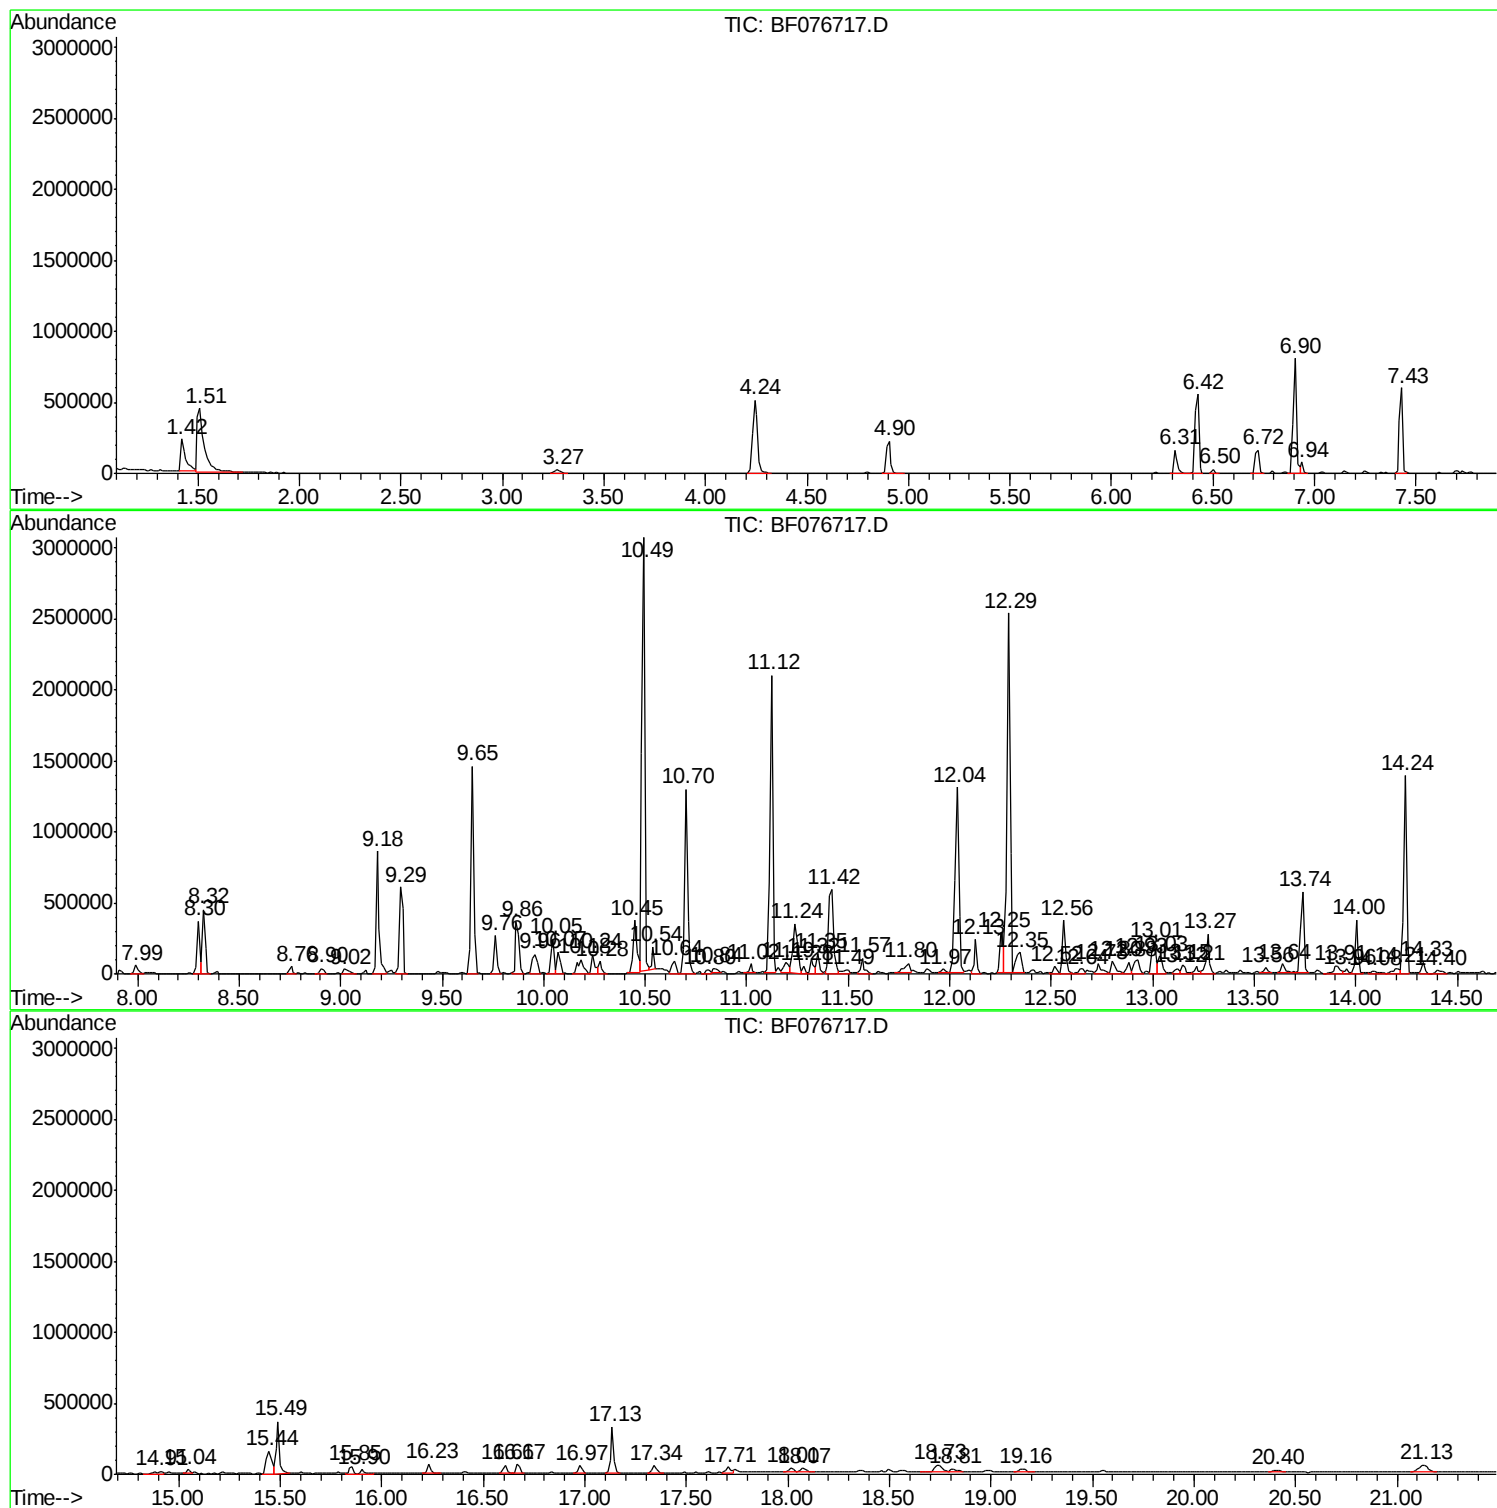

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF123114\
Data_File : BF076717.D
Acq_On : 31-Dec-2014 23:377
Operator : IZ_/ TPP
Sample : F5249-011
Misc : WW
ALS_Vial : 19 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
RWB4

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121714.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
