
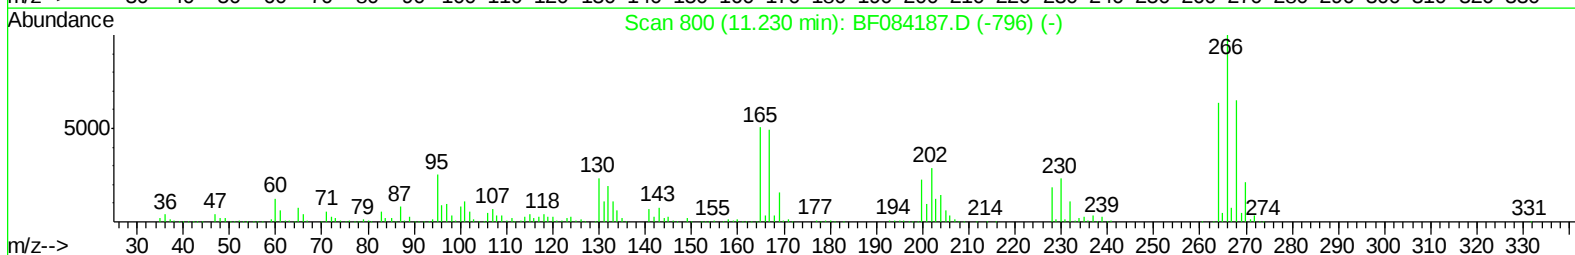
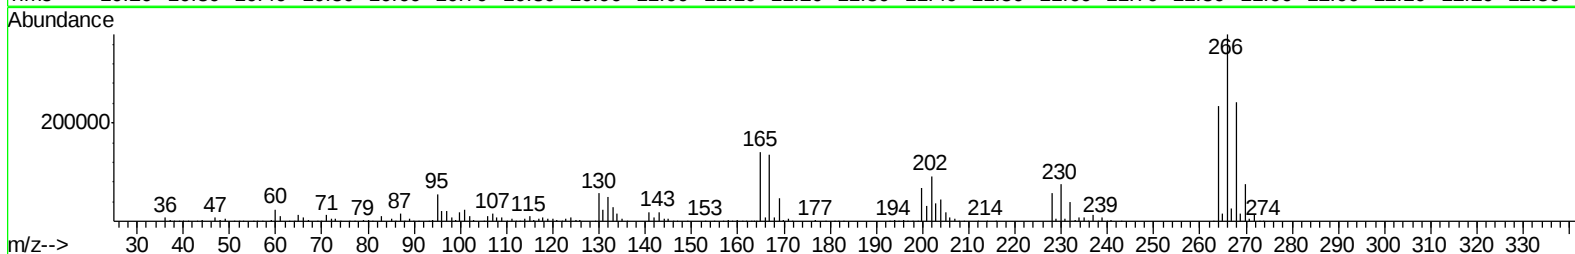


Data Path : Z:\HPCHEM1\BNA F\DATA\BF123115\  
Data File : BF084183.D  
Acq On : 31 Dec 2015 8:52  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 19:02:27 2015  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Dec 31 14:15:57 2015  
Response via : Initial Calibration

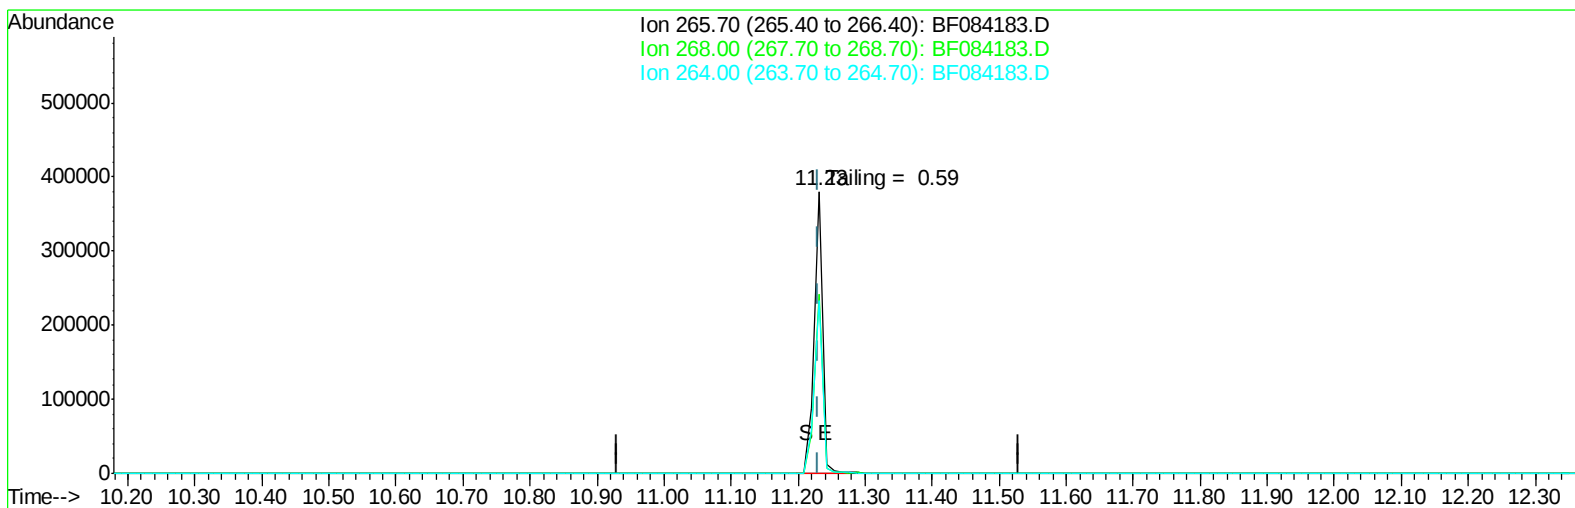

TIC: BF084183.D

(69) Pentachlorophenol (C)




11.231min (+0.001) 18628.88ng

response 337357

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.50 | 63.77 |
| 264.00 | 62.70 | 61.45 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\DATA\BF123115\  
 Data File : BF084183.D  
 Acq On : 31 Dec 2015 8:52  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 19:02:27 2015  
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Dec 31 14:15:57 2015  
 Response via : Initial Calibration

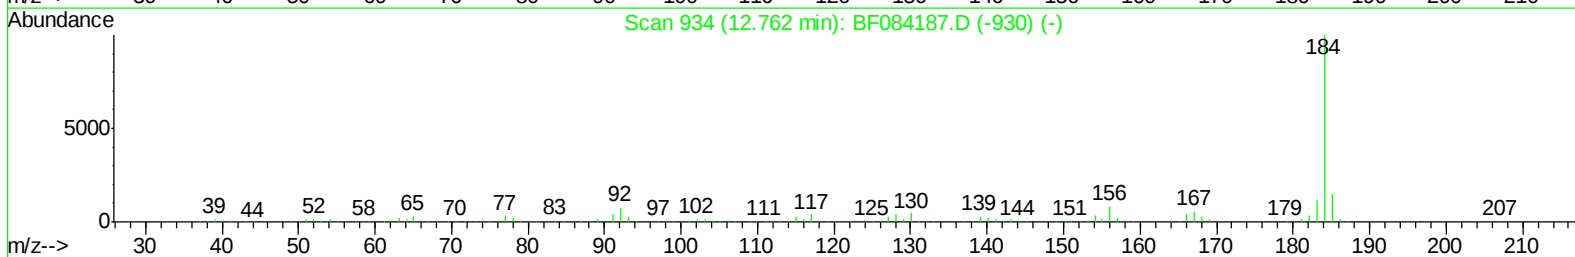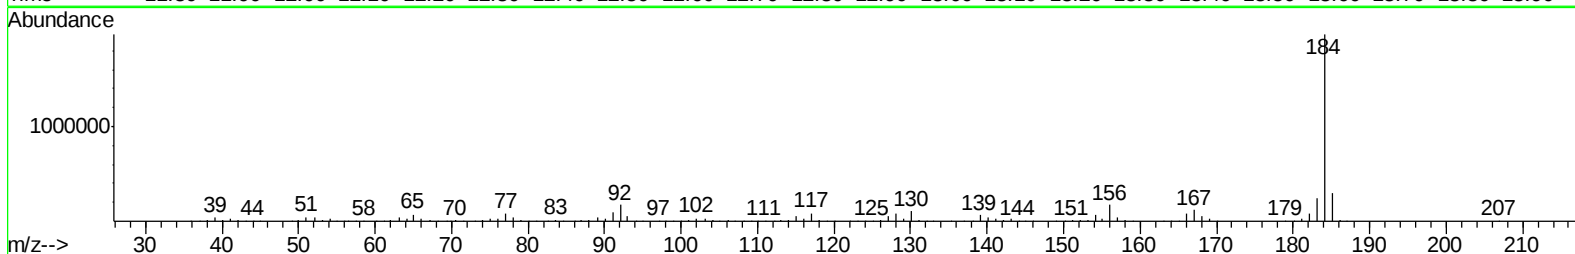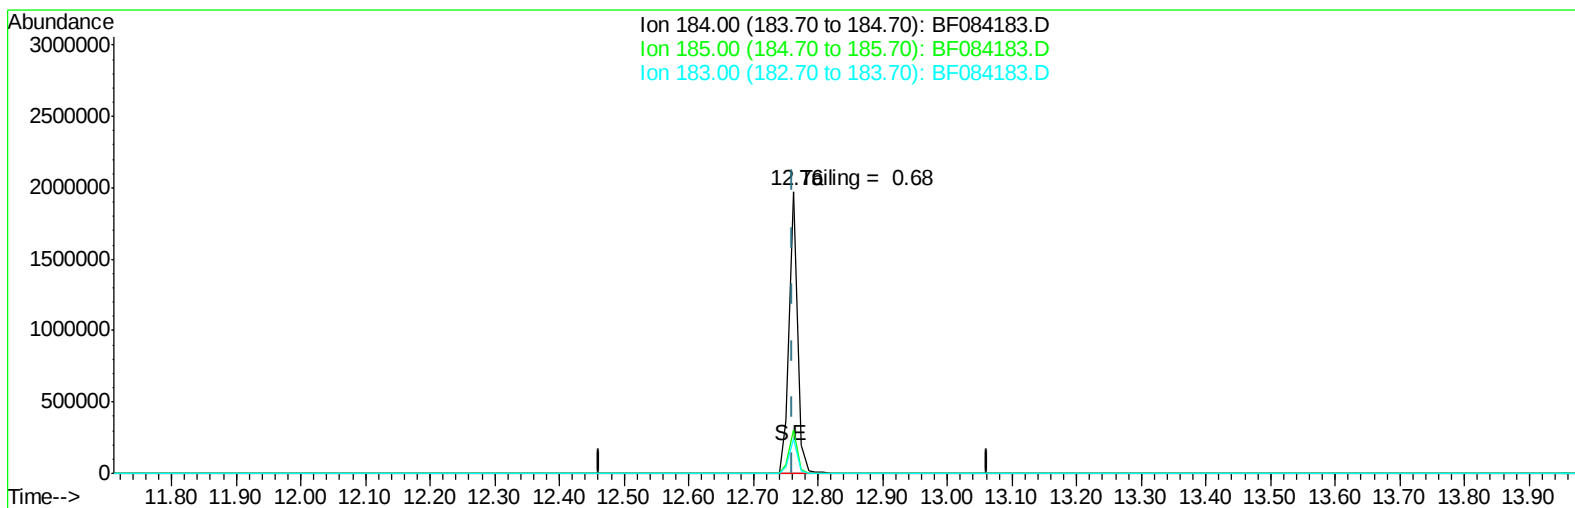

TIC: BF084183.D

(76) Benzidine

12.762min (+0.000) 16628.27ng

response 1785045

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.20 | 15.29 |
| 183.00 | 12.30 | 12.21 |
| 0.00   | 0.00  | 0.00  |