
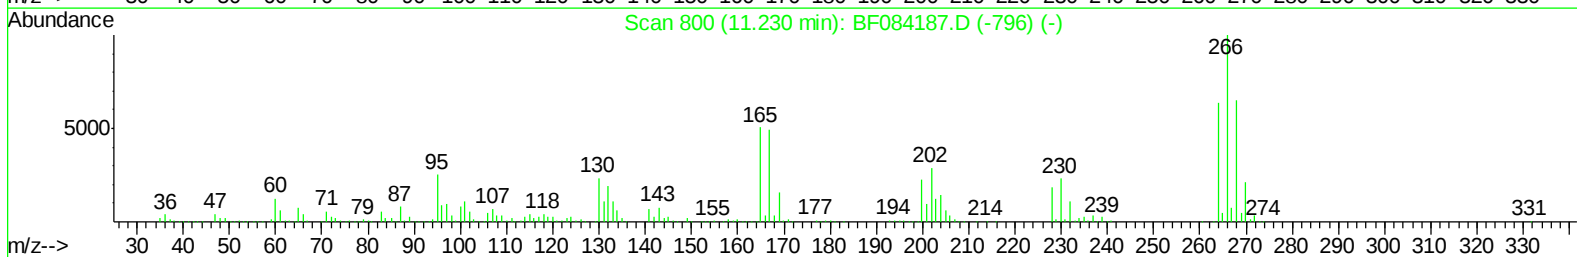
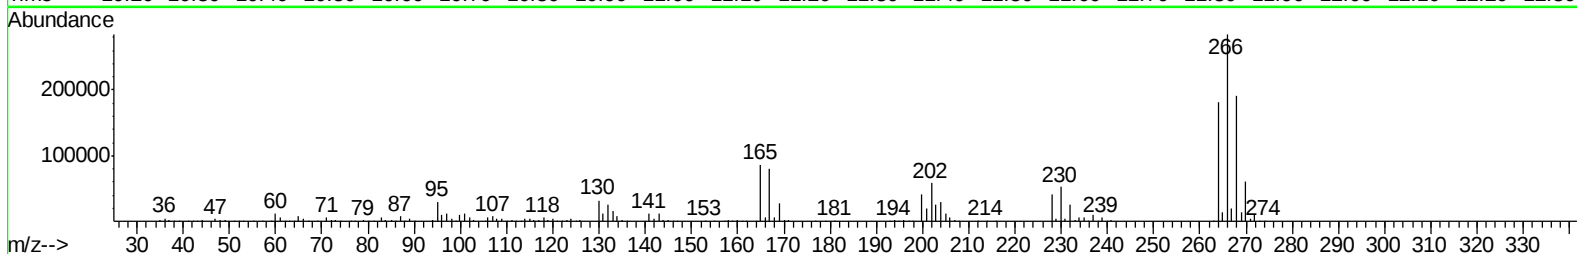


Data Path : Z:\HPCHEM1\BNA_F\Data\BF123115\
Data File : BF084207.D
Acq On : 31 Dec 2015 20:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 00:43:21 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 31 14:15:57 2015
Response via : Initial Calibration

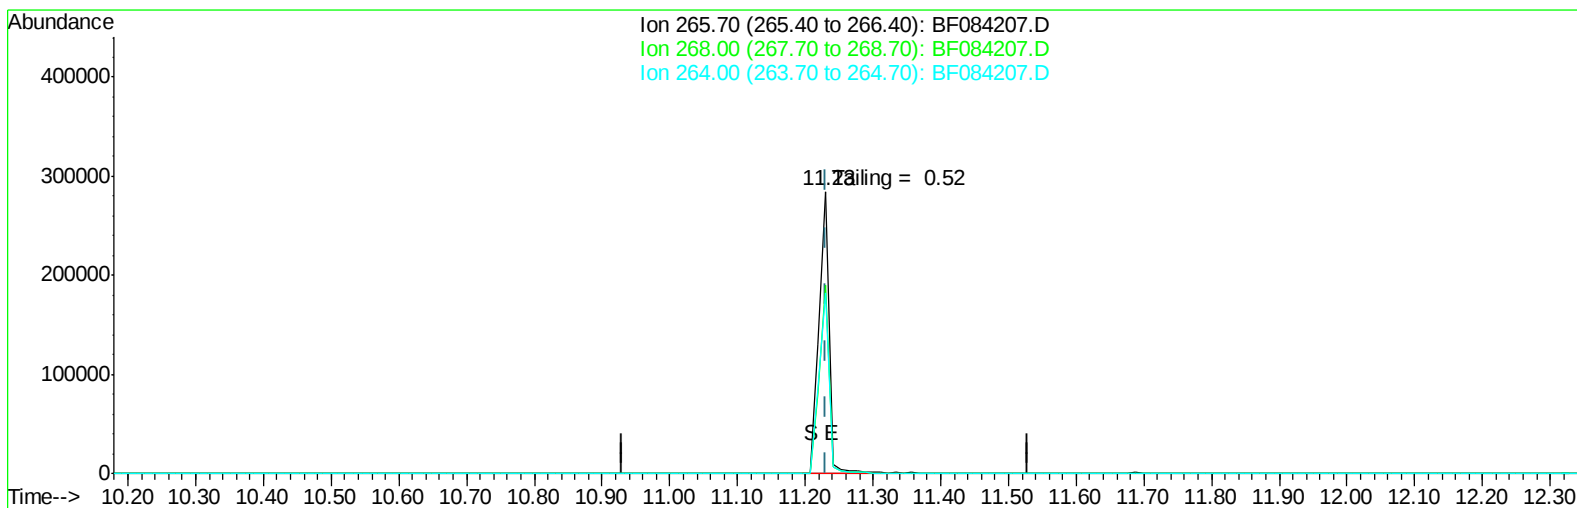

TIC: BF084207.D

(69) Pentachlorophenol (C)




11.231min (+0.001) 21718.83ng

response 300272

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	66.91
264.00	62.70	64.03
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF123115\
Data File : BF084207.D
Acq On : 31 Dec 2015 20:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 00:43:21 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 31 14:15:57 2015
Response via : Initial Calibration

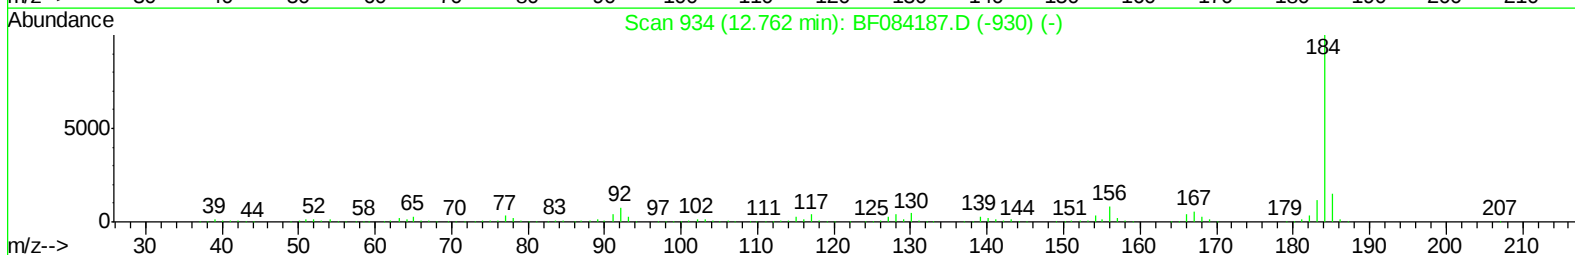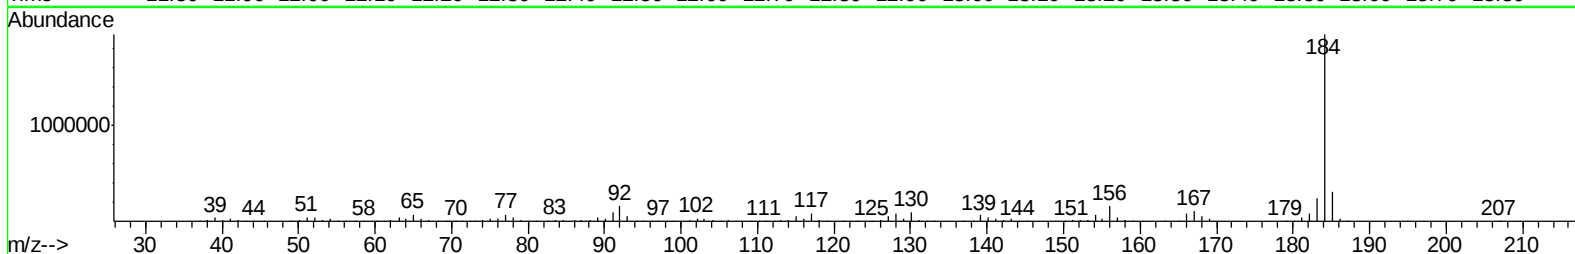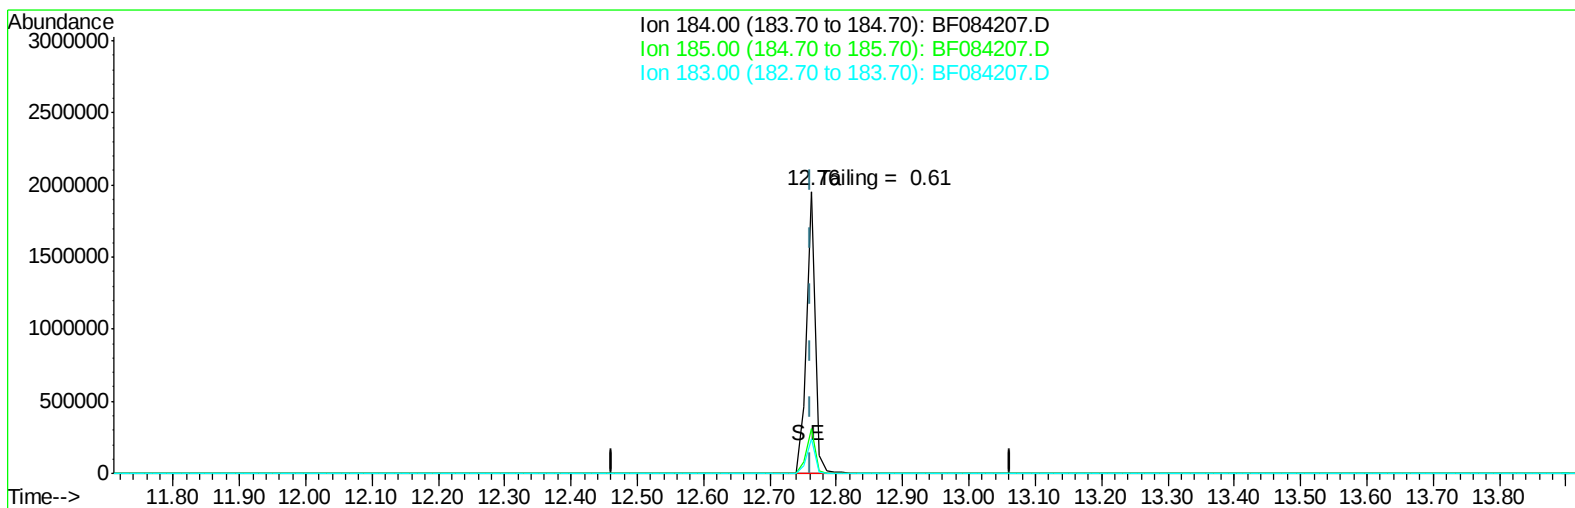

TIC: BF084207.D

(76) Benzidine

12.762min (+0.000) 28022.56ng

response 1781422

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.90
183.00	12.30	12.44
0.00	0.00	0.00