

Data Path : Z:\HPCHEM1\BNA F\DATA\BF123115\
 Data File : BF084192.D
 Acq On : 31 Dec 2015 14:01
 Operator : UM/SJ
 Sample : PB87600BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB87600BL

Quant Time: Jan 02 04:04:29 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 31 14:15:57 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	300335	20.00	ng	0.00
21) Naphthalene-d8	8.18	136	1201869	20.00	ng	-0.01
38) Acenaphthene-d10	9.94	164	572044	20.00	ng	-0.01
63) Phenanthrene-d10	11.42	188	1116125	20.00	ng	0.00
75) Chrysene-d12	14.05	240	810278	20.00	ng	-0.01
86) Perylene-d12	15.49	264	615165	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	1815603	97.78	ng	0.01
7) Phenol-d6	6.52	99	2369556	101.61	ng	-0.01
23) Nitrobenzene-d5	7.46	82	1438437	66.61	ng	-0.01
41) 2,4,6-Tribromophenol	10.73	330	584667	101.24	ng	-0.01
44) 2-Fluorobiphenyl	9.26	172	2553610	78.01	ng	0.00
78) Terphenyl-d14	13.01	244	2408751	66.36	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF123115\
Data File : BF084192.D
Acq On : 31 Dec 2015 14:01
Operator : UM/SJ
Sample : PB87600BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB87600BL

Quant Time: Jan 02 04:04:29 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 31 14:15:57 2015
Response via : Initial Calibration

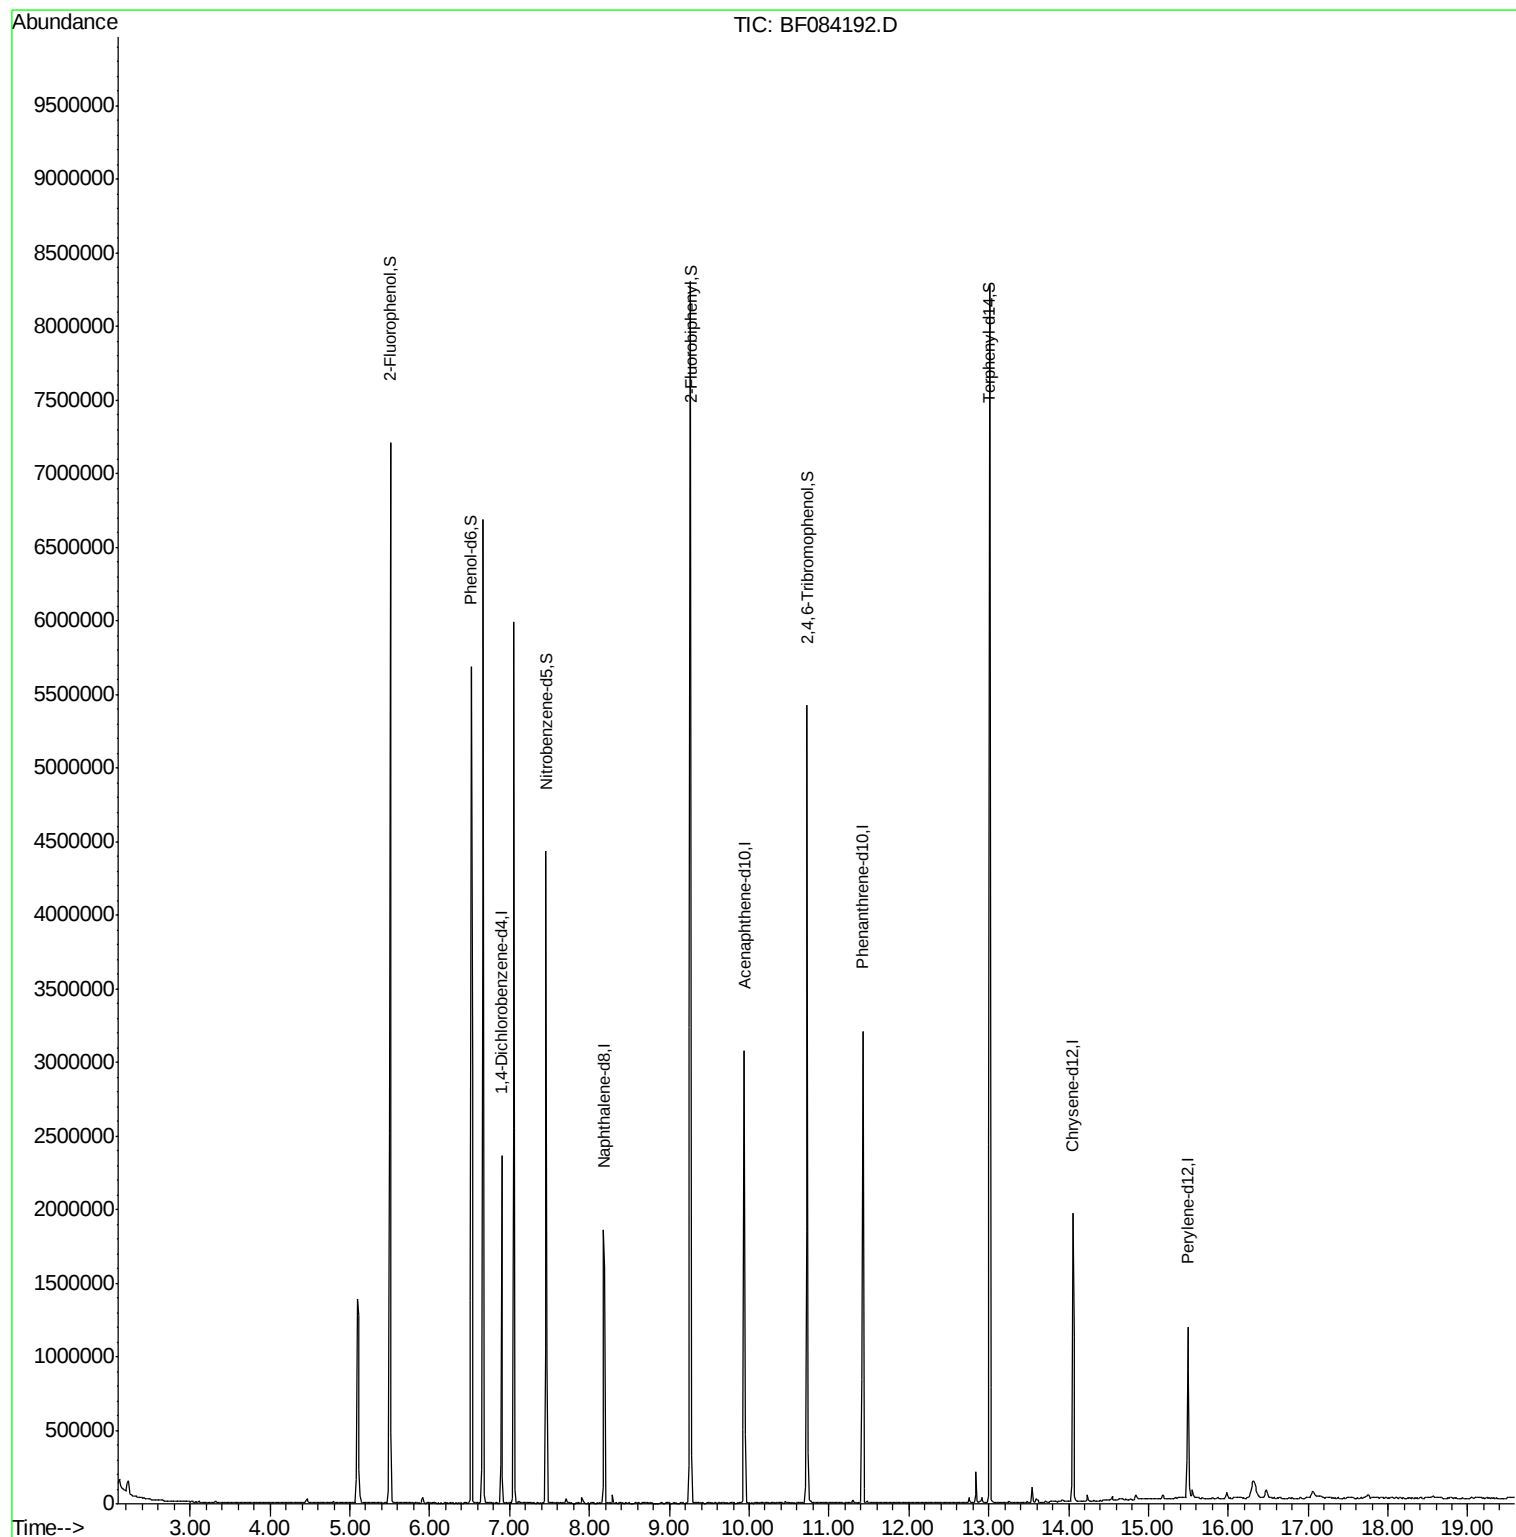



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.90 min Scan# 421

Delta R.T. 0.00 min

Lab File: BF084192.D

Acq: 31 Dec 2015 14:01

Instrument :

BNA_F

ClientSampleId :

PB87600BL


Tot Ion:152 Resp: 300335

Ion Ratio Lower Upper

152 100

150 154.3 123.0 184.4




115 68.8 51.4 77.2

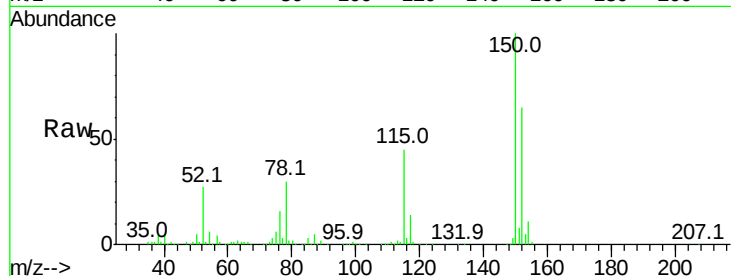

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

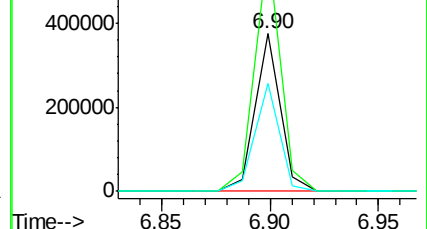

#5

2-Fluorophenol

Concen: 97.78 ng

RT: 5.50 min Scan# 299

Delta R.T. 0.01 min

Lab File: BF084192.D

Acq: 31 Dec 2015 14:01


Tgt Ion:112 Resp: 1815603

Ion Ratio Lower Upper

112 100

64 69.1 36.6 55.0#



63 37.0 19.4 29.0#




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

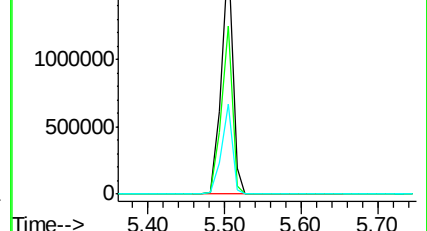

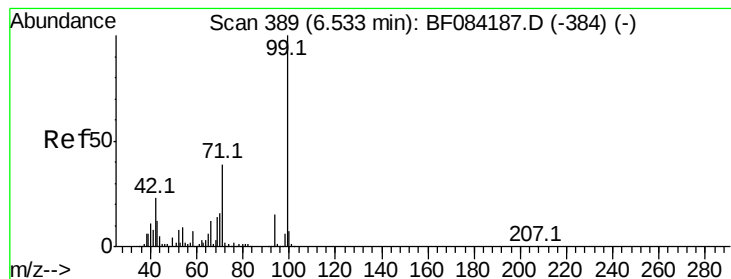

#7

Phenol-d6

Concen: 101.61 ng

RT: 6.52 min Scan# 388

Delta R.T. -0.01 min

Lab File: BF084192.D

Acq: 31 Dec 2015 14:01

Instrument :

BNA_F

ClientSampleId :

PB87600BL





Tot Ion: 99 Resp: 2369556

Ion Ratio Lower Upper

99 100

42 24.9 12.8 19.2#

71 40.0 30.9 46.3

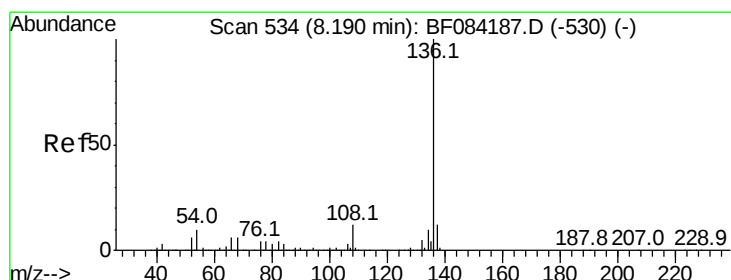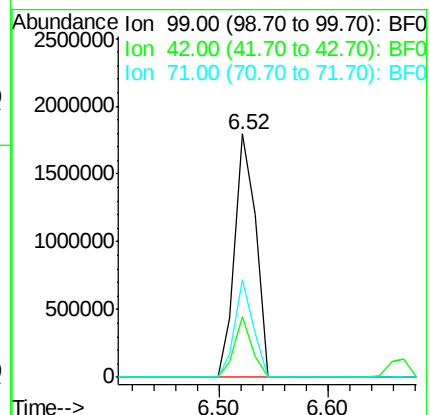

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.18 min Scan# 533

Delta R.T. -0.01 min

Lab File: BF084192.D

Acq: 31 Dec 2015 14:01

Tgt Ion: 136 Resp: 1201869




Ion Ratio Lower Upper


136 100

137 11.8 8.7 13.1

54 12.0 5.8 8.8#

68 6.3 4.2 6.2#



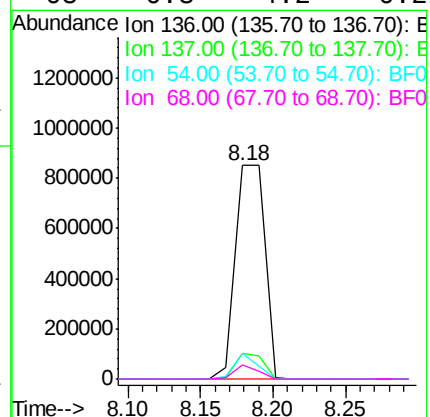



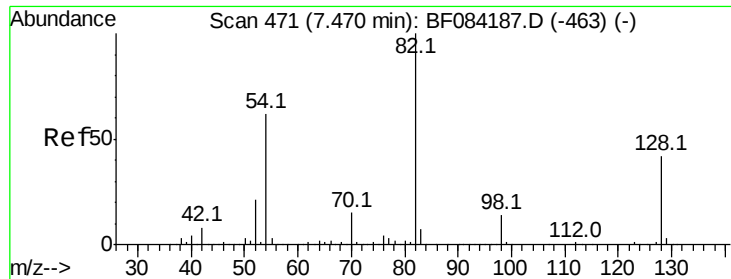

#23
 Nitrobenzene-d5
 Concen: 66.61 ng
 RT: 7.46 min Scan# 470
 Delta R.T. -0.01 min
 Lab File: BF084192.D
 Acq: 31 Dec 2015 14:01




Instrument :
 BNA_F
 ClientSampleId :
 PB87600BL


Tot Ion: 82 Resp: 1438437
 Ion Ratio Lower Upper
 82 100
 128 40.5 34.6 51.8
 54 62.2 38.4 57.6#

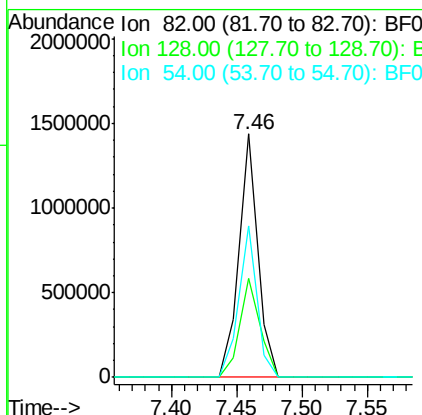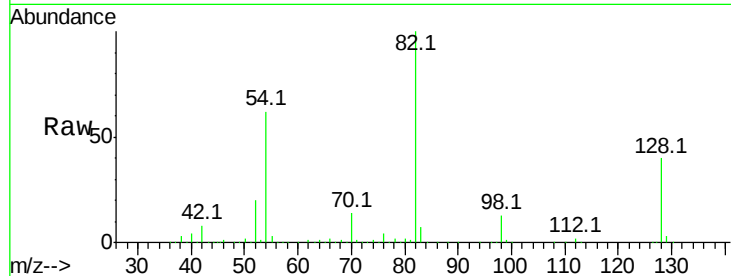

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.94 min Scan# 687
 Delta R.T. -0.01 min
 Lab File: BF084192.D
 Acq: 31 Dec 2015 14:01

Tgt Ion:164 Resp: 572044
 Ion Ratio Lower Upper
 164 100
 162 104.7 85.1 127.7
 160 48.4 37.5 56.3

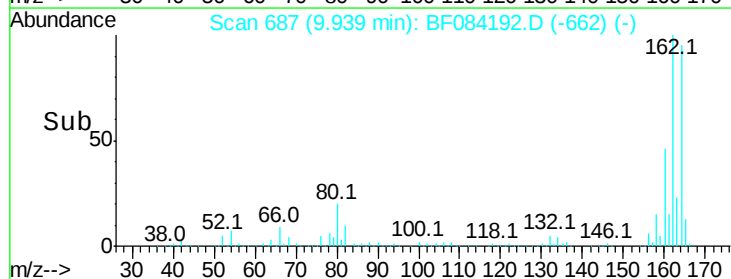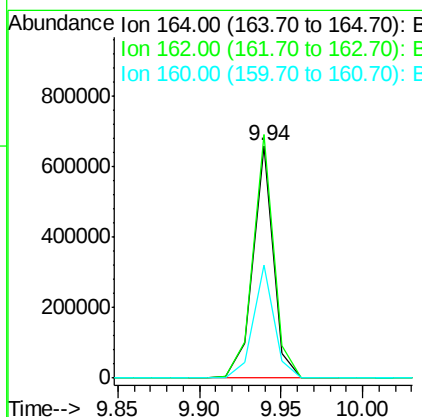


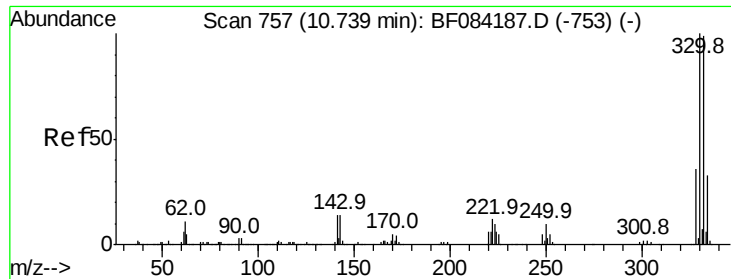




#41
 2,4,6-Tribromophenol
 Concen: 101.24 ng
 RT: 10.73 min Scan# 756
 Delta R.T. -0.01 min
 Lab File: BF084192.D
 Acq: 31 Dec 2015 14:01

Instrument :
 BNA_F
 ClientSampleId :
 PB87600BL

Tot Ion:330 Resp: 584667
 Ion Ratio Lower Upper
 330 100
 332 96.5 76.6 114.8
 141 43.9 27.8 41.6#




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

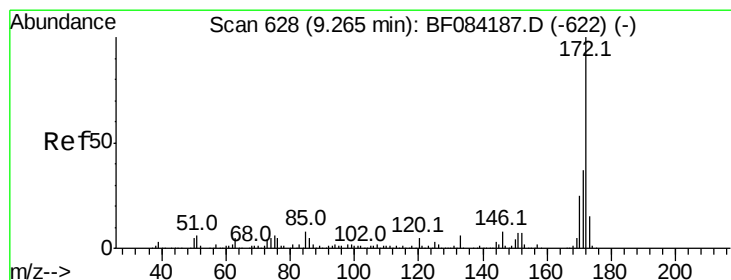
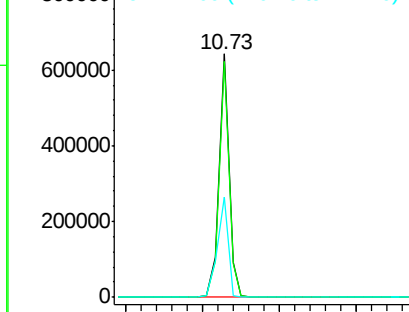



#44
 2-Fluorobiphenyl
 Concen: 78.01 ng
 RT: 9.26 min Scan# 628
 Delta R.T. 0.00 min
 Lab File: BF084192.D
 Acq: 31 Dec 2015 14:01

Tgt Ion:172 Resp: 2553610
 Ion Ratio Lower Upper
 172 100
 171 38.5 28.9 43.3
 170 26.6 18.6 27.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

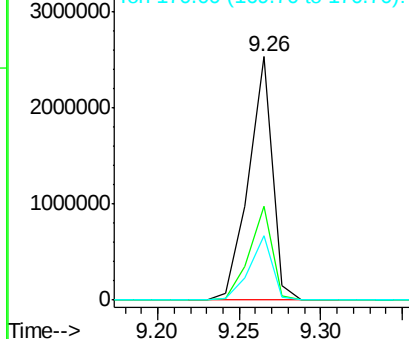


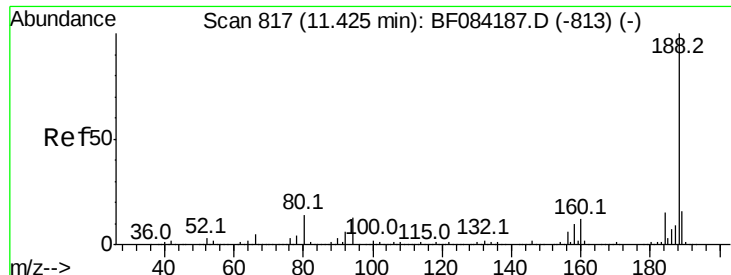




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.42 min Scan# 817
Delta R.T. 0.00 min
Lab File: BF084192.D
Acq: 31 Dec 2015 14:01

Instrument :
BNA_F
ClientSampleId :
PB87600BL

Tot Ion:188 Resp: 1116125
Ion Ratio Lower Upper
188 100
94 8.3 9.0 13.4#
80 8.9 9.6 14.4#

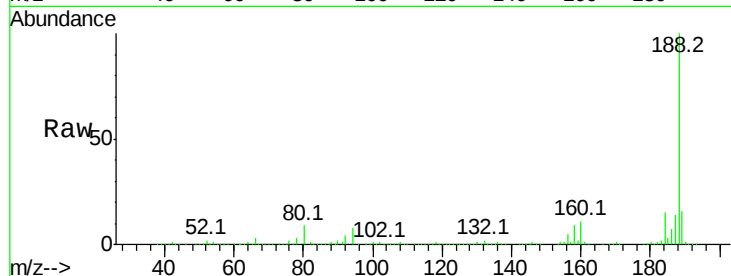


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


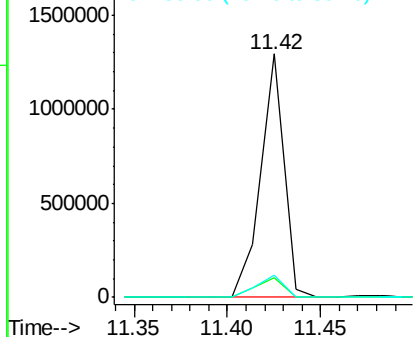



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.05 min Scan# 1047
Delta R.T. -0.01 min
Lab File: BF084192.D
Acq: 31 Dec 2015 14:01

Tgt Ion:240 Resp: 810278
Ion Ratio Lower Upper
240 100
120 16.2 9.5 14.3#
236 25.3 20.6 31.0



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E




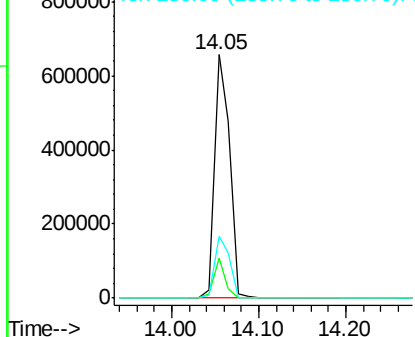


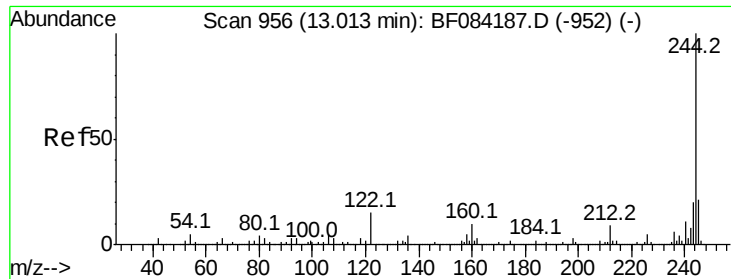

#78
 Terphenyl-d14
 Concen: 66.36 ng
 RT: 13.01 min Scan# 956
 Delta R.T. 0.00 min
 Lab File: BF084192.D
 Acq: 31 Dec 2015 14:01

Instrument :
 BNA_F
 ClientSampleId :
 PB87600BL

Tot Ion:244 Resp: 2408751
 Ion Ratio Lower Upper
 244 100
 212 8.4 5.7 8.5
 122 14.1 7.4 11.0#

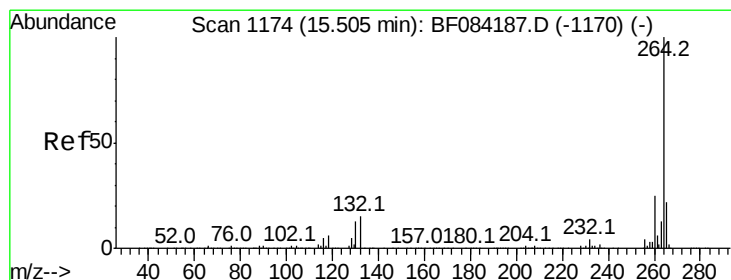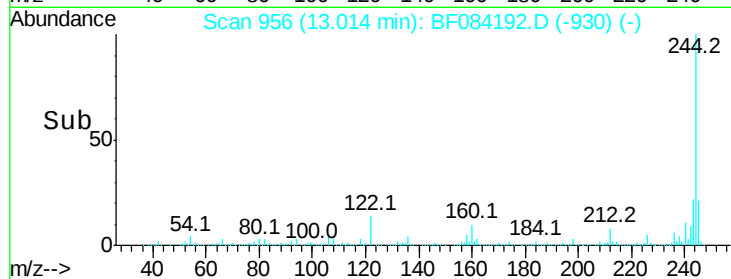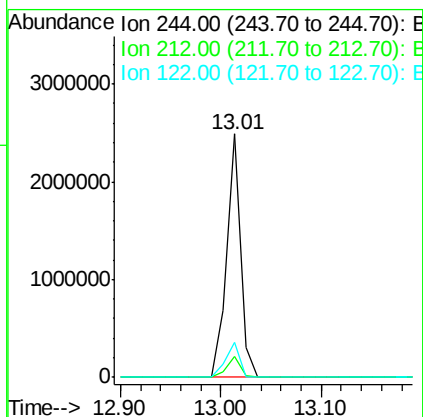

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.49 min Scan# 1173
 Delta R.T. -0.01 min
 Lab File: BF084192.D
 Acq: 31 Dec 2015 14:01

Tgt Ion:264 Resp: 615165
 Ion Ratio Lower Upper
 264 100
 260 23.0 19.4 29.2
 265 21.2 17.8 26.6

