

Data Path : Z:\HPCHEM1\BNA F\DATA\BF123115\
 Data File : BF084221.D
 Acq On : 1 Jan 2016 3:25
 Operator : UM/SJ
 Sample : G4981-04
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S8-0531

Quant Time: Jan 02 02:44:19 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 31 14:15:57 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	280610	20.00	ng	0.00
21) Naphthalene-d8	8.19	136	1183913	20.00	ng	0.00
38) Acenaphthene-d10	9.94	164	492146	20.00	ng	-0.01
63) Phenanthrene-d10	11.43	188	791011	20.00	ng	0.00
75) Chrysene-d12	14.05	240	518023	20.00	ng	-0.01
86) Perylene-d12	15.51	264	539796	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	1033396	59.57	ng	0.01
7) Phenol-d6	6.52	99	729739	33.49	ng	-0.01
23) Nitrobenzene-d5	7.47	82	1976612	92.92	ng	0.00
41) 2,4,6-Tribromophenol	10.73	330	521378	104.93	ng	-0.01
44) 2-Fluorobiphenyl	9.26	172	2593051	93.31	ng	0.00
78) Terphenyl-d14	13.01	244	1829229	78.82	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.65	163	80417	2.29	ng	Qvalue # 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF123115\
Data File : BF084221.D
Acq On : 1 Jan 2016 3:25
Operator : UM/SJ
Sample : G4981-04
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S8-0531

Quant Time: Jan 02 02:44:19 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 31 14:15:57 2015
Response via : Initial Calibration

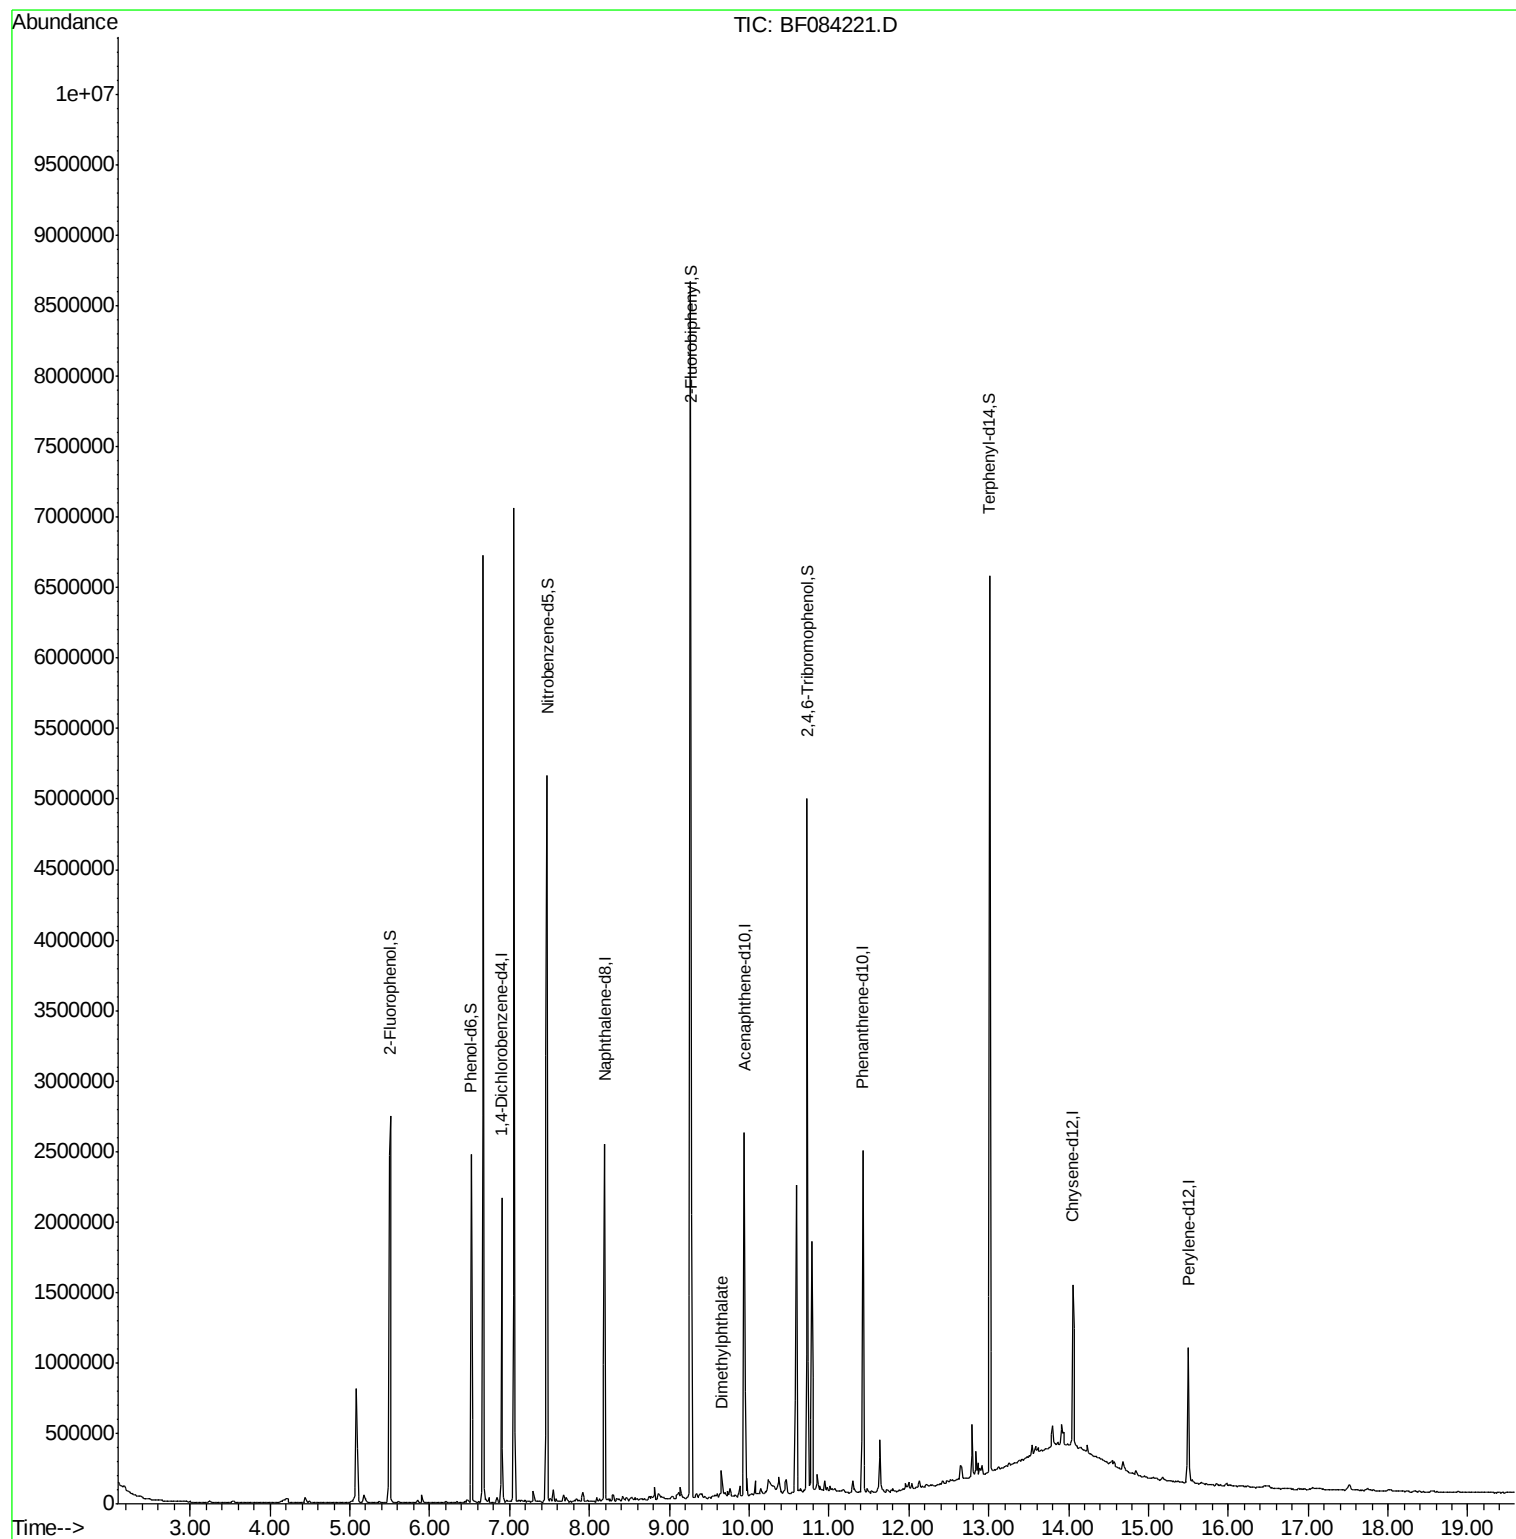

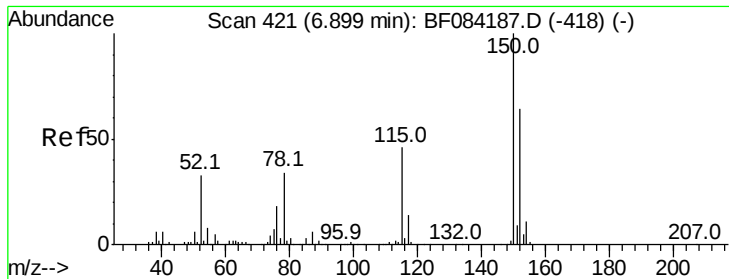


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.90 min Scan# 421
Delta R.T. 0.00 min
Lab File: BF084221.D
Acq: 1 Jan 2016 3:25

Instrument :
BNA_F
ClientSampleId :
S8-0531

Tot Ion:152 Resp: 280610
Ion Ratio Lower Upper
152 100
150 159.5 123.0 184.4
115 71.6 51.4 77.2

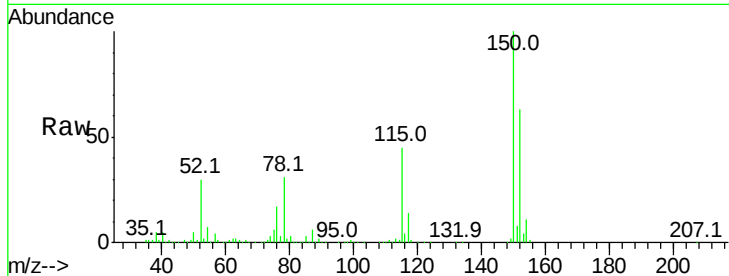


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

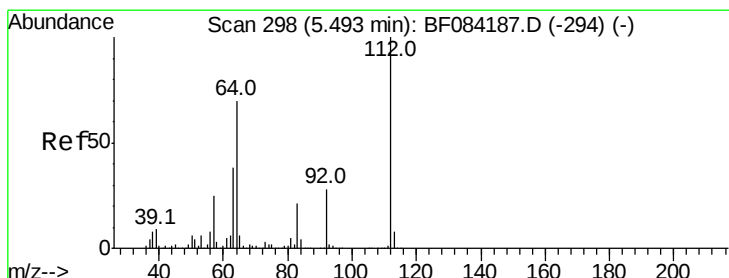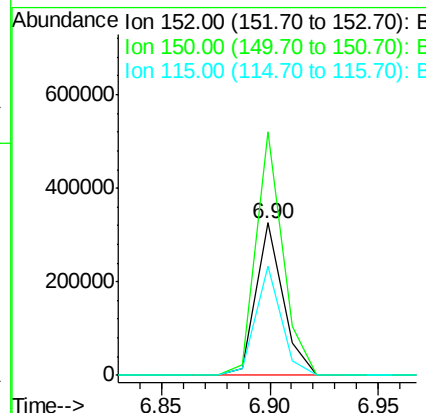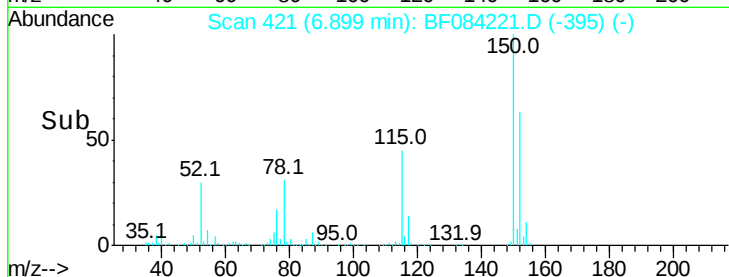



#5


2-Fluorophenol
Concen: 59.57 ng
RT: 5.50 min Scan# 299
Delta R.T. 0.01 min
Lab File: BF084221.D
Acq: 1 Jan 2016 3:25

Tgt Ion:112 Resp: 1033396
Ion Ratio Lower Upper
112 100
64 51.2 36.6 55.0
63 26.9 19.4 29.0

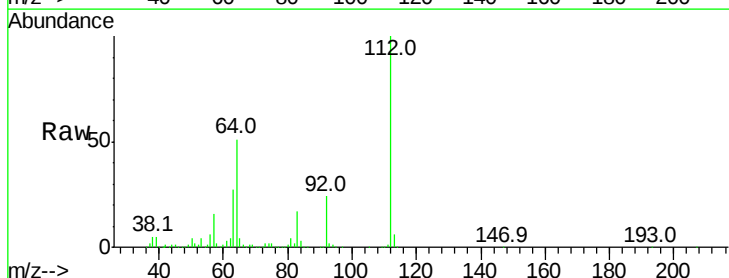

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

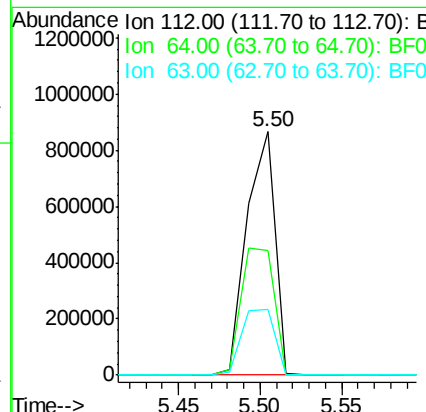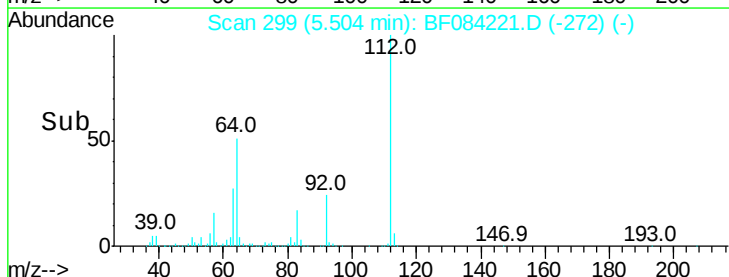

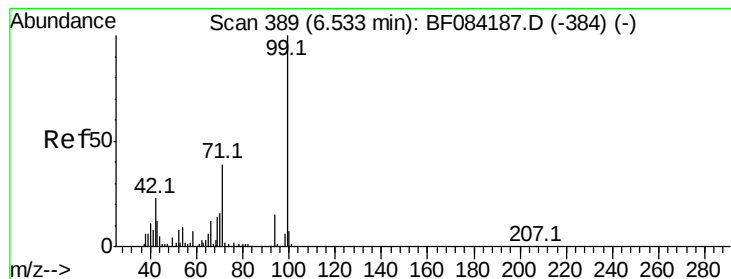

#7

Phenol-d6

Concen: 33.49 ng

RT: 6.52 min Scan# 388

Delta R.T. -0.01 min

Lab File: BF084221.D

Acq: 1 Jan 2016 3:25

Instrument :

BNA_F

ClientSampled :

S8-0531


Tot Ion: 99 Resp: 729739

Ion Ratio Lower Upper

99 100

42 24.2 12.8 19.2#




71 37.2 30.9 46.3

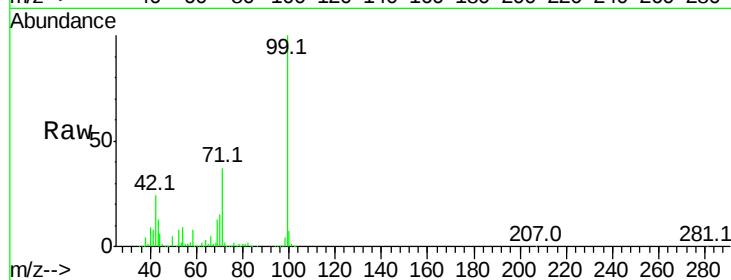

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

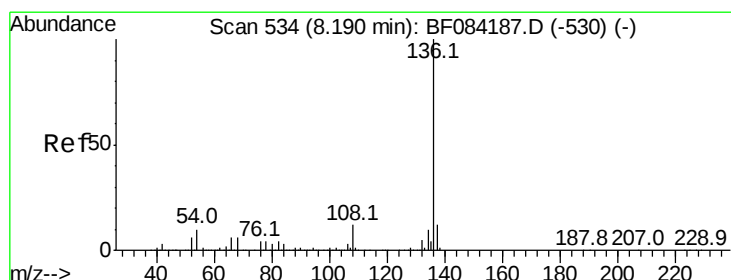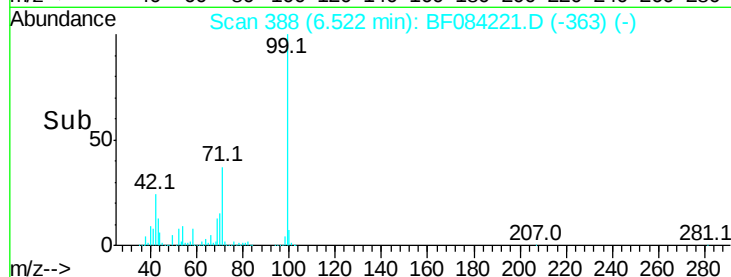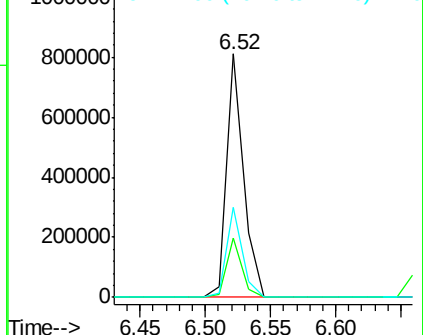

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.19 min Scan# 534

Delta R.T. 0.00 min

Lab File: BF084221.D

Acq: 1 Jan 2016 3:25

Tgt Ion:136 Resp: 1183913


Ion Ratio Lower Upper

136 100

137 11.1 8.7 13.1

54 7.6 5.8 8.8

68 4.7 4.2 6.2


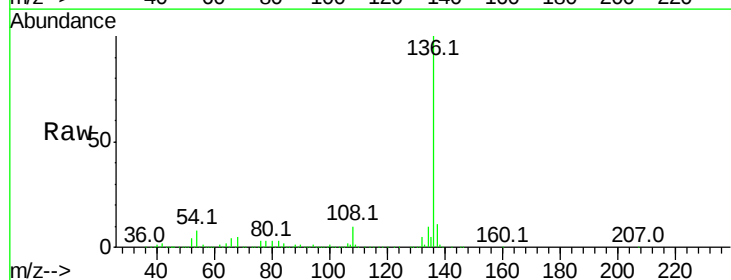



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



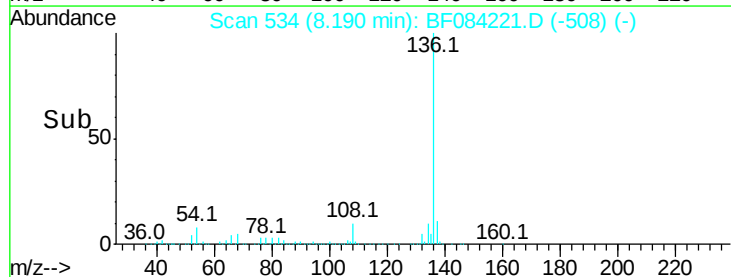
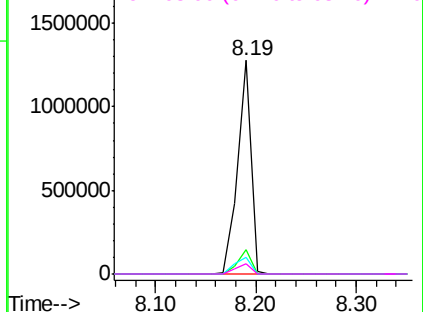


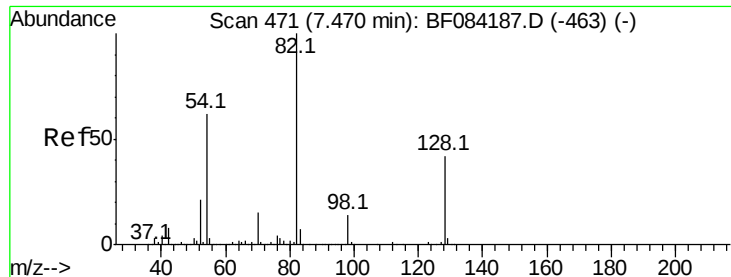

#23
Nitrobenzene-d5
Concen: 92.92 ng
RT: 7.47 min Scan# 471
Delta R.T. 0.00 min
Lab File: BF084221.D
Acq: 1 Jan 2016 3:25




Instrument :
BNA_F
ClientSampled :
S8-0531


Tot Ion: 82 Resp: 1976612
Ion Ratio Lower Upper
82 100
128 47.3 34.6 51.8
54 55.3 38.4 57.6

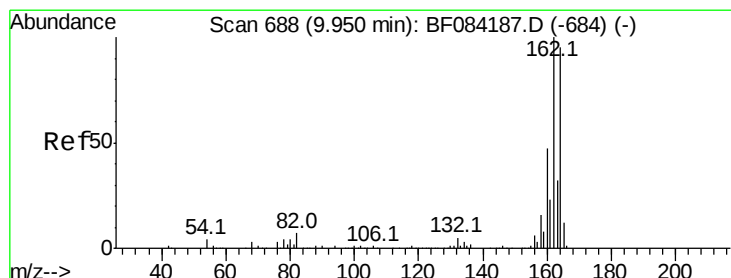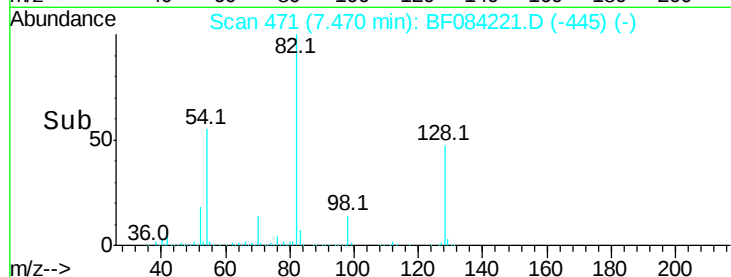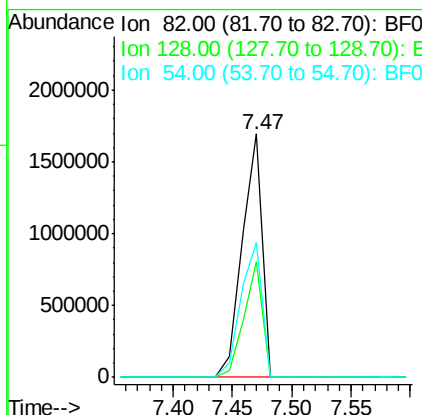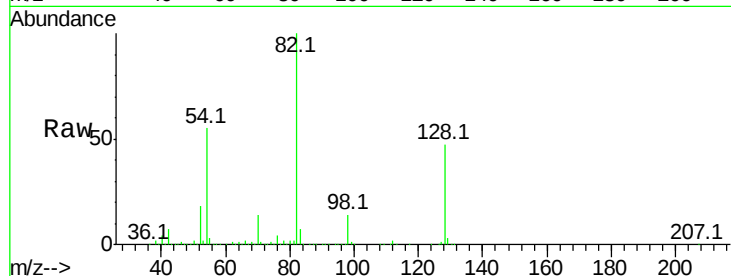

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.94 min Scan# 687
Delta R.T. -0.01 min
Lab File: BF084221.D
Acq: 1 Jan 2016 3:25

Tgt Ion:164 Resp: 492146
Ion Ratio Lower Upper
164 100
162 103.5 85.1 127.7
160 47.2 37.5 56.3

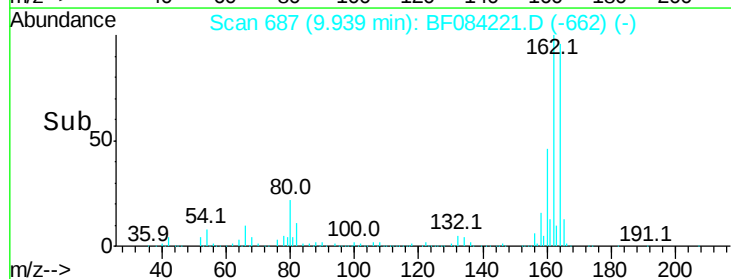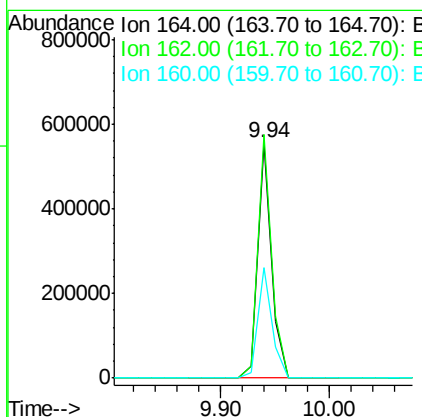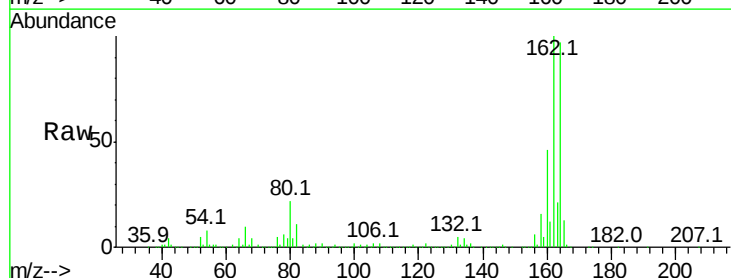

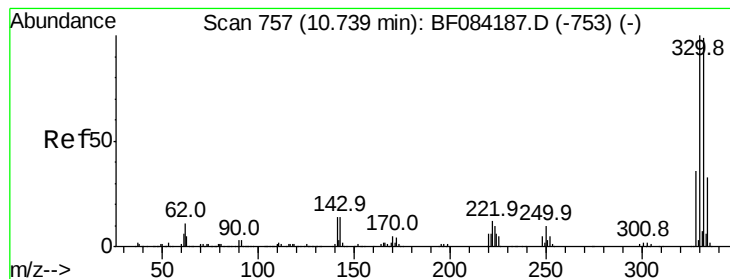

#41

2,4,6-Tribromophenol

Concen: 104.93 ng

RT: 10.73 min Scan# 756

Delta R.T. -0.01 min

Lab File: BF084221.D

Acq: 1 Jan 2016 3:25

Instrument :

BNA_F

ClientSampleId :

S8-0531


Tot Ion:330 Resp: 521378

Ion Ratio Lower Upper




330 100

332 97.9 76.6 114.8

141 40.9 27.8 41.6

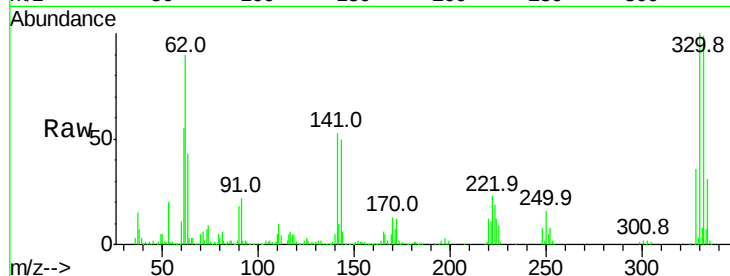

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

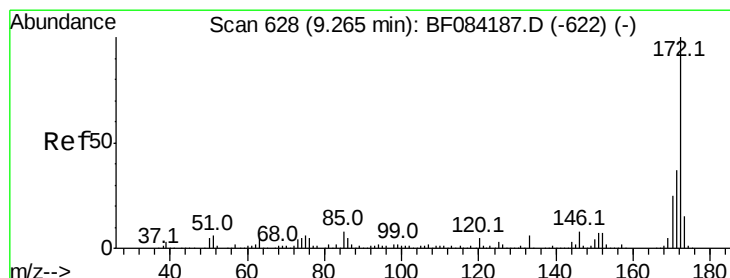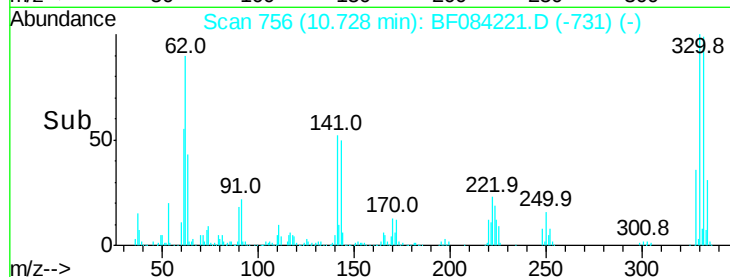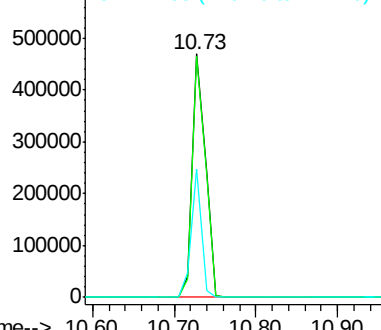

#44

2-Fluorobiphenyl

Concen: 93.31 ng

RT: 9.26 min Scan# 628

Delta R.T. 0.00 min

Lab File: BF084221.D

Acq: 1 Jan 2016 3:25


Tgt Ion:172 Resp: 2593051

Ion Ratio Lower Upper



172 100


171 38.2 28.9 43.3

170 26.4 18.6 27.8

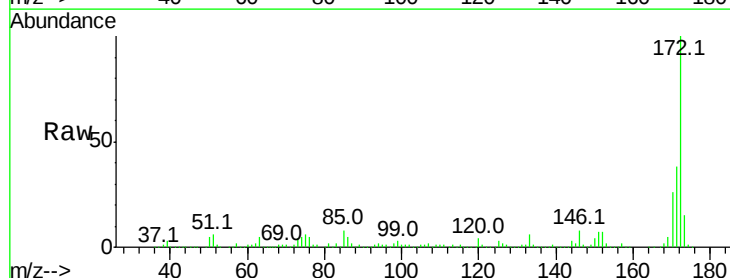

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

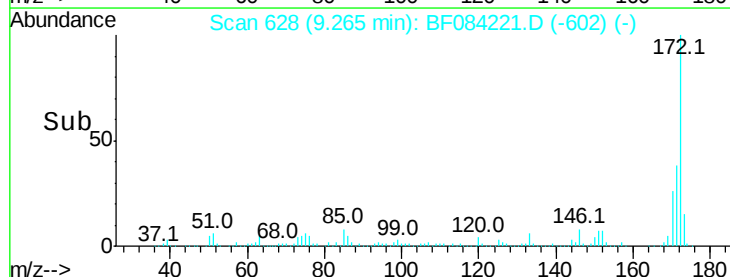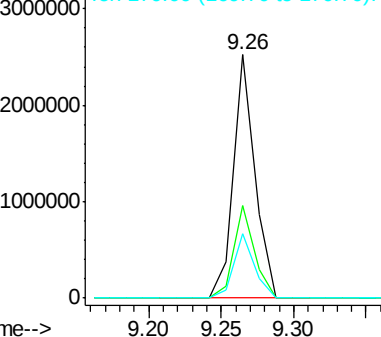

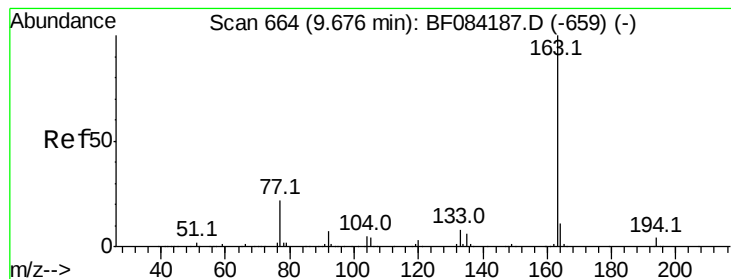

#49

Dimethylphthalate

Concen: 2.29 ng

RT: 9.65 min Scan# 662

Delta R.T. -0.02 min

Lab File: BF084221.D

Acq: 1 Jan 2016 3:25

Instrument :

BNA_F

ClientSampleId :

S8-0531


Tot Ion:163 Resp: 80417

Ion Ratio Lower Upper

163 100

194 3.4 8.0 12.0#




164 10.7 8.0 12.0

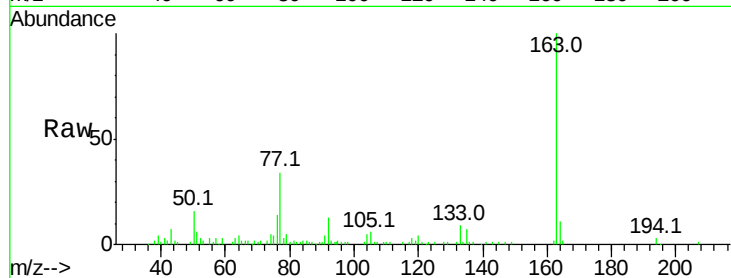

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

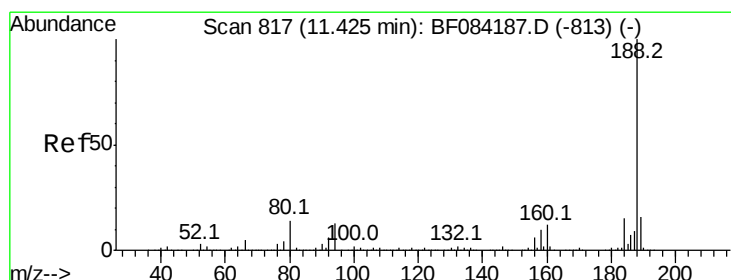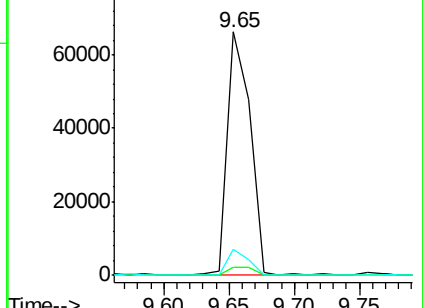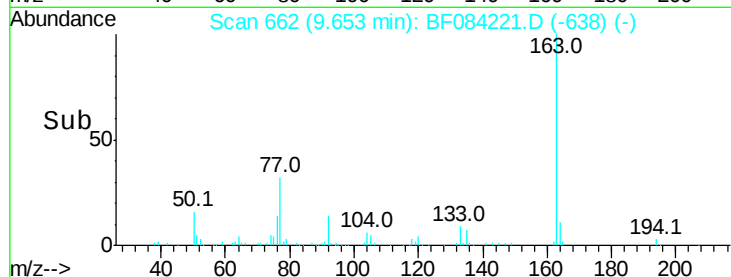

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.43 min Scan# 817

Delta R.T. 0.00 min

Lab File: BF084221.D

Acq: 1 Jan 2016 3:25


Tgt Ion:188 Resp: 791011

Ion Ratio Lower Upper

188 100

94 9.8 9.0 13.4



80 10.0 9.6 14.4

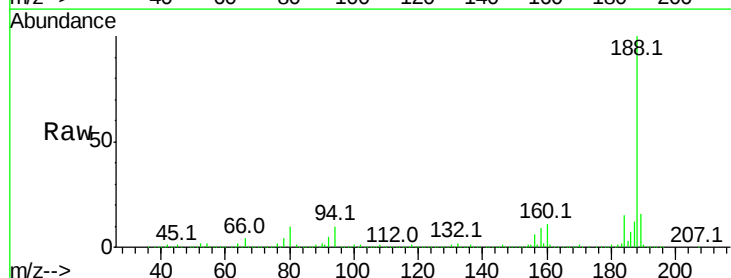


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

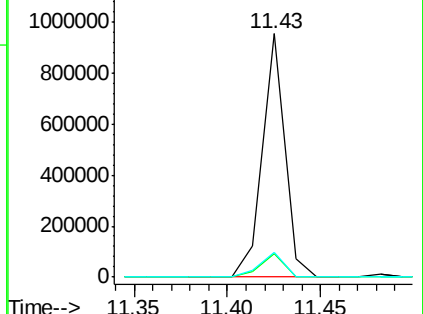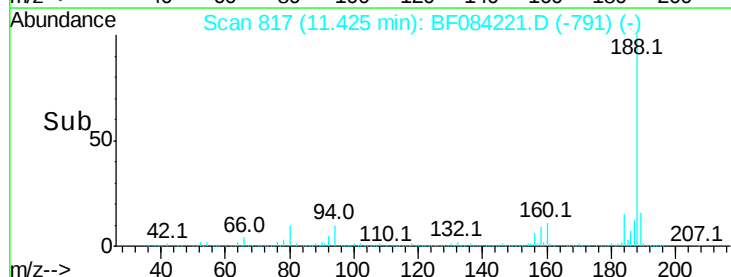

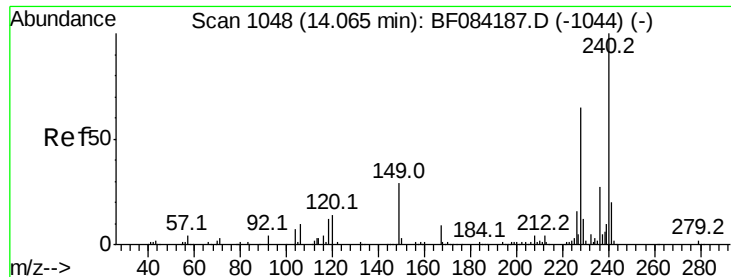

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.05 min Scan# 1047

Delta R.T. -0.01 min

Lab File: BF084221.D

Acq: 1 Jan 2016 3:25

Instrument :

BNA_F

ClientSampleID :

S8-0531


Tot Ion:240 Resp: 518023

Ion Ratio Lower Upper

240 100

120 16.8 9.5 14.3#




236 25.7 20.6 31.0

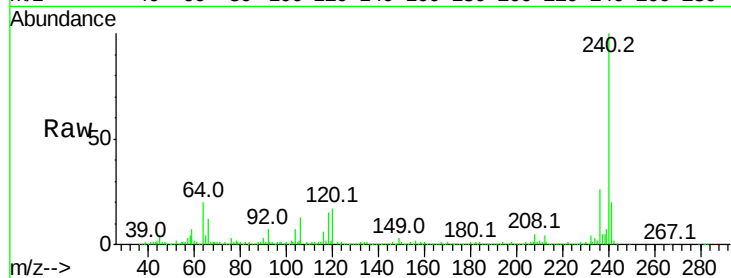

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

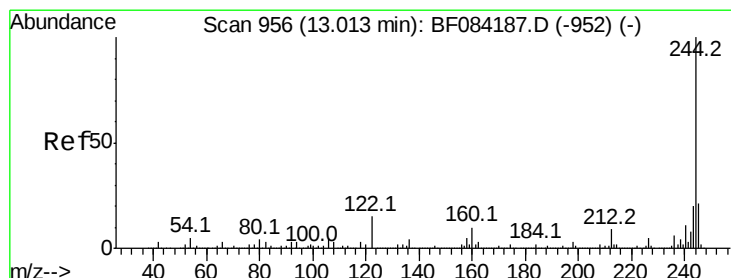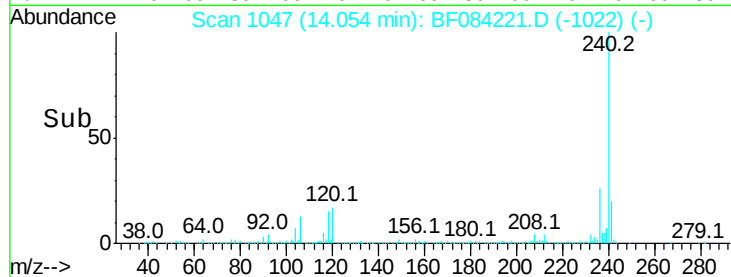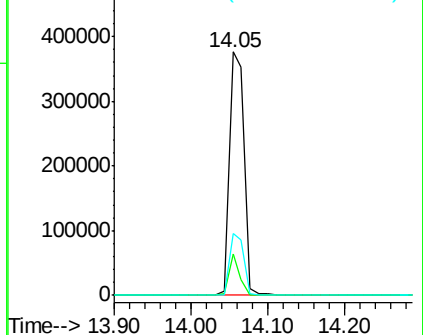

#78

Terphenyl-d14

Concen: 78.82 ng

RT: 13.01 min Scan# 956

Delta R.T. 0.00 min

Lab File: BF084221.D

Acq: 1 Jan 2016 3:25


Tgt Ion:244 Resp: 1829229

Ion Ratio Lower Upper

244 100

212 8.2 5.7 8.5



122 13.6 7.4 11.0#

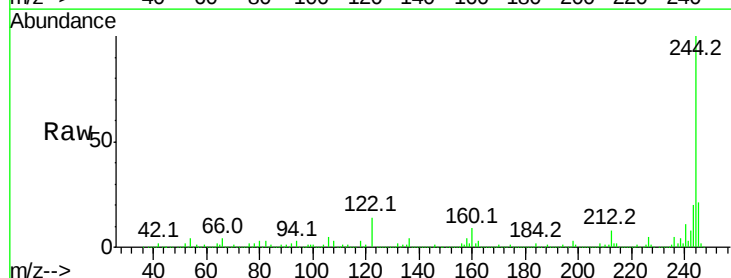


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

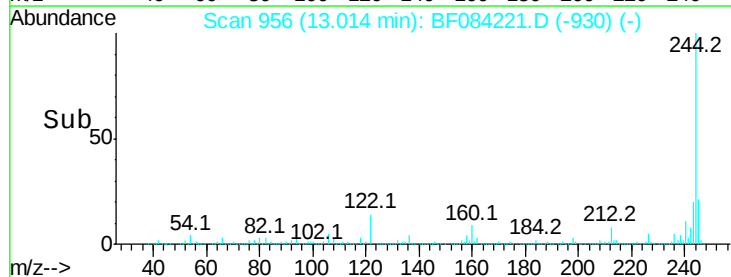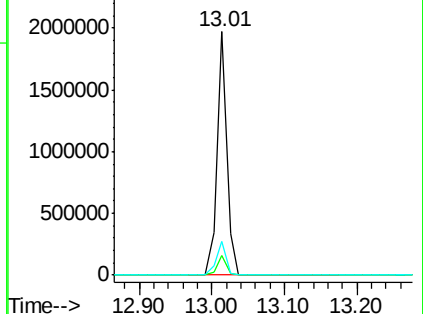

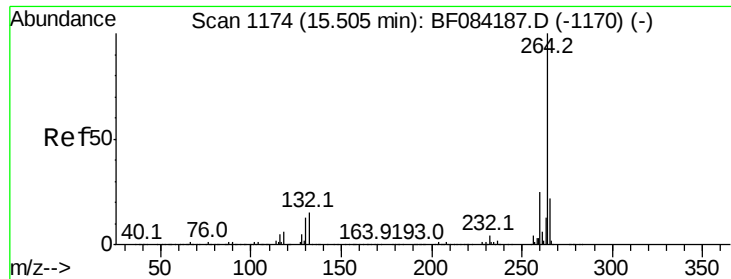

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.51 min Scan# 1174
Delta R.T. 0.00 min
Lab File: BF084221.D
Acq: 1 Jan 2016 3:25

Instrument :
BNA_F
ClientSampleId :
S8-0531

Tot Ion: 264 Resp: 539796

Ion	Ratio	Lower	Upper
264	100		
260	24.1	19.4	29.2
265	20.9	17.8	26.6

