


Data Path : Z:\HPCHEM1\BNA F\Data\BF123115\
 Data File : BF084183.D
 Acq On : 31 Dec 2015 8:52
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 04 12:22:40 2016

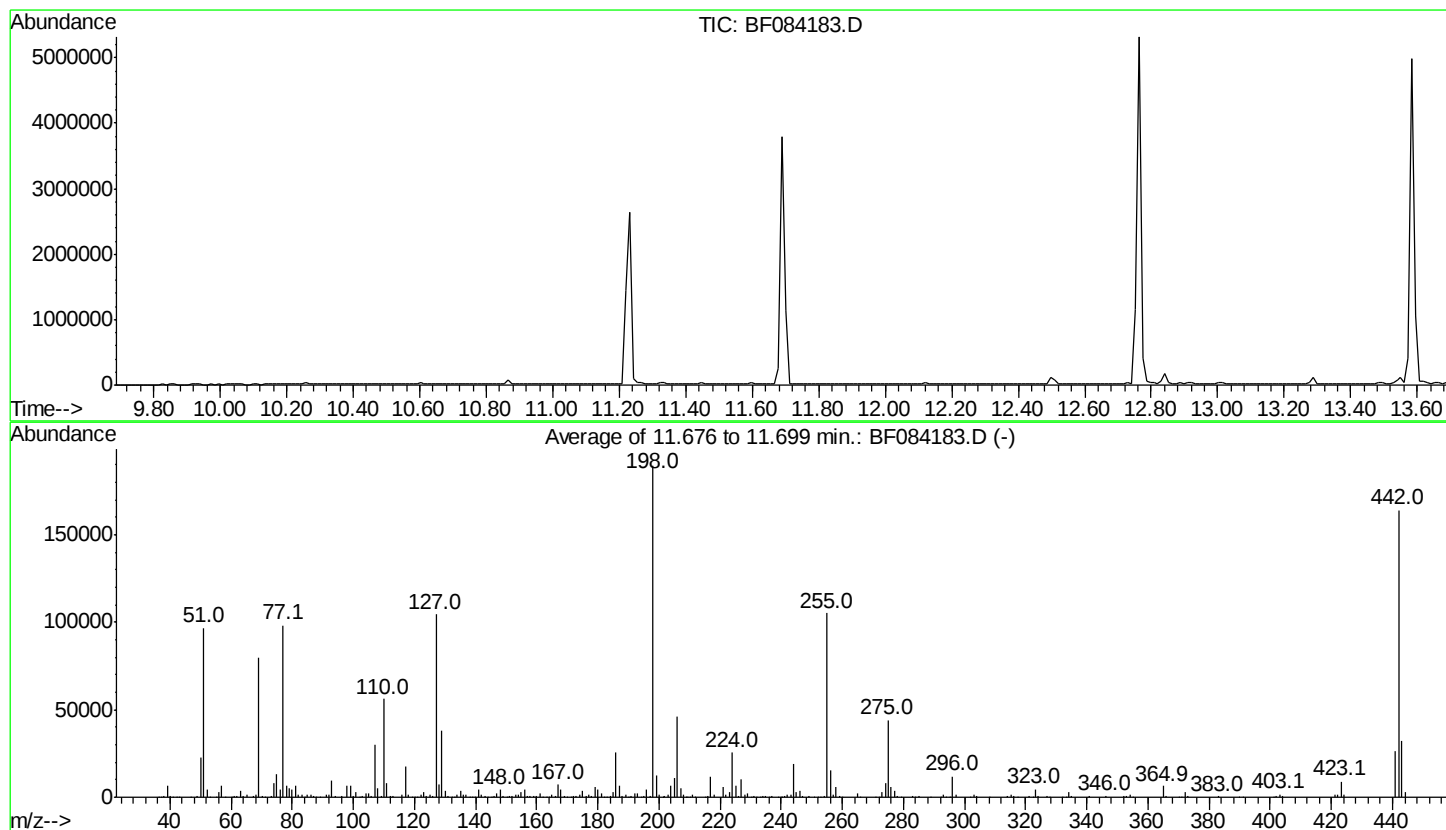

AutoFind: Scans 839, 840, 841; Background Corrected with Scan 836

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.0	96682	PASS
68	69	0.00	2	1.7	1327	PASS
69	198	0.00	100	42.3	80062	PASS
70	69	0.00	2	0.8	663	PASS
127	198	10	80	55.2	104565	PASS
197	198	0.00	2	0.5	916	PASS
198	198	100	100	100.0	189424	PASS
199	198	5	9	6.7	12599	PASS
275	198	10	60	23.2	43882	PASS
365	198	1	100	3.3	6339	PASS
441	442	0.01	24	16.1	26418	PASS
442	198	50	100	86.5	163870	PASS
443	442	15	24	19.9	32560	PASS