


Data Path : Z:\HPCHEM1\BNA F\DATA\BF123115\
 Data File : BF084207.D
 Acq On : 31 Dec 2015 20:59
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 04 12:22:40 2016

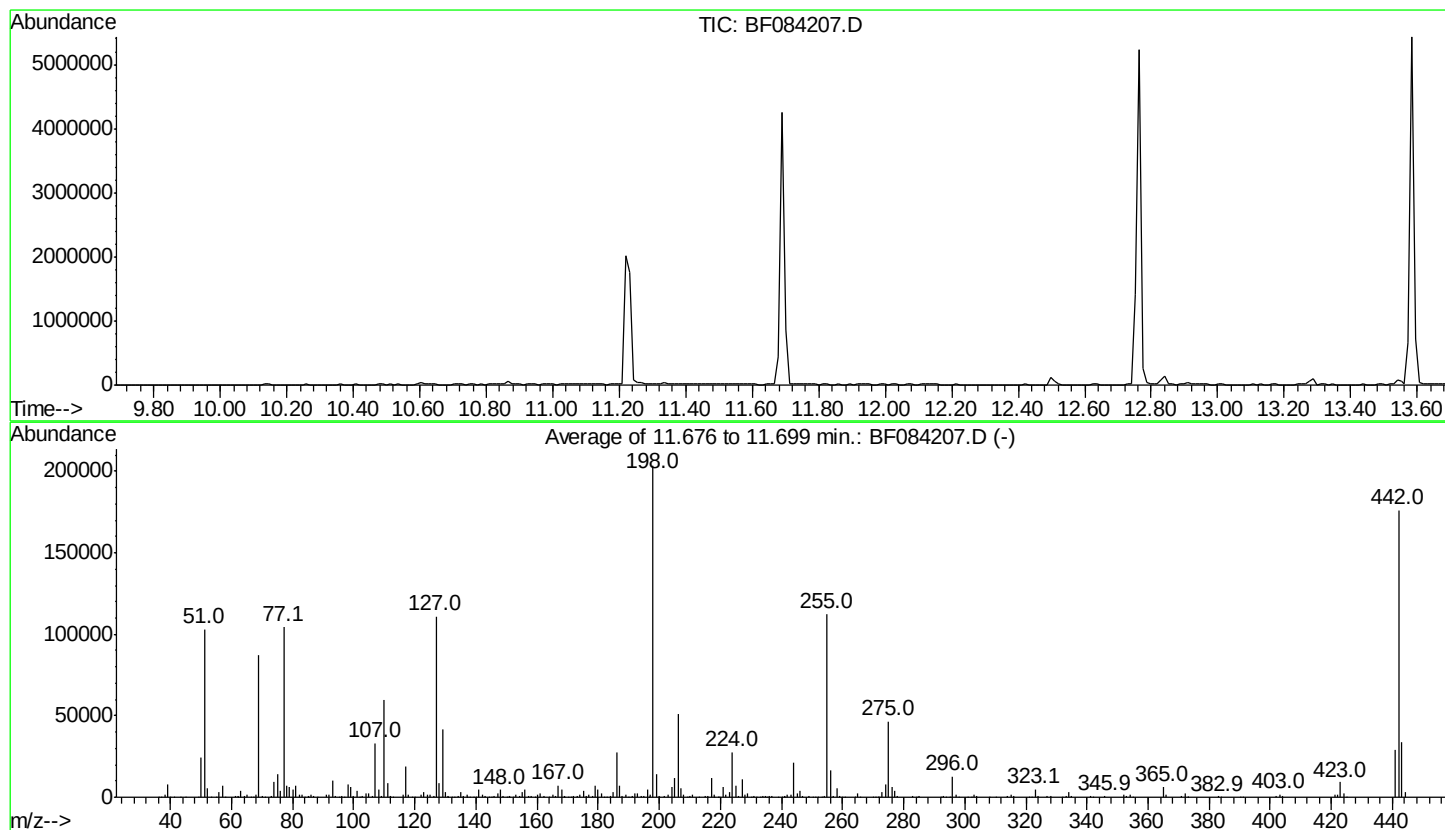

AutoFind: Scans 839, 840, 841; Background Corrected with Scan 836

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.6	102943	PASS
68	69	0.00	2	1.5	1284	PASS
69	198	0.00	100	43.1	87625	PASS
70	69	0.00	2	0.8	697	PASS
127	198	10	80	54.6	111079	PASS
197	198	0.00	2	0.7	1344	PASS
198	198	100	100	100.0	203520	PASS
199	198	5	9	6.9	14020	PASS
275	198	10	60	22.9	46649	PASS
365	198	1	100	3.2	6415	PASS
441	442	0.01	24	16.6	29161	PASS
442	198	50	100	86.5	176014	PASS
443	442	15	24	19.0	33416	PASS