
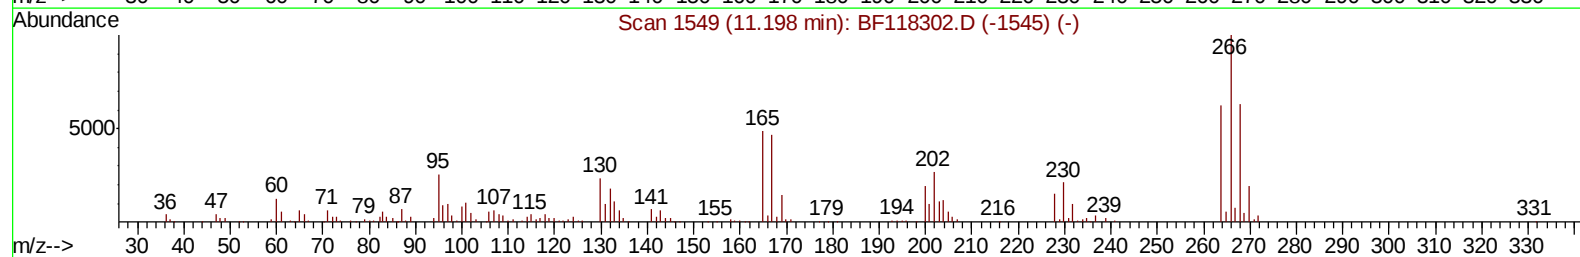
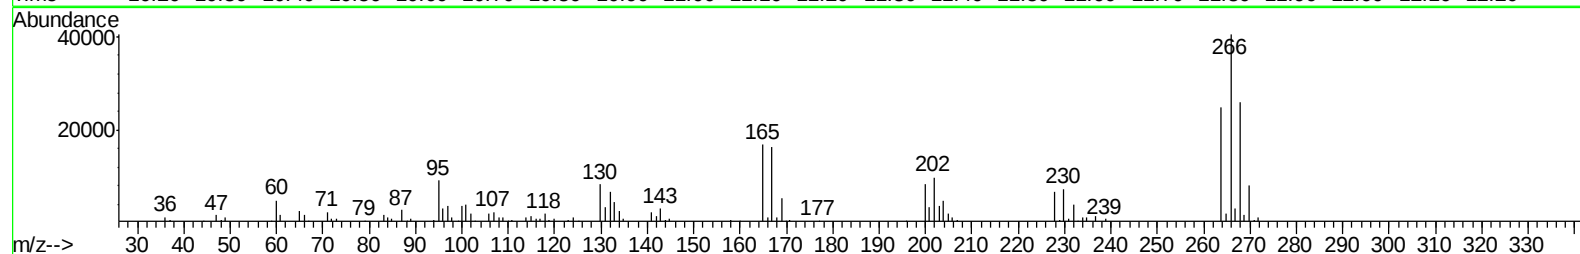


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF123119\
Data File : BF118398.D
Acq On : 31 Dec 2019 11:36
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 01 05:46:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF122419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 15:58:52 2019
Response via : Initial Calibration

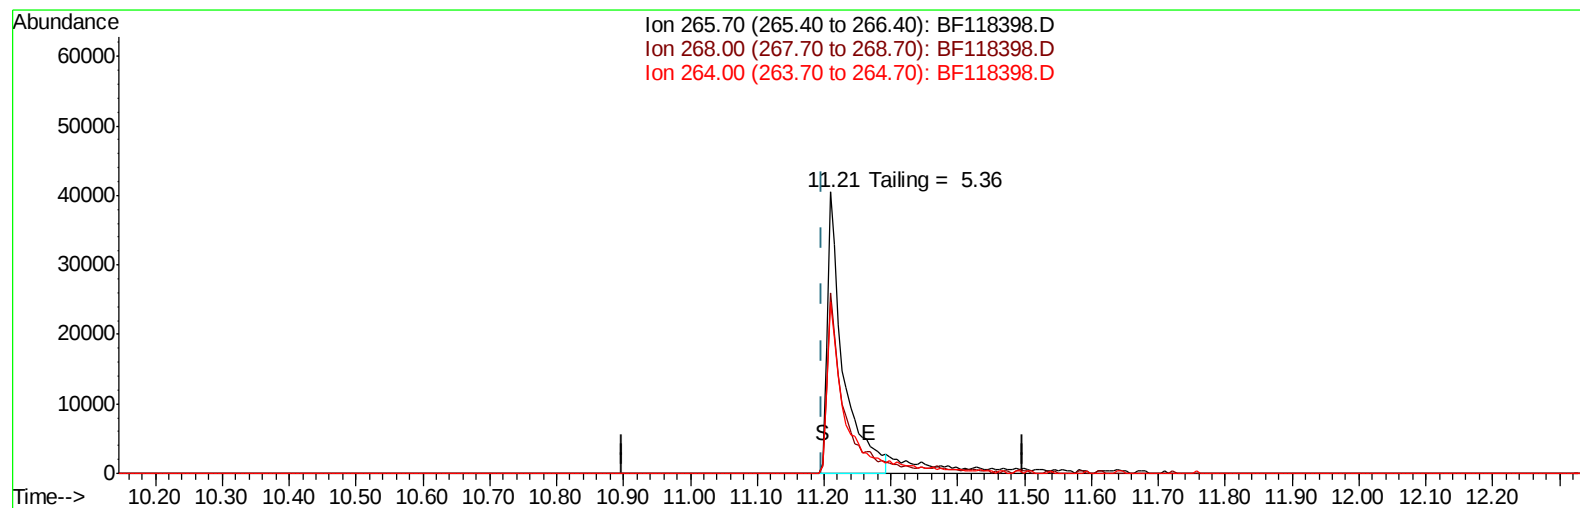

TIC: BF118398.D

(70) Pentachlorophenol (C)




11.210min (+0.012) 27329.13ng

response 71575

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	64.19
264.00	62.40	60.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF123119\
 Data File : BF118398.D
 Acq On : 31 Dec 2019 11:36
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 01 05:46:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF122419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 24 15:58:52 2019
 Response via : Initial Calibration

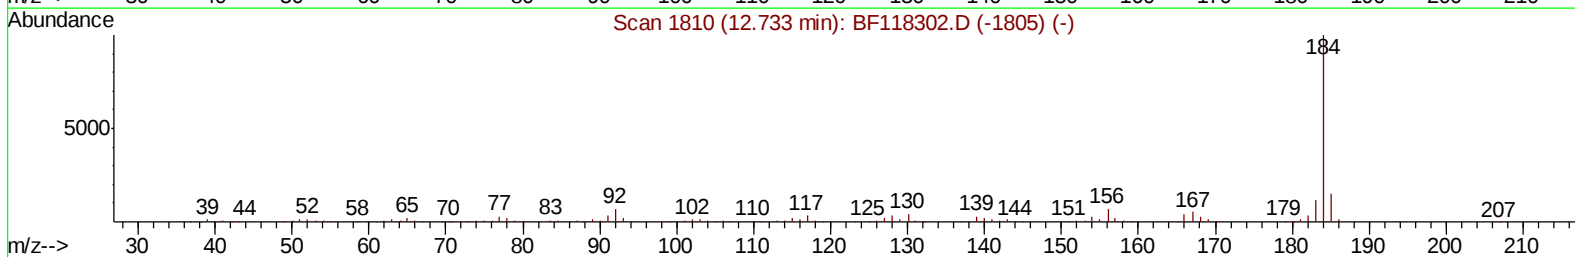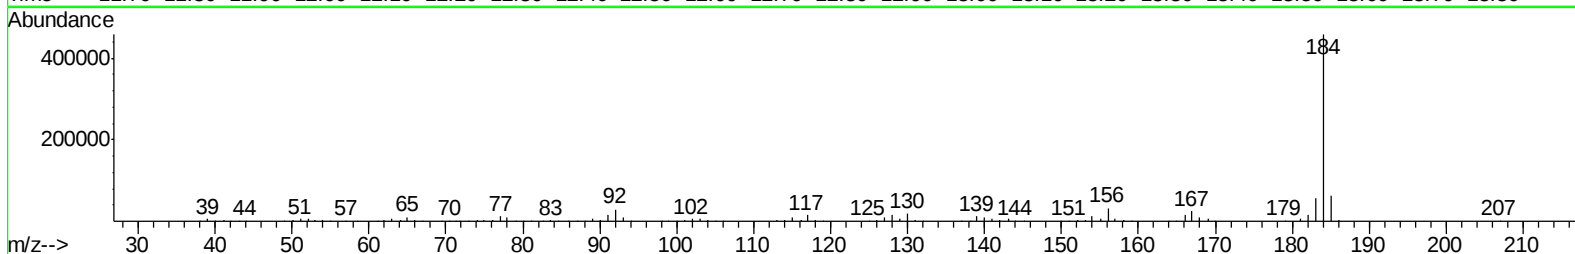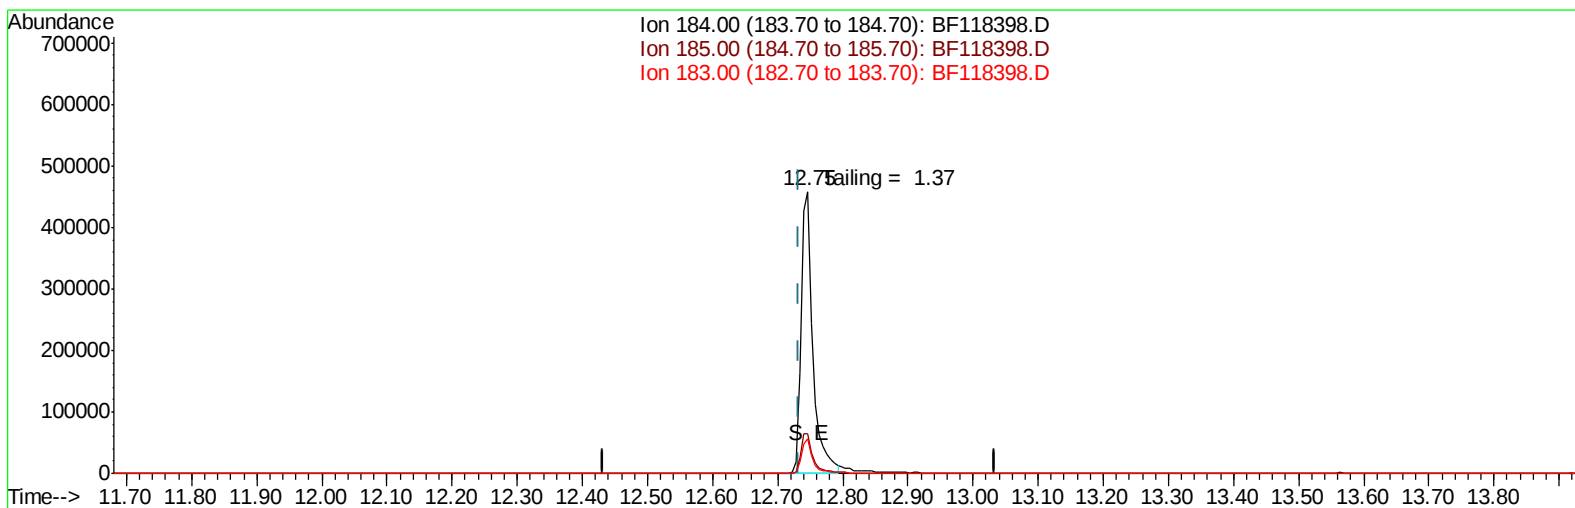

TIC: BF118398.D

(77) Benzidine

12.745min (+0.012) 0.00ng

response 596327

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	13.98
183.00	11.80	12.12
0.00	0.00	0.00