

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF123119\
 Data File : BF118417.D
 Acq On : 31 Dec 2019 20:48
 Operator : JU
 Sample : K6463-01RE 2X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GP-6-(1-3)RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.051	500	504	522	rVB	90197	111943	12.92%	1.004%
2	5.469	572	575	596	rBV	574184	681994	78.74%	6.117%
3	6.487	745	748	768	rBV	607484	779716	90.02%	6.994%
4	6.622	768	771	779	rVV	914753	866117	100.00%	7.769%
5	6.851	807	810	818	rBV	524331	421859	48.71%	3.784%
6	7.010	833	837	851	rVB	703623	631831	72.95%	5.667%
7	7.416	903	906	916	rBV	433605	469013	54.15%	4.207%
8	8.139	1026	1029	1048	rBV	516116	523139	60.40%	4.692%
9	9.216	1208	1212	1223	rBV	871204	845131	97.58%	7.581%
10	9.328	1228	1231	1235	rVB2	15659	17933	2.07%	0.161%
11	9.616	1277	1280	1287	rVB	48109	55145	6.37%	0.495%
12	9.904	1325	1329	1342	rVB	548080	605447	69.90%	5.431%
13	10.322	1397	1400	1403	rVB2	9700	9908	1.14%	0.089%
14	10.457	1419	1423	1425	rBV2	8803	10176	1.17%	0.091%
15	10.698	1460	1464	1475	rBV	598736	623742	72.02%	5.595%
16	10.798	1479	1481	1486	rVB2	11504	16417	1.90%	0.147%
17	11.245	1554	1557	1561	rBV2	11325	12096	1.40%	0.108%
18	11.398	1579	1583	1585	rBV	576661	532464	61.48%	4.776%
19	11.422	1585	1587	1592	rVV	181809	168595	19.47%	1.512%
20	11.475	1592	1596	1602	rVB	29867	36888	4.26%	0.331%
21	11.675	1628	1630	1636	rVB4	11909	12888	1.49%	0.116%
22	11.916	1666	1671	1672	rBV2	49005	56315	6.50%	0.505%
23	11.933	1672	1674	1680	rVV2	42276	51992	6.00%	0.466%
24	11.980	1680	1682	1685	rVV2	14404	17030	1.97%	0.153%
25	12.016	1685	1688	1690	rVV	33316	38120	4.40%	0.342%
26	12.039	1690	1692	1697	rVV	18037	19793	2.29%	0.178%
27	12.086	1697	1700	1703	rVB2	13691	13299	1.54%	0.119%
28	12.198	1716	1719	1723	rBV	13515	14883	1.72%	0.133%
29	12.239	1723	1726	1729	rVB5	12168	12165	1.40%	0.109%
30	12.451	1759	1762	1764	rBV	18657	21143	2.44%	0.190%
31	12.474	1764	1766	1770	rVB4	14810	14537	1.68%	0.130%
32	12.551	1775	1779	1781	rBV3	12500	16355	1.89%	0.147%
33	12.616	1787	1790	1795	rBV	258931	241732	27.91%	2.168%
34	12.710	1804	1806	1810	rBV4	9606	14299	1.65%	0.128%

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF123119\
 Data File : BF118417.D
 Acq On : 31 Dec 2019 20:48
 Operator : JU
 Sample : K6463-01RE 2X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GP-6-(1-3)RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.769	1813	1816	1820	rVV4	11401	16205	1.87%	0.145%
36	12.851	1823	1830	1836	rVV	228586	267248	30.86%	2.397%
37	12.898	1836	1838	1843	rVB2	17361	15618	1.80%	0.140%
38	12.986	1849	1853	1856	rBV	779543	740247	85.47%	6.640%
39	13.074	1862	1868	1873	rBV6	16472	31363	3.62%	0.281%
40	13.116	1873	1875	1879	rBV5	7281	9763	1.13%	0.088%
41	13.174	1879	1885	1888	rVV2	25638	51394	5.93%	0.461%
42	13.204	1888	1890	1893	rVB2	27896	29365	3.39%	0.263%
43	13.245	1895	1897	1900	rBV4	10720	10939	1.26%	0.098%
44	13.286	1900	1904	1907	rBV2	19345	27572	3.18%	0.247%
45	13.374	1917	1919	1922	rBV	13267	11910	1.38%	0.107%
46	13.410	1922	1925	1926	rBV3	13257	12198	1.41%	0.109%
47	13.551	1946	1949	1952	rBV4	18225	18850	2.18%	0.169%
48	13.604	1956	1958	1960	rBV3	11315	9681	1.12%	0.087%
49	13.698	1971	1974	1978	rBV	22326	24280	2.80%	0.218%
50	13.804	1990	1992	1994	rBV2	23035	18037	2.08%	0.162%
51	13.857	1999	2001	2002	rBV	19790	16710	1.93%	0.150%
52	13.880	2002	2005	2008	rBV4	93747	109126	12.60%	0.979%
53	14.051	2029	2034	2037	rBV2	541684	608238	70.23%	5.456%
54	14.080	2037	2039	2042	rVB	99779	90250	10.42%	0.810%
55	14.198	2057	2059	2061	rBV2	23191	16430	1.90%	0.147%
56	14.504	2109	2111	2114	rBV3	34486	36461	4.21%	0.327%
57	14.815	2161	2164	2166	rBV	41302	41109	4.75%	0.369%
58	15.110	2212	2214	2217	rBV	58708	68976	7.96%	0.619%
59	15.421	2265	2267	2270	rVB	44572	42934	4.96%	0.385%
60	15.486	2275	2278	2283	rBV	72560	96144	11.10%	0.862%
61	15.551	2284	2289	2294	rBV	397775	548445	63.32%	4.919%
62	17.086	2545	2550	2557	rBV6	32955	94186	10.87%	0.845%
63	17.639	2642	2644	2645	rBV2	18357	17647	2.04%	0.158%
64	18.209	2736	2741	2743	rBV6	31810	57966	6.69%	0.520%
65	18.327	2756	2761	2762	rBV4	27421	45252	5.22%	0.406%


Sum of corrected areas: 11148649

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF123119\
Data File : BF118417.D
Acq On : 31 Dec 2019 20:48
Operator : JU
Sample : K6463-01RE 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
GP-6-(1-3)RE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF122419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

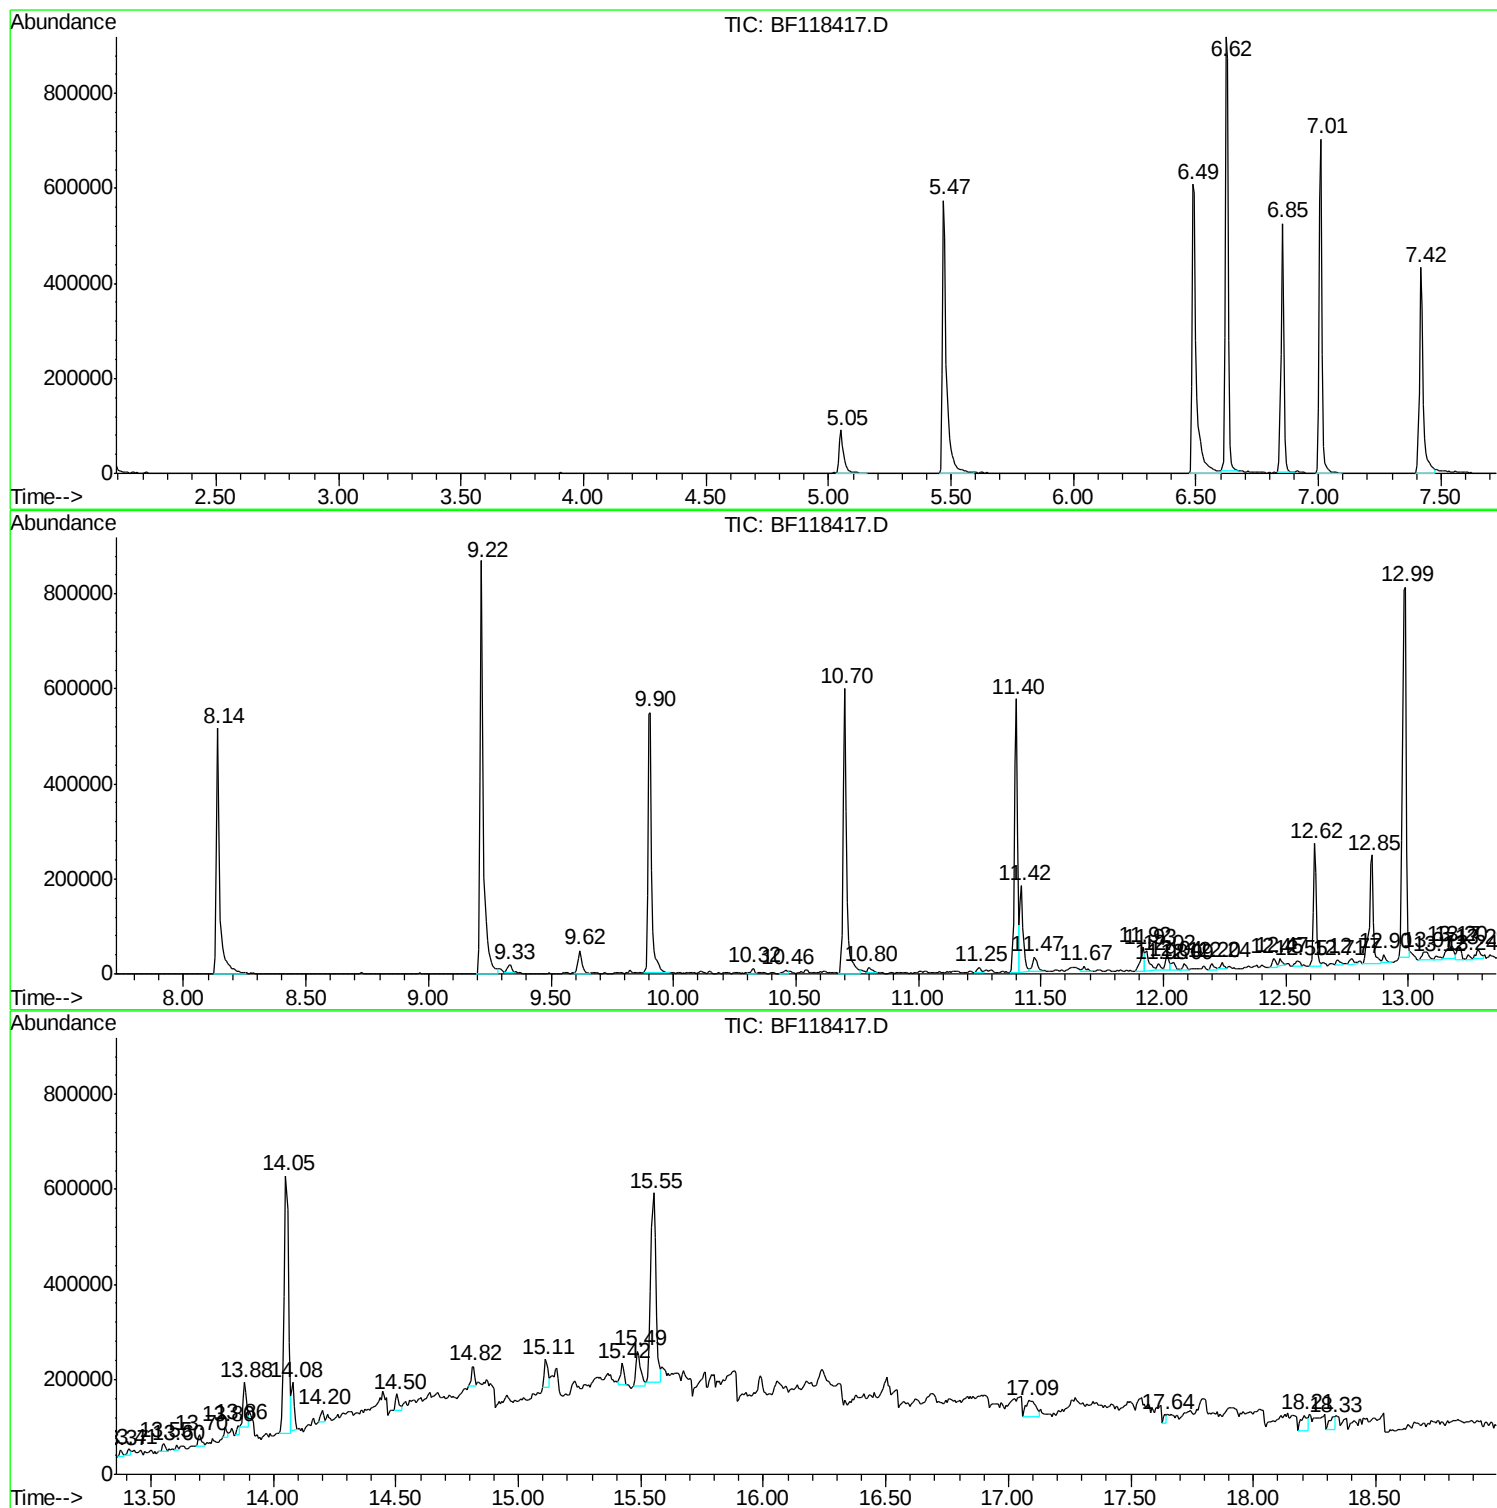

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF123119\
Data_File : BF118417.D
Acq_On : 31-Dec-2019 20:488
Operator : JUJ
Sample : K6463-01RE_2XX
Misc :
ALS_Vial : 20 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
GP-6-(1-3)RE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
