


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF123119\
 Data File : BF118398.D
 Acq On : 31 Dec 2019 11:36
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 24 15:58:52 2019

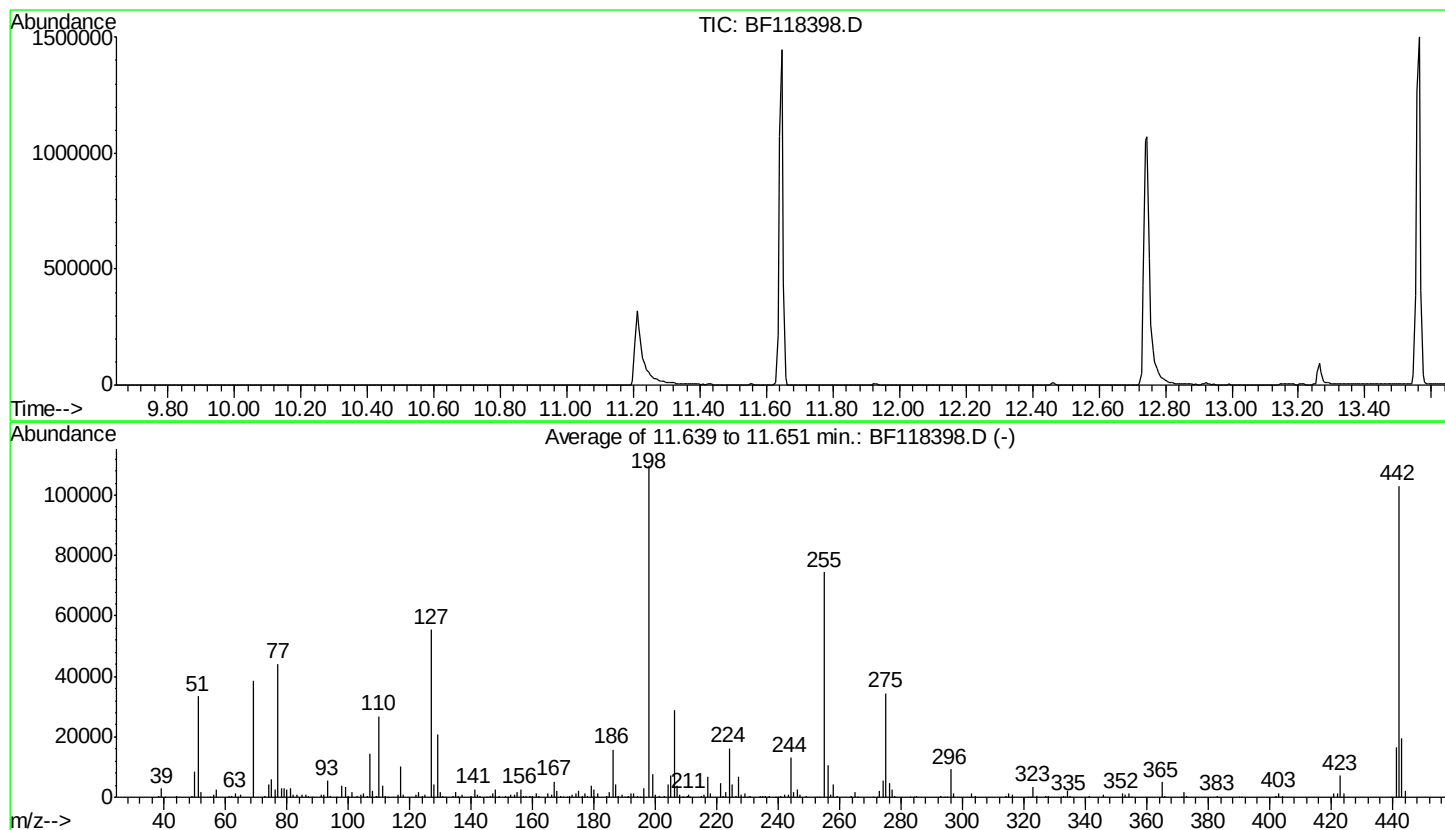

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	33448	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.3	38735	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.5	55450	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	109768	PASS
199	198	5	9	6.8	7495	PASS
275	198	10	60	31.4	34493	PASS
365	198	1	100	4.6	5075	PASS
441	198	0.01	100	15.2	16634	PASS
442	198	50	100	93.9	103082	PASS
443	442	15	24	19.1	19711	PASS