

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123124\
Data File : BF141048.D
Acq On : 31 Dec 2024 10:17
Operator : RC/JU
Sample : PB165790BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165790BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141048.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.451	563	571	576	rBV	5391822	8034461	74.72%	13.106%
2	6.451	733	741	746	rBV	5414798	8154851	75.84%	13.302%
3	6.828	799	805	810	rBV	1301330	1615450	15.02%	2.635%
4	7.386	893	900	905	rBV	3803918	5425994	50.46%	8.851%
5	8.104	1016	1022	1028	rBV	1633600	2190374	20.37%	3.573%
6	9.180	1198	1205	1211	rBV	6846520	9677576	90.00%	15.786%
7	9.857	1314	1320	1334	rBV	1937508	2526214	23.49%	4.121%
8	10.645	1447	1454	1479	rBV	4551602	6327417	58.85%	10.321%
9	11.345	1567	1573	1578	rBV	2034588	2573891	23.94%	4.199%
10	12.933	1837	1843	1849	rBV	7539977	10752410	100.00%	17.540%
11	13.980	2016	2021	2035	rBV	1756457	2301986	21.41%	3.755%
12	15.445	2264	2270	2277	rBV	1055418	1723264	16.03%	2.811%




Sum of corrected areas: 61303888

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123124\
Data File : BF141048.D
Acq On : 31 Dec 2024 10:17
Operator : RC/JU
Sample : PB165790BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165790BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

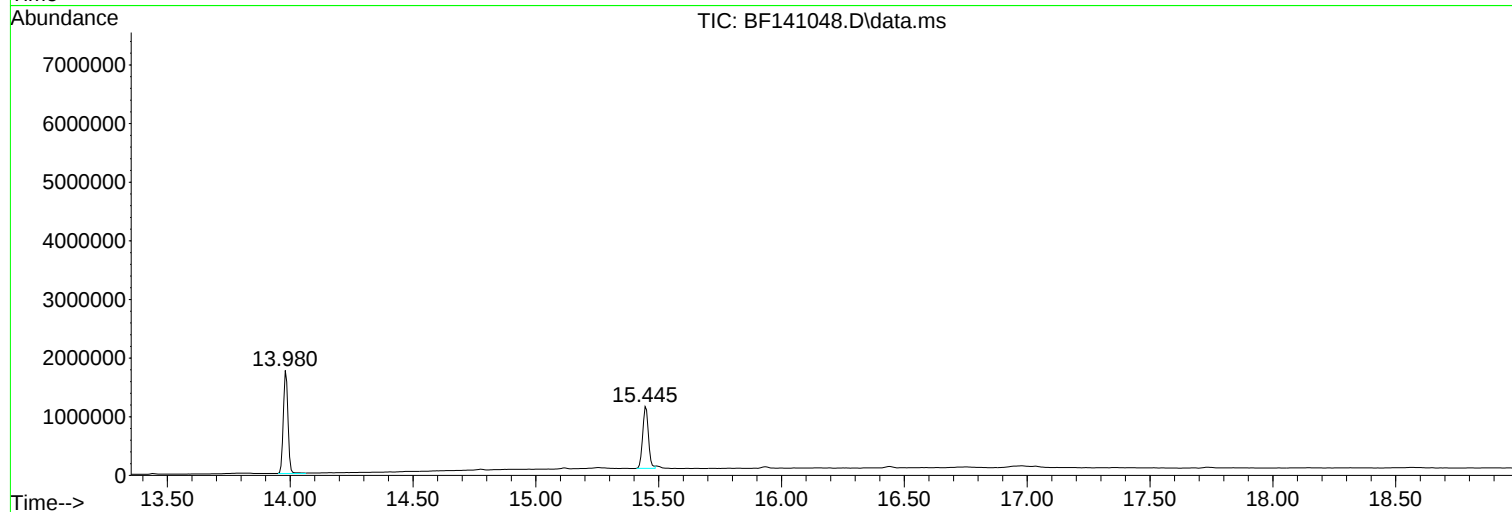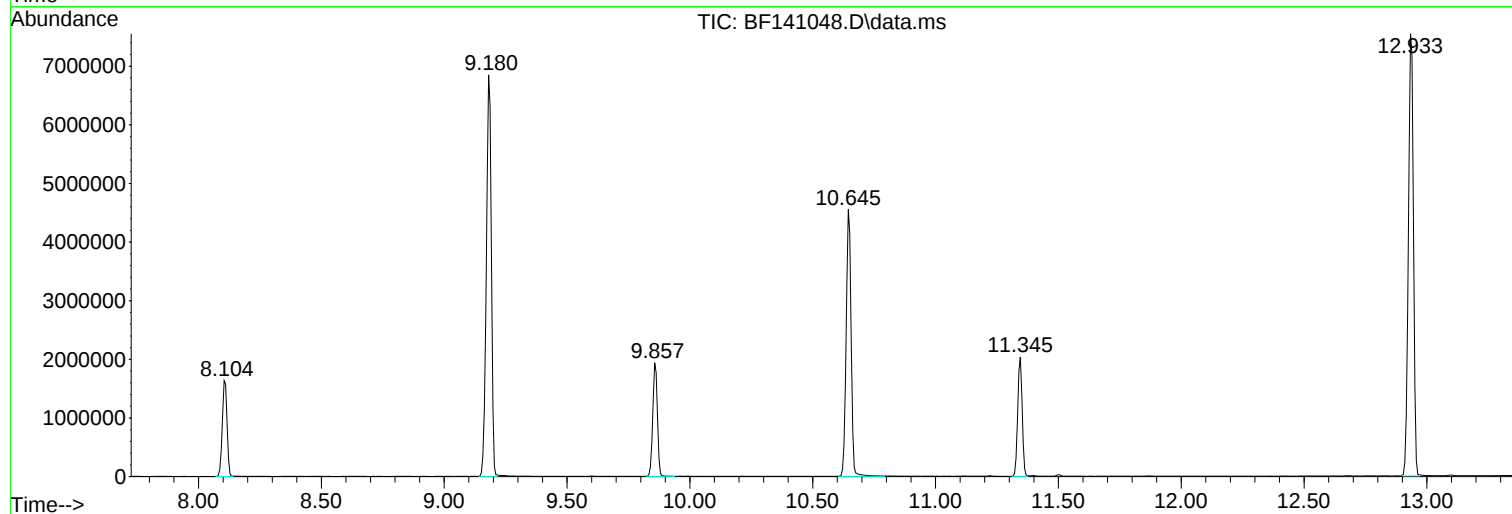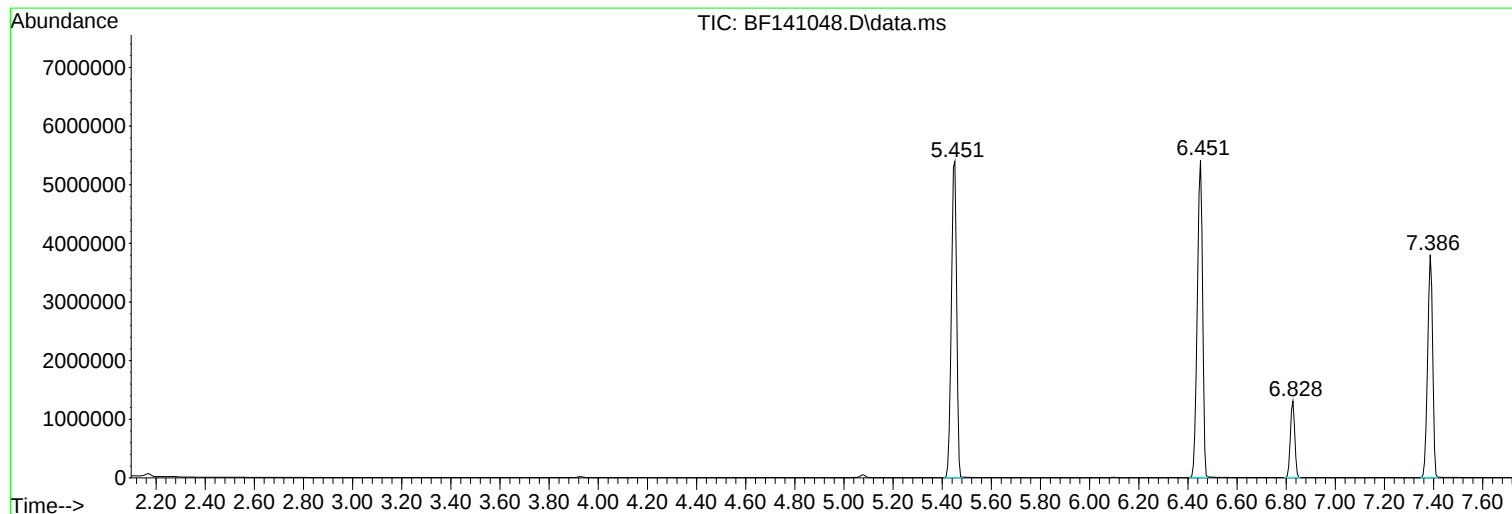

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123124\
Data File : BF141048.D
Acq On : 31 Dec 2024 10:17
Operator : RC/JU
Sample : PB165790BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165790BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123124\
Data File : BF141048.D
Acq On : 31 Dec 2024 10:17
Operator : RC/JU
Sample : PB165790BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165790BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------