


Data Path : Z:\HPCHEM1\BNA_J\data\BJ041712\
 Data File : BJ000752.D
 Acq On : 17 Apr 2012 12:55
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 BNA_J HLM
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_J
 ClientSampleId :
 DFTPP050

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_J\method\BJ041712.M
 Title : CWA degradation products by GCMS
 Last Update : Tue Apr 17 17:08:29 2012

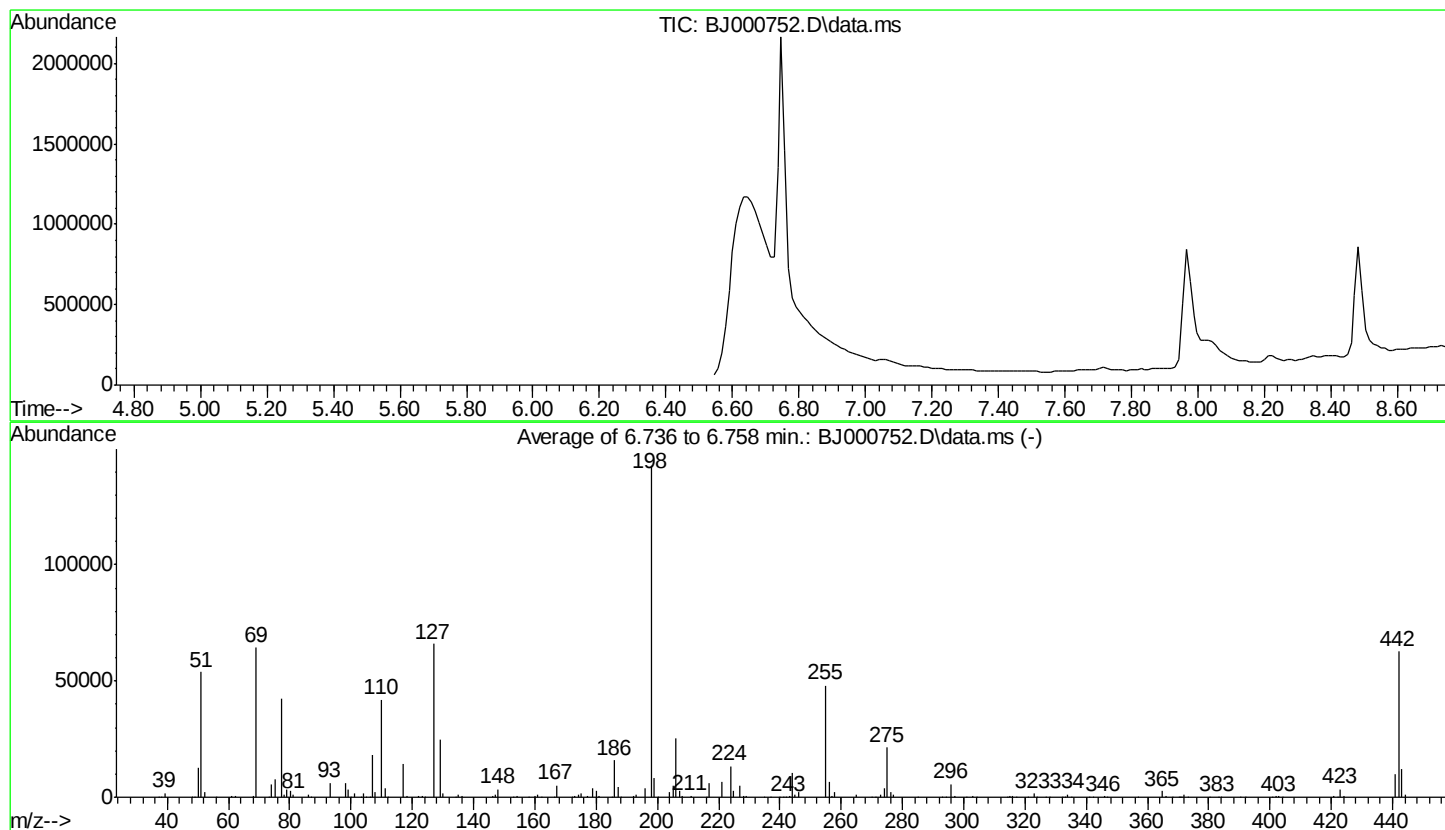

AutoFind: Scans 18, 19, 20; Background Corrected with Scan 13

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	37.7	53768	PASS
68	69	0.00	2	0.7	429	PASS
69	198	0.00	100	45.1	64274	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	46.2	65866	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	142642	PASS
199	198	5	9	5.9	8474	PASS
275	198	10	30	14.9	21309	PASS
365	198	1	100	1.8	2552	PASS
441	443	0.01	100	82.7	9966	PASS
442	198	40	100	43.9	62630	PASS
443	442	17	23	19.2	12053	PASS