

Data File : H:\VOL1\GCMSDATA\J\120718\BJ001019.D
Acq On : 18 Jul 2012 15:16
Sample : D3369-01MSD
Misc : WATER BNA J HLM
MS Integration Params: RTEINT.P
Quant Time: Jul 18 16:07 2012

Vial: 14
Operator: HLM
Inst : BNA J
Multiplr: 1.00

Quant Results File: BJ071812.RES

Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M (RTE Integrator)
Title : P4 by SOP M.5
Last Update : Wed Jul 18 14:03:32 2012
Response via : Initial Calibration
DataAcq Meth : P4

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.65	150	381769	2.50	ug/ml	0.01
System Monitoring Compounds						
2) Tripropylphosphate	6.73	99	704510	2.30	ug/ml	0.00
Spiked Amount	2.500	Range	20 - 150	Recovery	=	92.00%
Target Compounds						Ovalue
3) White Phosphorus	5.05	124	166784	0.53	ug/ml	94

Quantitation Report

Data File : H:\VOL1\GCMSDATA\J\120718\BJ001019.D

Vial: 14

Acq On : 18 Jul 2012 15:16

Operator: HLM

Sample : D3369-01MSD

Inst : BNA J

Misc : WATER BNA J HLM

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Jul 18 16:07 2012


Quant Results File: BJ071812.RES


Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M (RTE Integrator)

Title : P4 by SOP M.5

Last Update : Wed Jul 18 14:03:32 2012

Response via : Initial Calibration

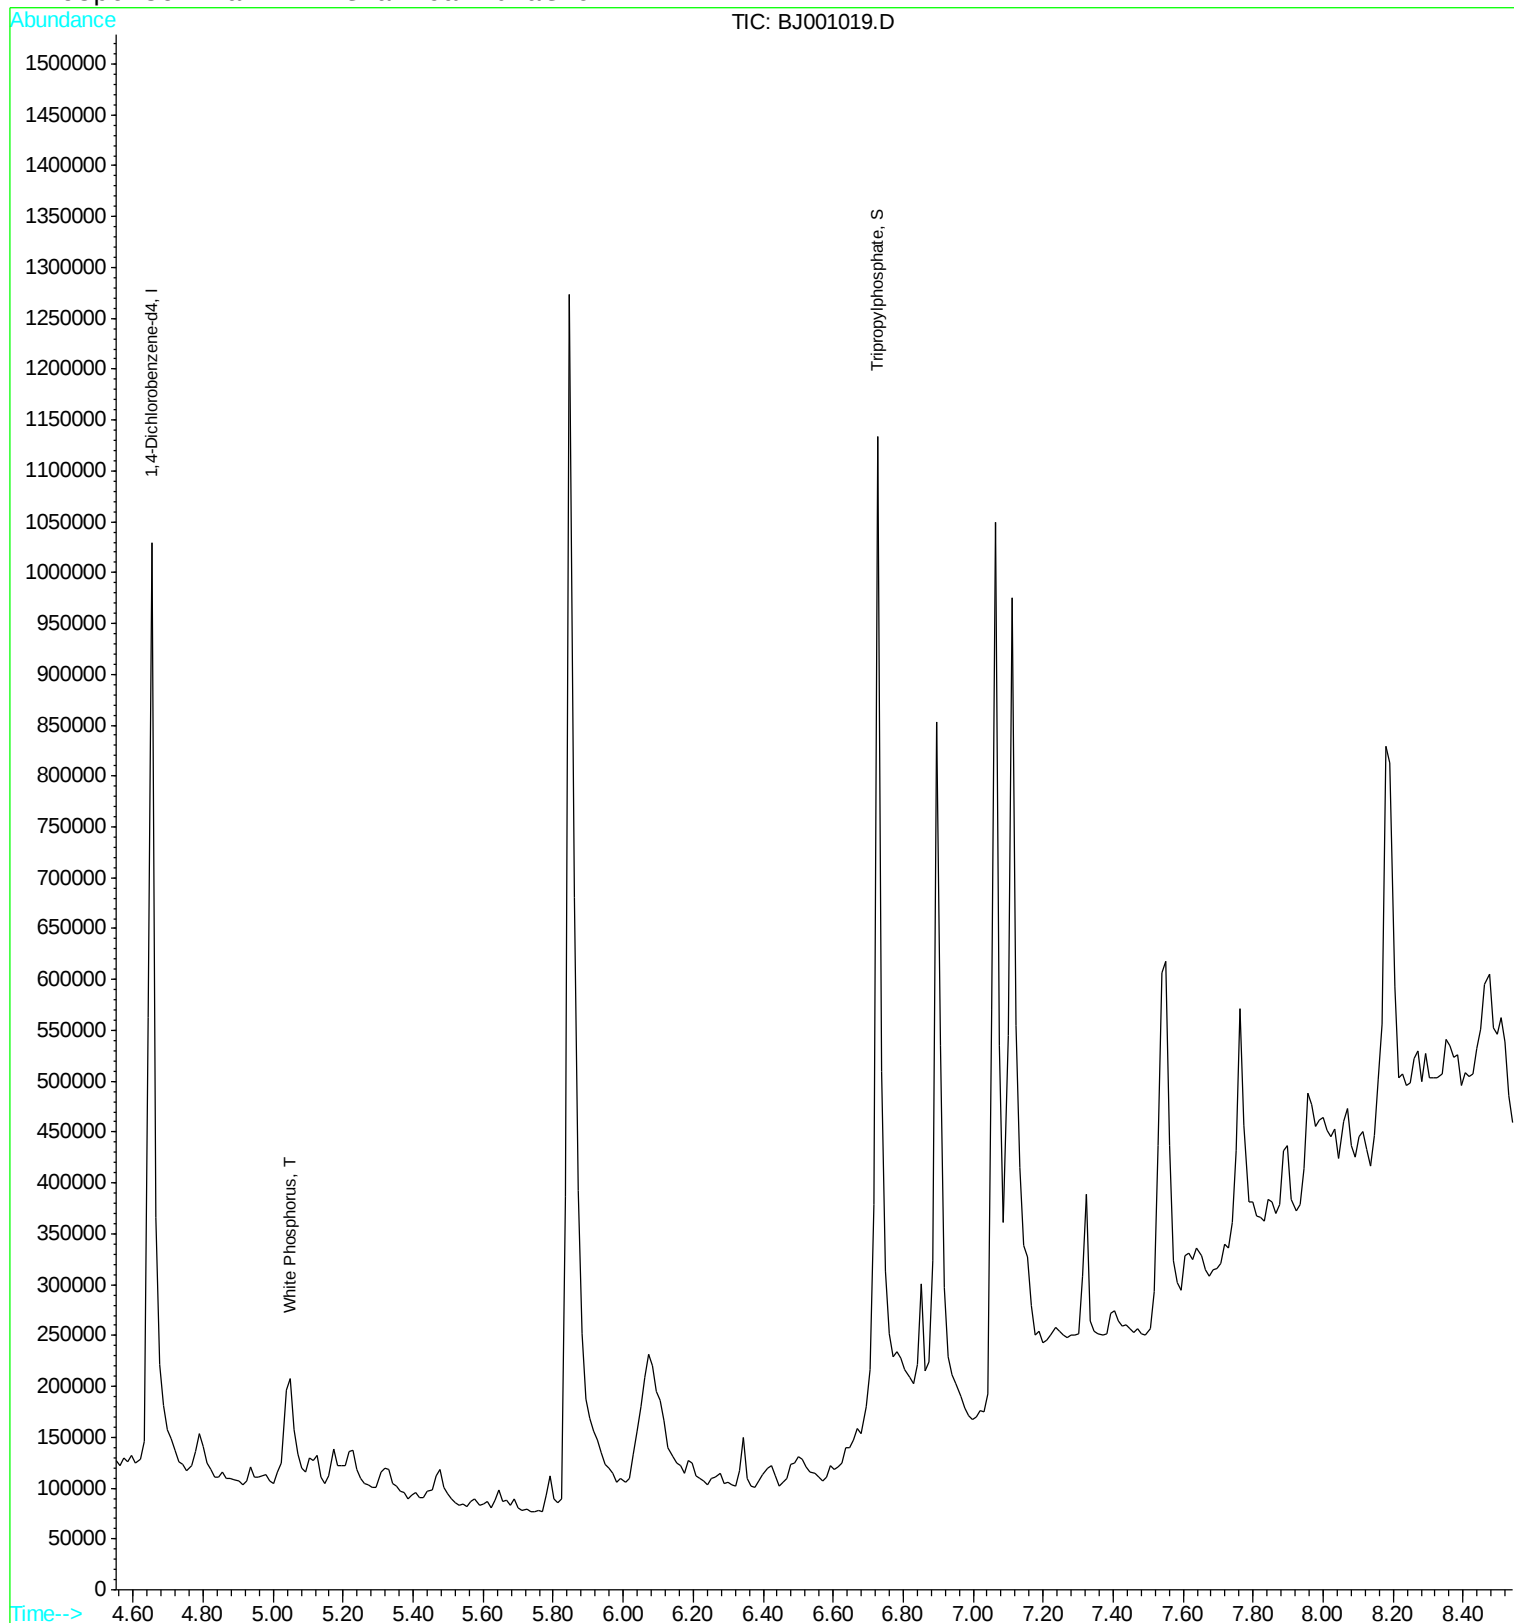

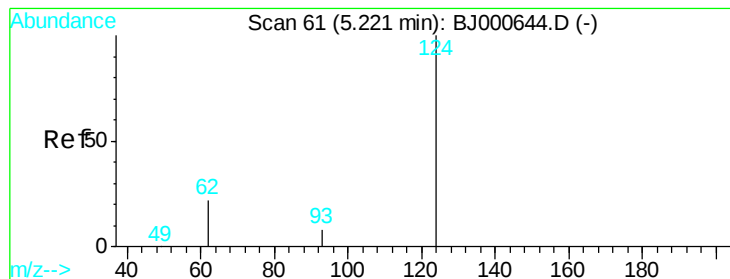

#3

White Phosphorus

Concen: 0.53 ug/ml

RT: 5.05 min Scan# 45

Delta R.T. 0.01 min

Lab File: BJ001019.D

Acq: 18 Jul 2012 15:16


Tgt Ion:124 Resp: 166784

Ion Ratio Lower Upper

124 100

93 9.0 0.0 27.8

62 21.9 0.0 39.0

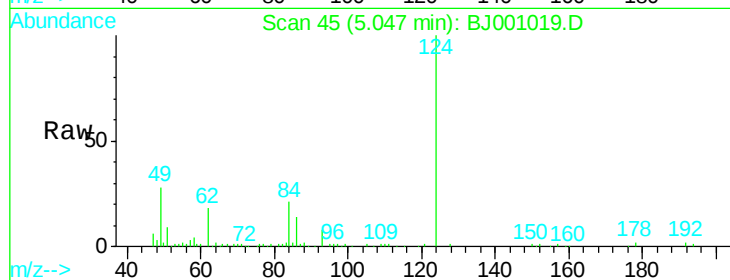

Abundance

Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

