

DFTPP

Data File : H:\VOL1\GCMSDATA\J\120718\BJ001006.D

Vial: 1

Acq On : 18 Jul 2012 11:19

Operator: HLM

Sample : DFTPP050

Inst : BNA_J


Misc : DFTPP050 BNA_J HLM

Multiplr: 1.00

MS Integration Params: RTEINT.P

Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M (RTE Integrator)

Title : P4 by SOP M.5

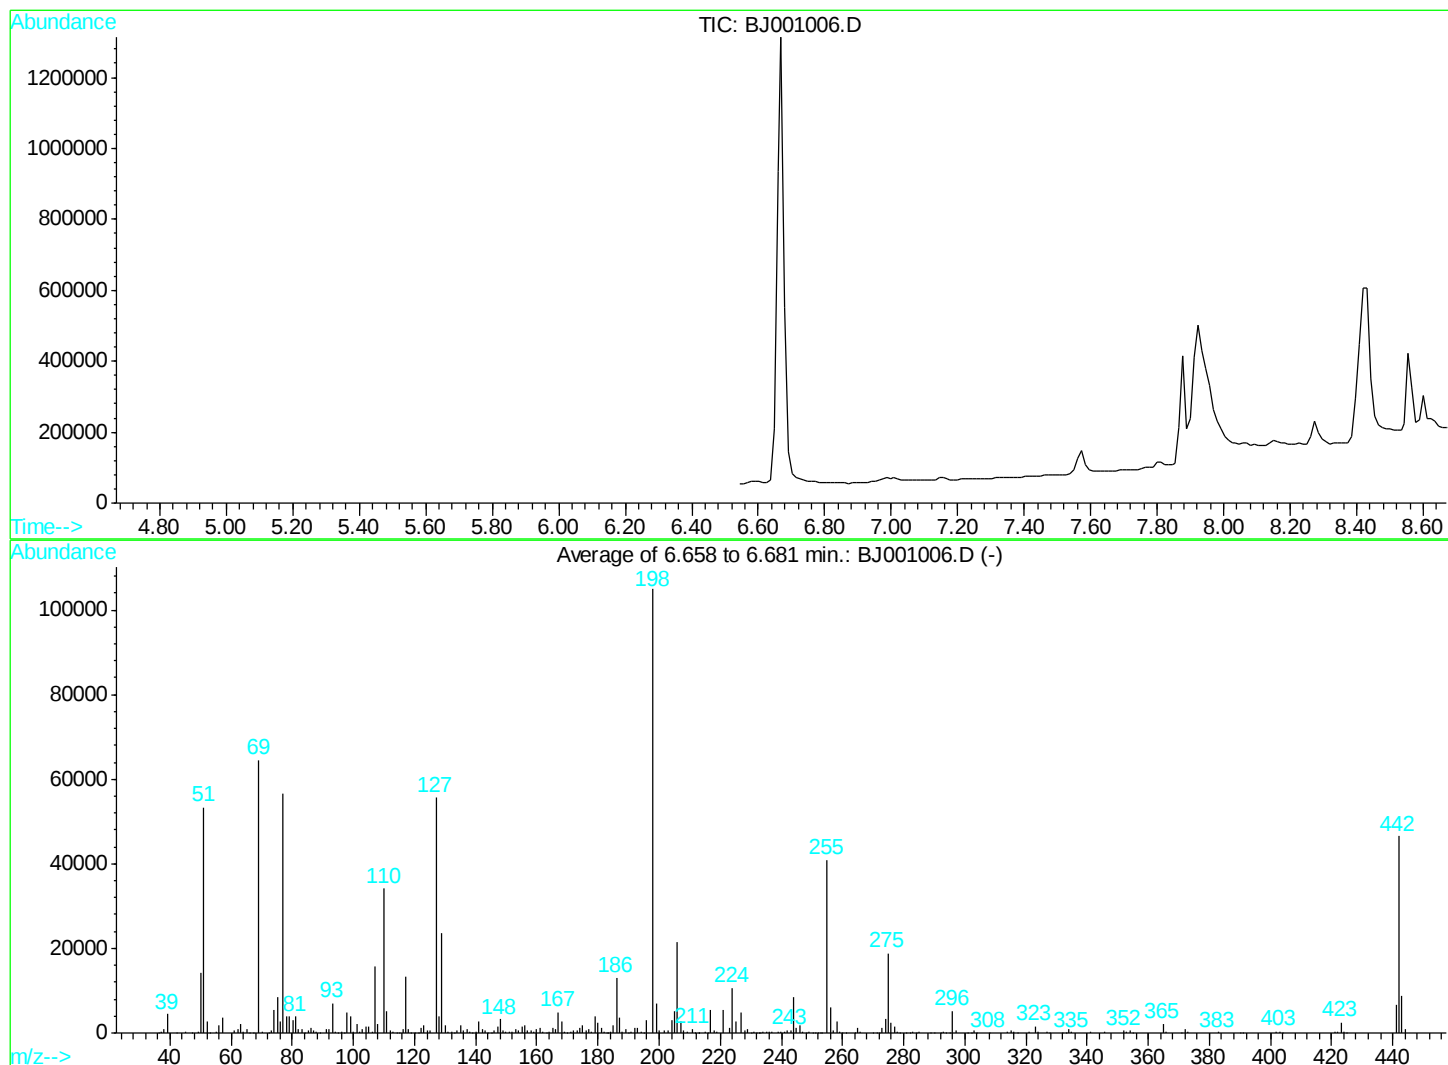

AutoFind: Scans 11, 12, 13; Background Corrected with Scan 6

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	50.8	53299	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	61.6	64559	PASS
70	69	0.00	2	0.5	295	PASS
127	198	40	60	53.0	55615	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	104888	PASS
199	198	5	9	6.6	6970	PASS
275	198	10	30	17.9	18821	PASS
365	198	1	100	2.2	2263	PASS
441	443	0.01	100	77.2	6815	PASS
442	198	40	100	44.3	46509	PASS
443	442	17	23	19.0	8824	PASS