



Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ071812\
Data File : BJ001007.D
Acq On : 18 Jul 2012 11:41
Operator : HLM
Sample : P4-7
Misc : 10.0ug/mL BNA_J HLM
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
P4-7

Quant Time: Jul 23 01:40:19 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Jul 18 14:01:29 2012
Response via : Initial Calibration

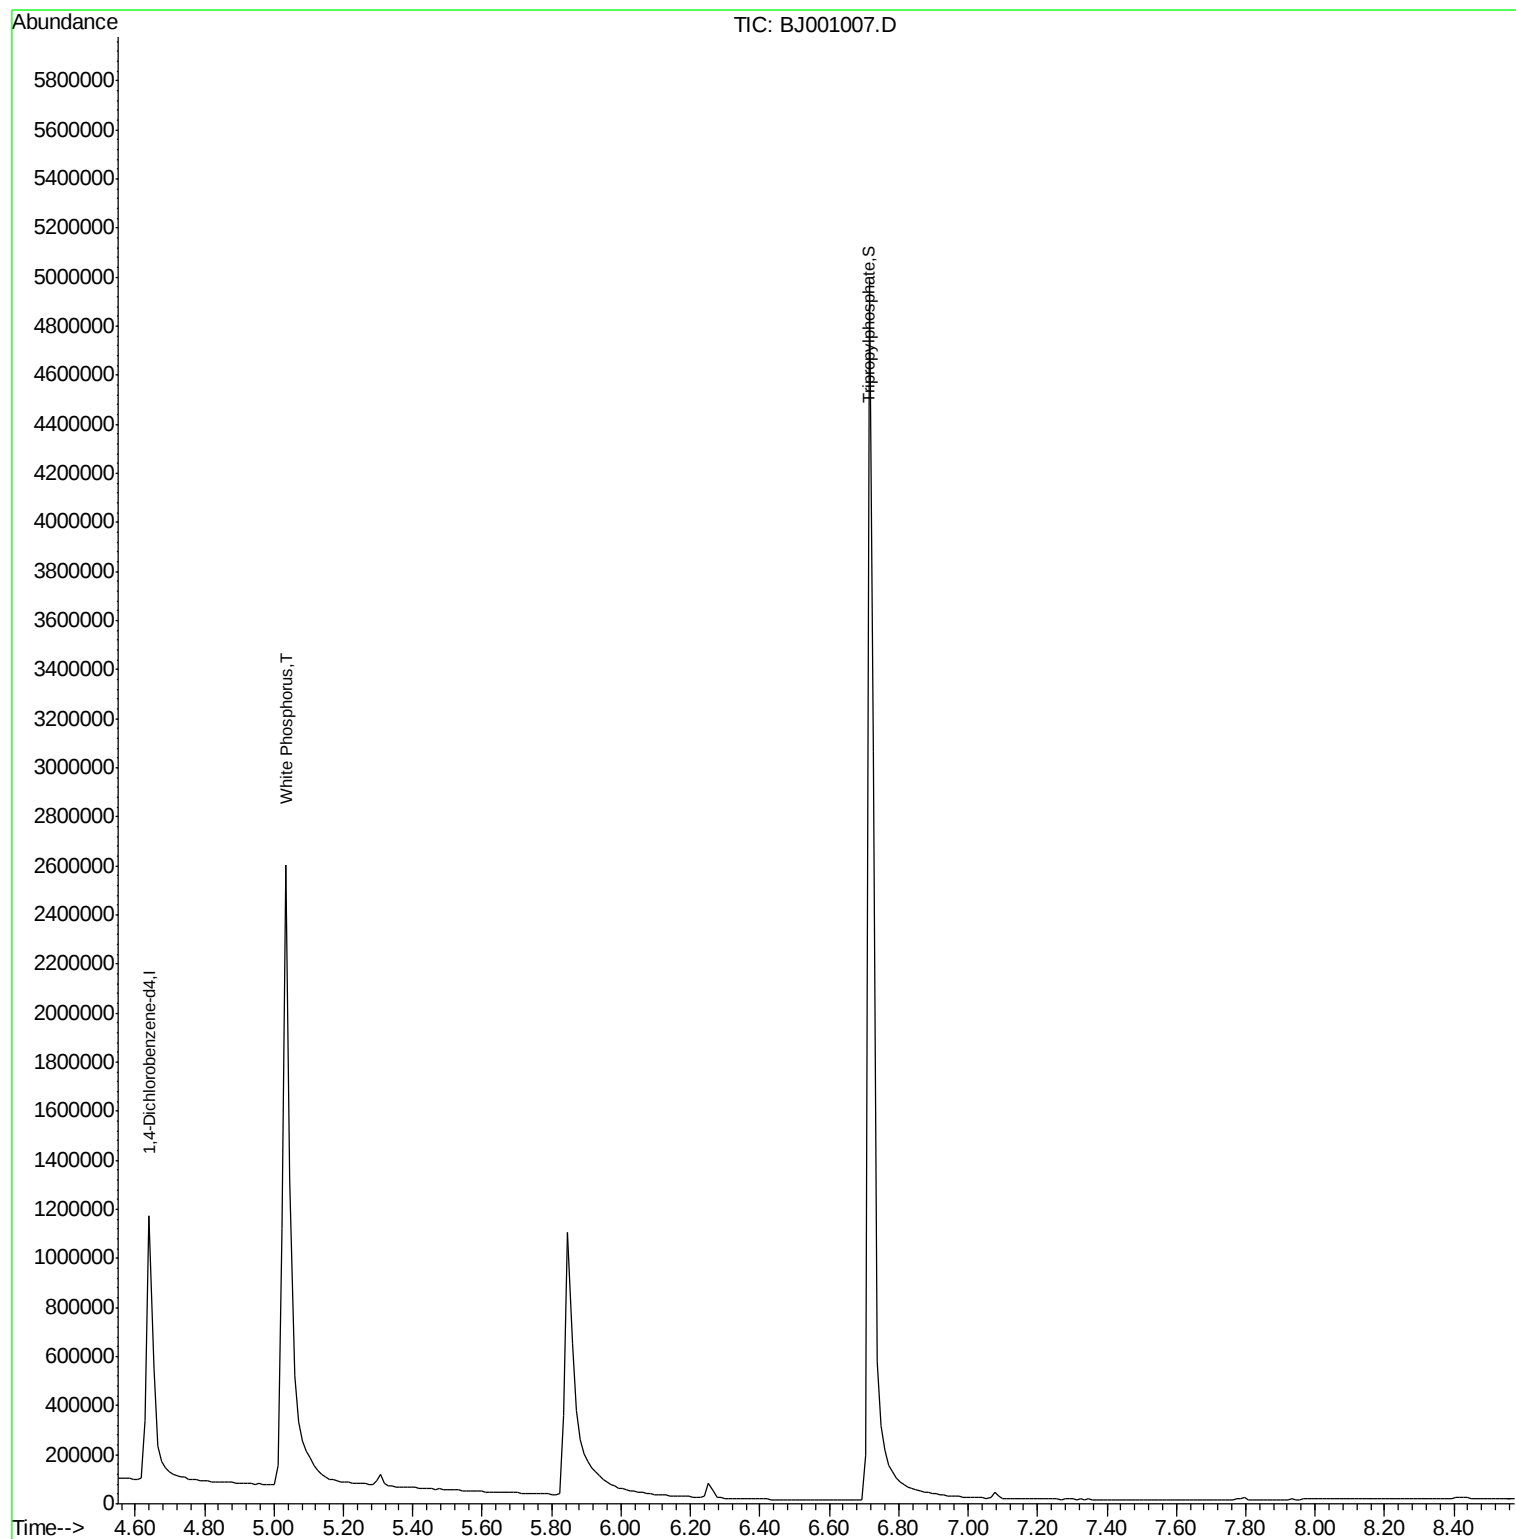

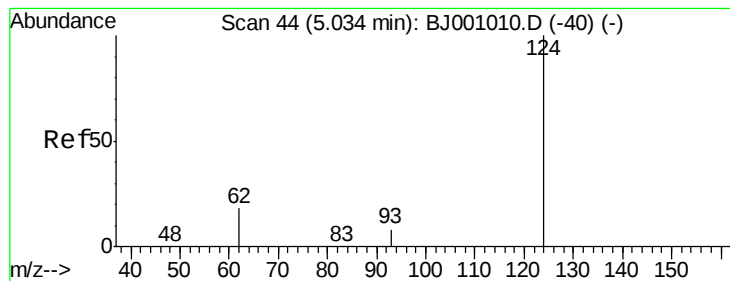

#3

White Phosphorus

Concen: 11.77 ug/ml

RT: 5.04 min Scan# 44

Delta R.T. 0.00 min

Lab File: BJ001007.D


Acq: 18 Jul 2012 11:41

Instrument :

BNA_J

ClientSampleId :

P4-7

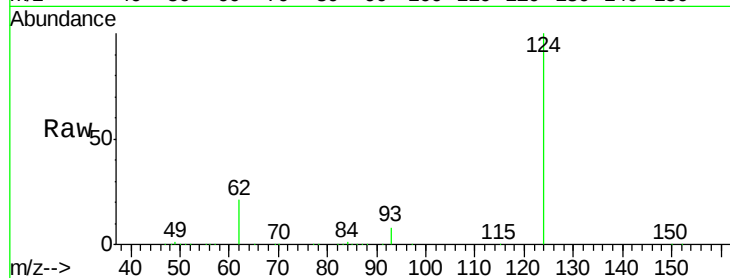


Tgt Ion:124 Resp: 3512932

Ion Ratio Lower Upper

124 100

93 8.3 0.0 27.8


62 20.6 0.0 39.0

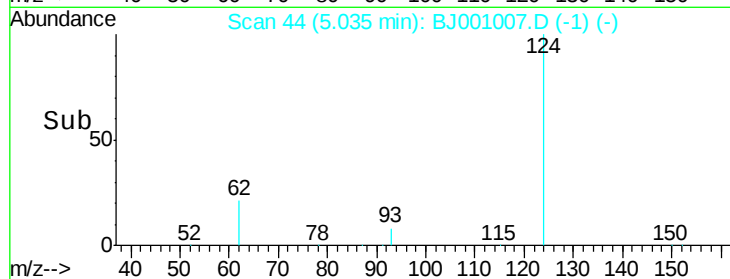

Abundance Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

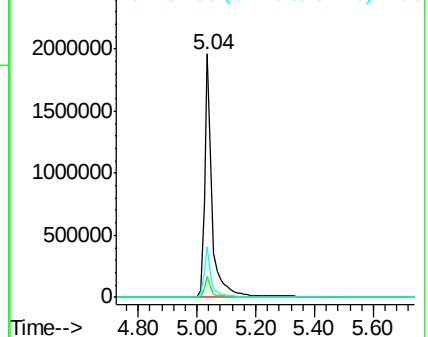

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ071812\
Data File : BJ001007.D
Acq On : 18 Jul 2012 11:41
Operator : HLM
Sample : P4-7
Misc : 10.0ug/mL BNA_J HLM
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
P4-7

Quant Time: Jul 23 01:40:19 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Jul 18 14:01:29 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.64	150	438206	2.50	ug/ml	0.00

System Monitoring Compounds
2) Tripropylphosphate 6.71 99 3549266 14.04 ug/ml -0.01
Spiked Amount 2.500 Range 20 - 150 Recovery = 561.60%#

Target Compounds					Qvalue
3) White Phosphorus	5.04	124	3512932	11.77 ug/ml	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed