



Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ071812\
Data File : BJ001009.D
Acq On : 18 Jul 2012 12:07
Operator : HLM
Sample : P4-5
Misc : 2.5ug/mL BNA_J HLM
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
P4-5

Quant Time: Jul 23 01:40:40 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Jul 18 14:01:29 2012
Response via : Initial Calibration

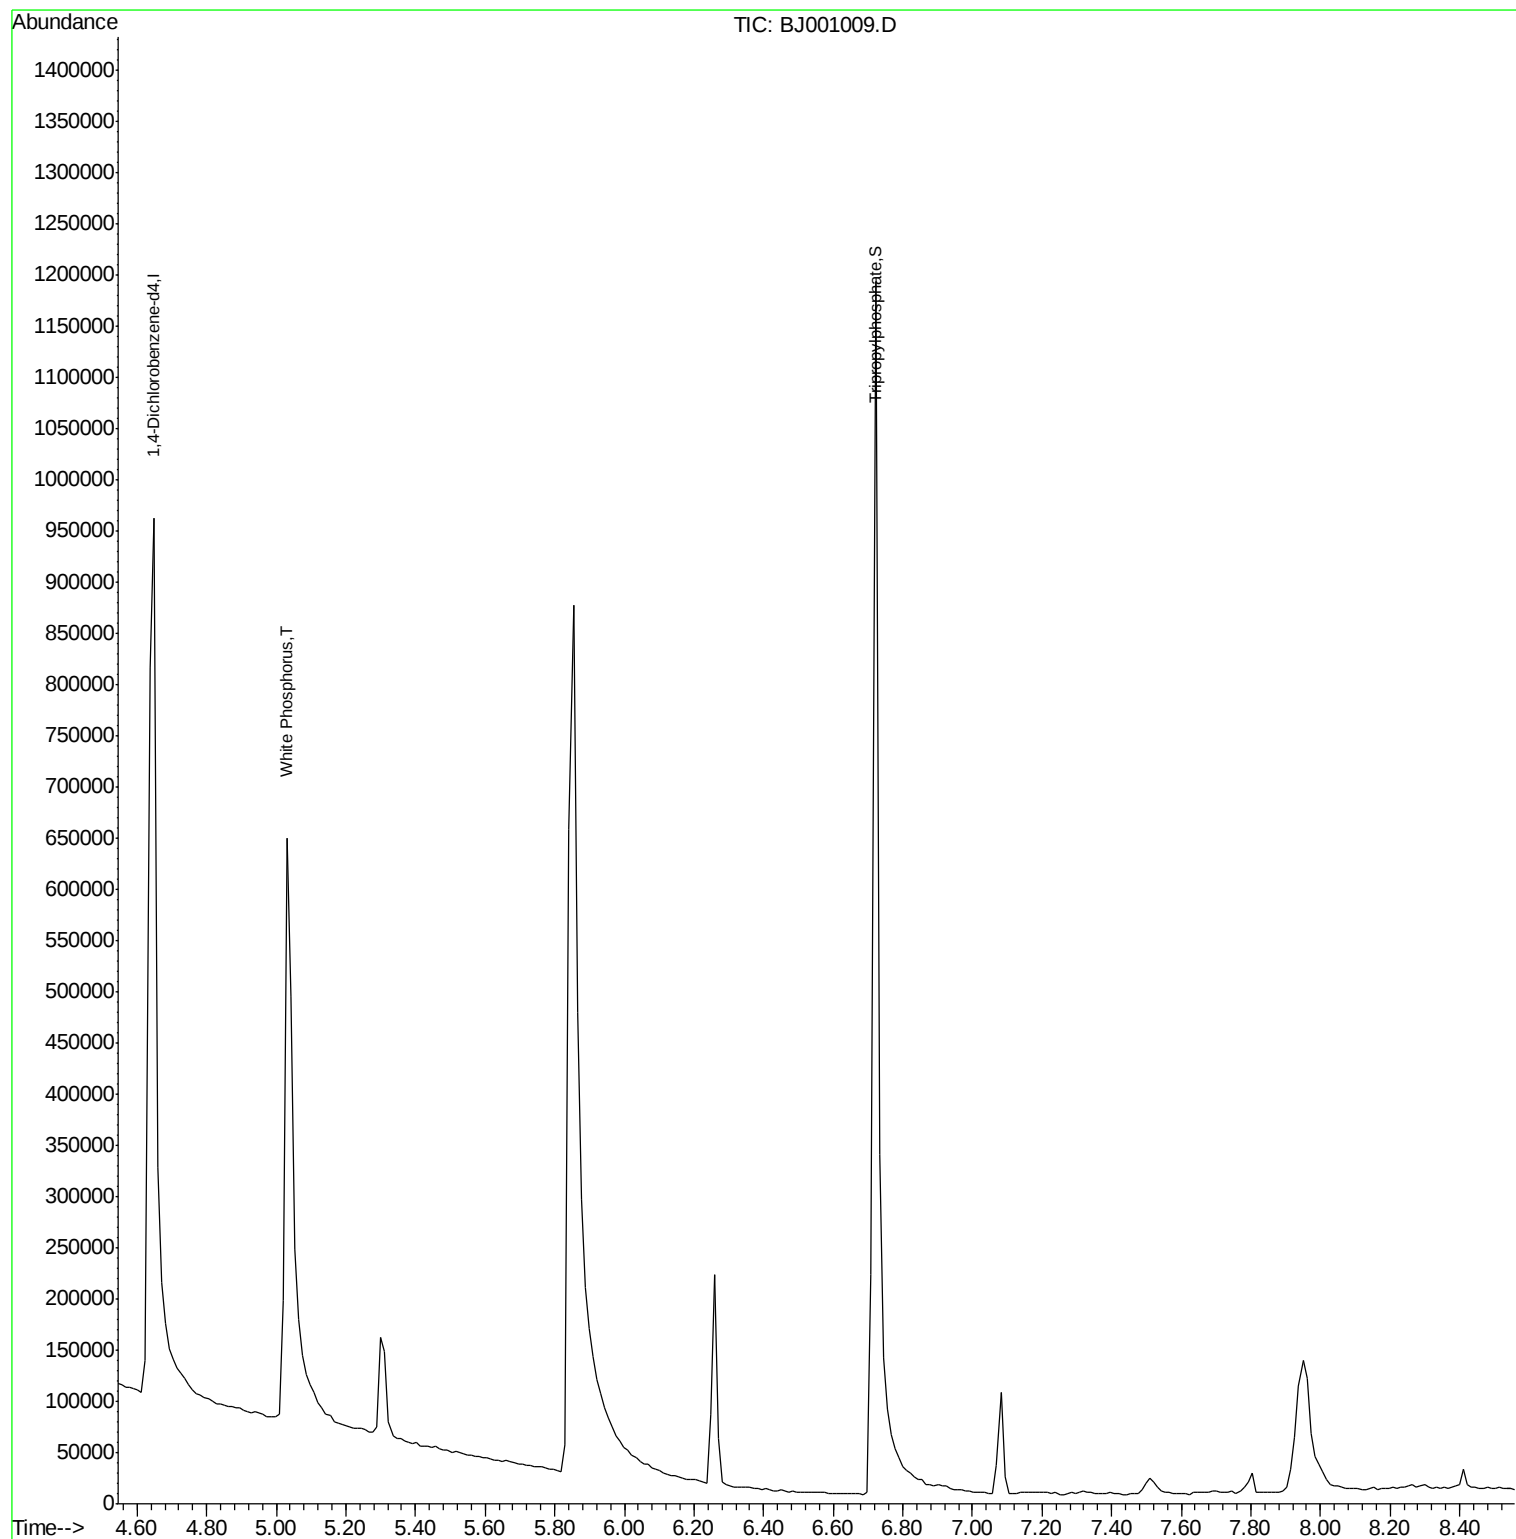

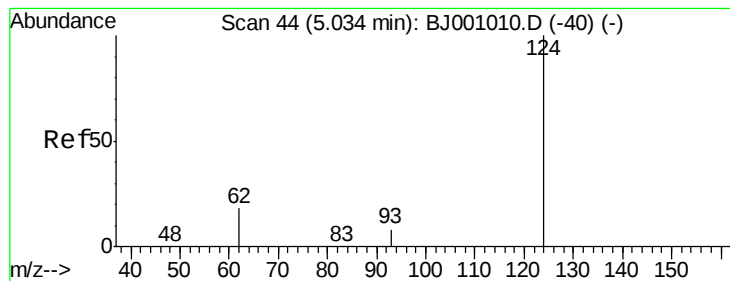

#3

White Phosphorus

Concen: 2.99 ug/ml

RT: 5.03 min Scan# 44

Delta R.T. -0.00 min

Lab File: BJ001009.D


Acq: 18 Jul 2012 12:07

Instrument :

BNA_J

ClientSampleId :

P4-5

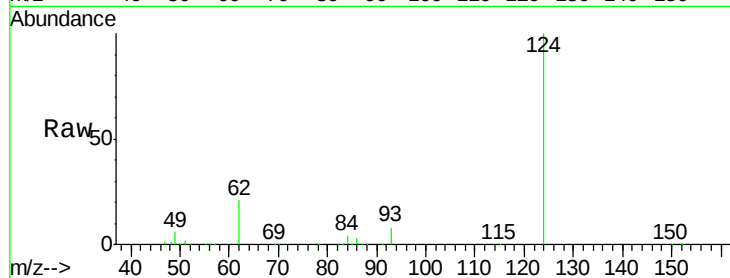


Tgt Ion:124 Resp: 932791

Ion Ratio Lower Upper

124 100

93 7.9 0.0 27.8


62 19.1 0.0 39.0

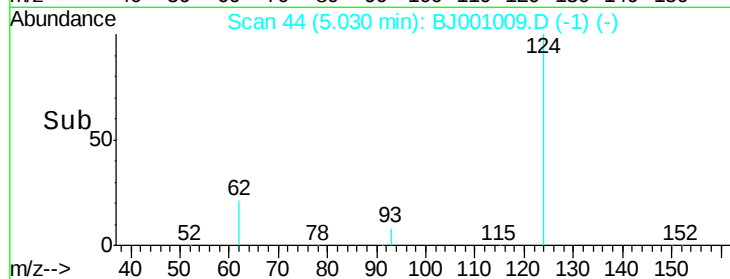

Abundance Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

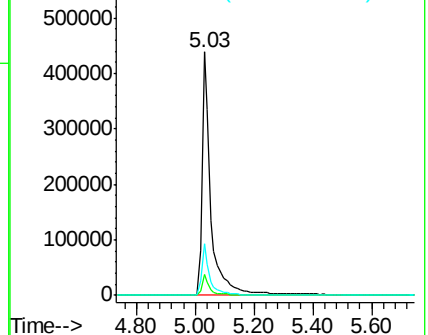

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ071812\
Data File : BJ001009.D
Acq On : 18 Jul 2012 12:07
Operator : HLM
Sample : P4-5
Misc : 2.5ug/mL BNA_J HLM
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
P4-5

Quant Time: Jul 23 01:40:40 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Jul 18 14:01:29 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.65	150	458214	2.50	ug/ml	0.00

System Monitoring Compounds

2) Tripropylphosphate	6.72	99	799409	3.02	ug/ml	0.00
Spiked Amount	2.500	Range	20 - 150	Recovery	=	120.80%

Target Compounds					Qvalue
3) White Phosphorus	5.03	124	932791	2.99	ug/ml 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed