



Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ071812\
Data File : BJ001012.D
Acq On : 18 Jul 2012 12:47
Operator : HLM
Sample : P4-2
Misc : 0.25ug/mL BNA_J HLM
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
P4-2

Quant Time: Jul 23 01:29:32 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Jul 18 14:01:29 2012
Response via : Initial Calibration

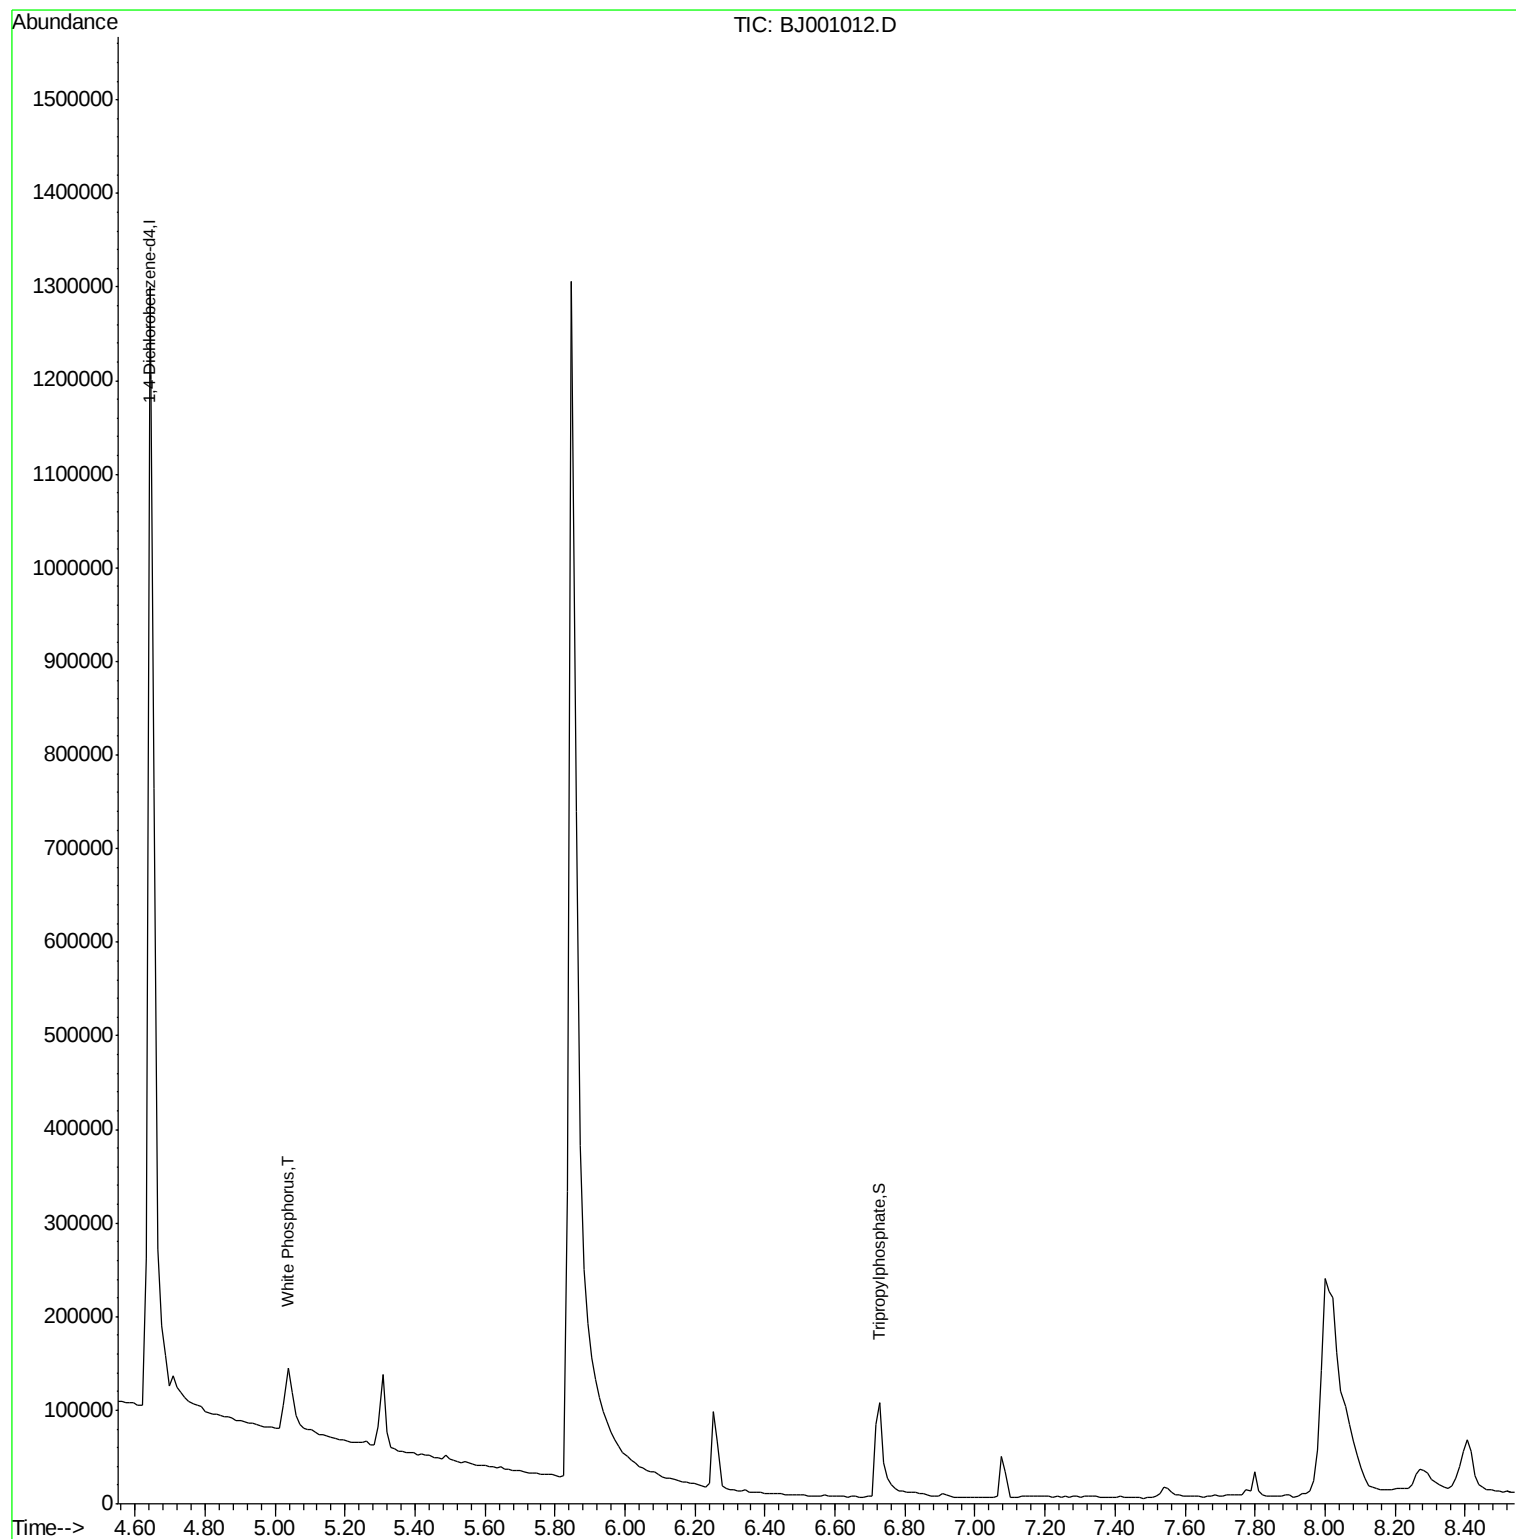

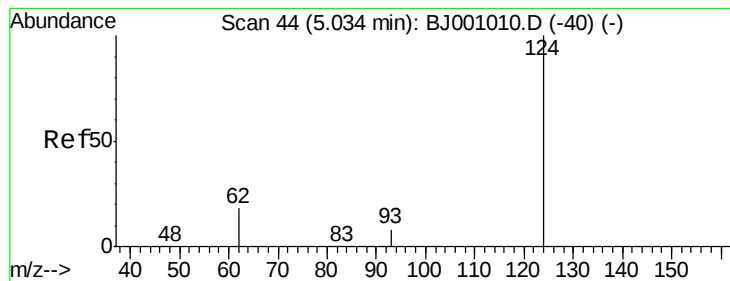

#3

White Phosphorus

Concen: 0.32 ug/ml

RT: 5.04 min Scan# 44

Delta R.T. 0.00 min

Lab File: BJ001012.D


Acq: 18 Jul 2012 12:47

Instrument :

BNA_J

ClientSampleId :

P4-2

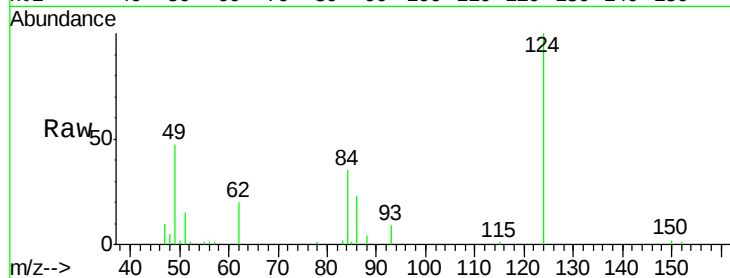


Tgt Ion:124 Resp: 111362

Ion Ratio Lower Upper

124 100

93 7.5 0.0 27.8


62 18.9 0.0 39.0

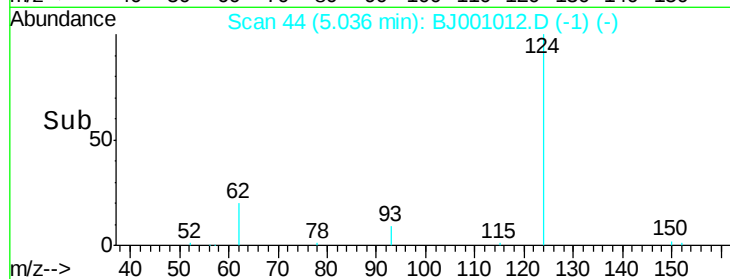

Abundance Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

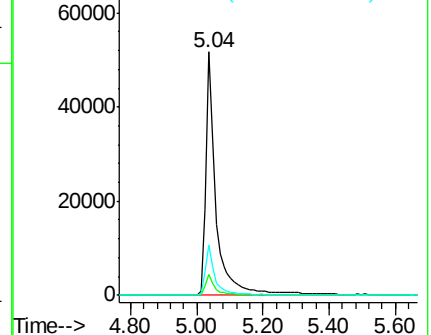

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ071812\
Data File : BJ001012.D
Acq On : 18 Jul 2012 12:47
Operator : HLM
Sample : P4-2
Misc : 0.25ug/mL BNA_J HLM
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
P4-2

Quant Time: Jul 23 01:29:32 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Jul 18 14:01:29 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.64	150	516590	2.50	ug/ml	0.00

System Monitoring Compounds

2) Tripropylphosphate	6.73	99	106989	0.36	ug/ml	0.00
Spiked Amount	2.500	Range	20 - 150	Recovery	=	14.40%#

Target Compounds					Qvalue
3) White Phosphorus	5.04	124	111362	0.32	ug/ml 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed