



Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ071812\
Data File : BJ001013.D
Acq On : 18 Jul 2012 13:00
Operator : HLM
Sample : P4-1
Misc : 0.10ug/mL BNA_J HLM
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
P4-1

Quant Time: Jul 19 04:22:46 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Jul 18 14:01:29 2012
Response via : Initial Calibration

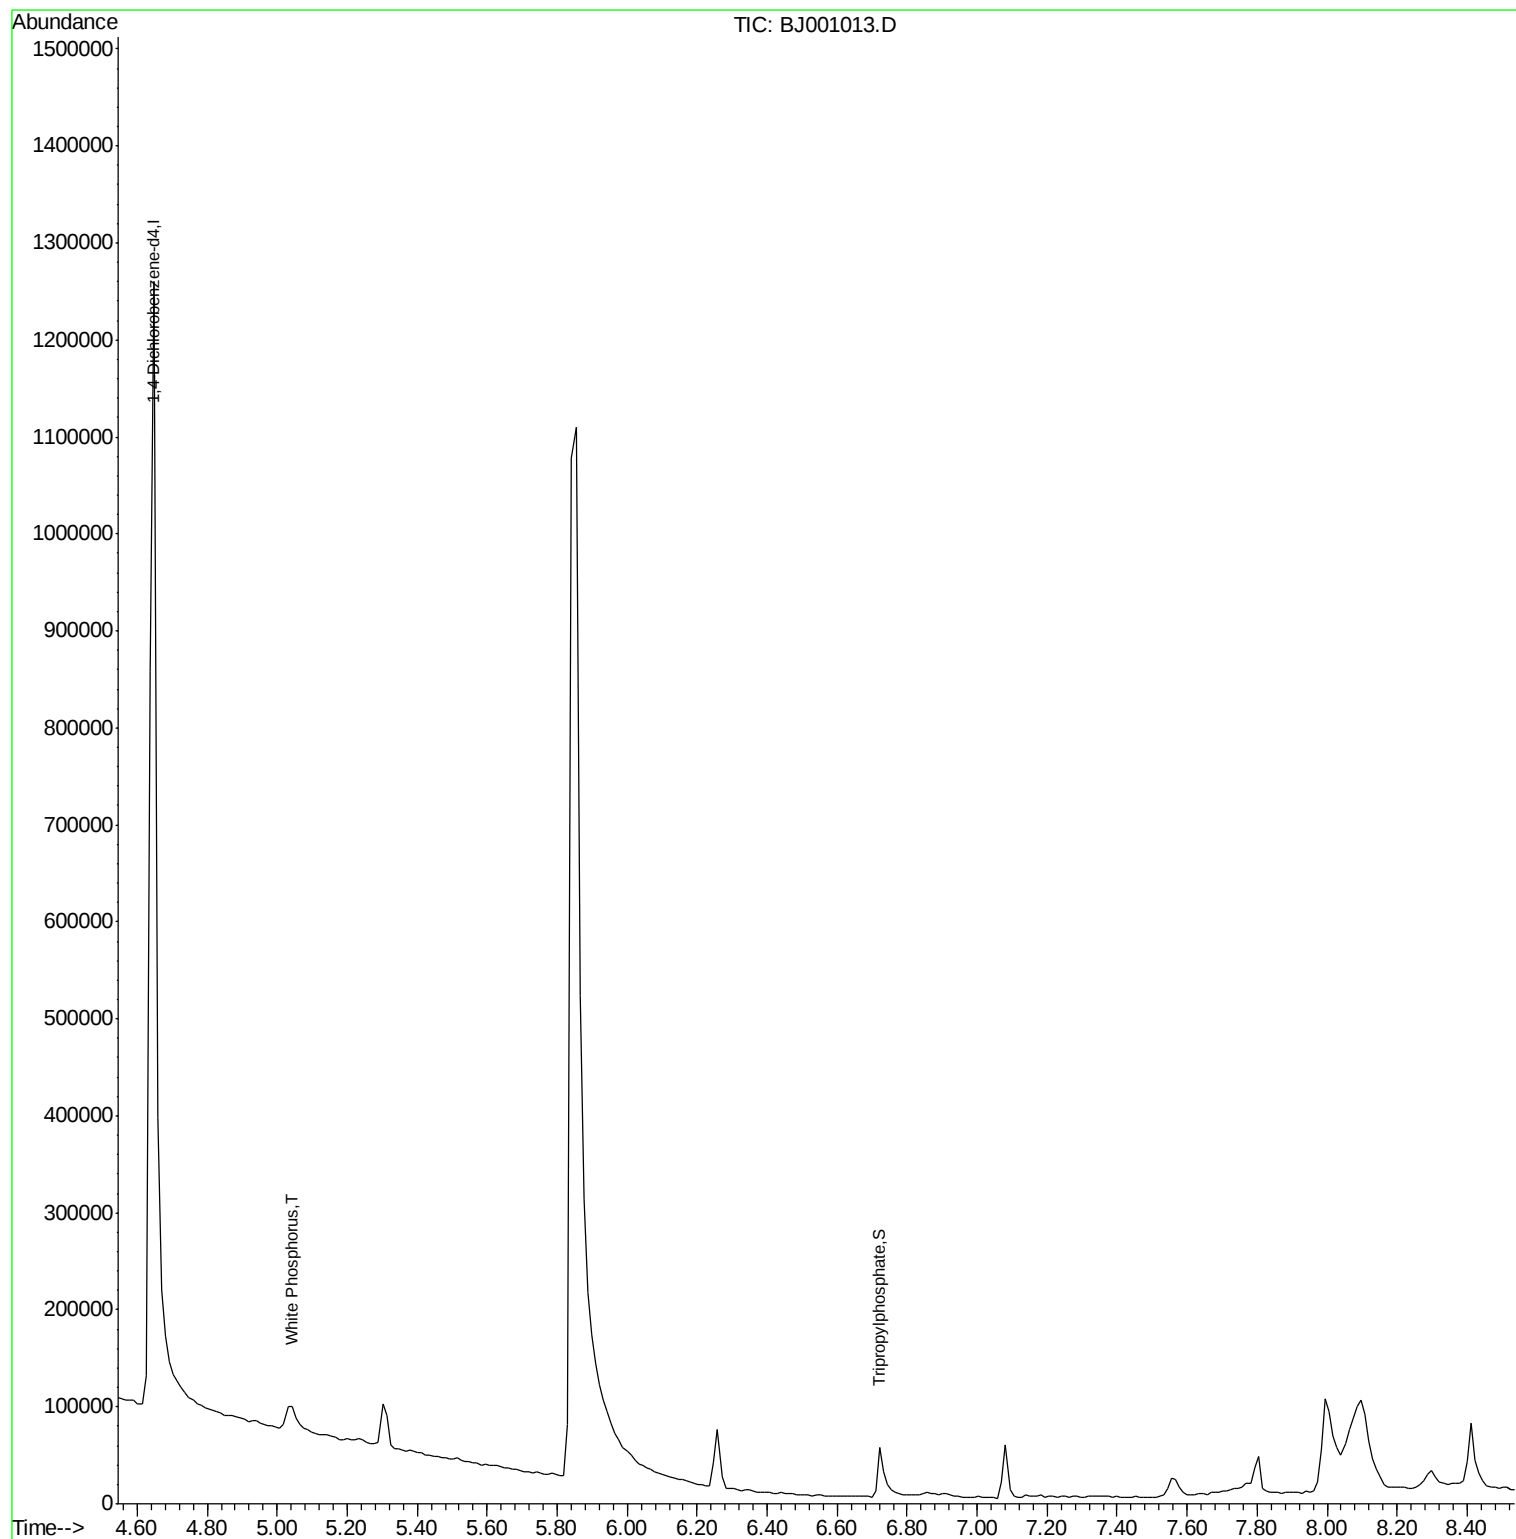

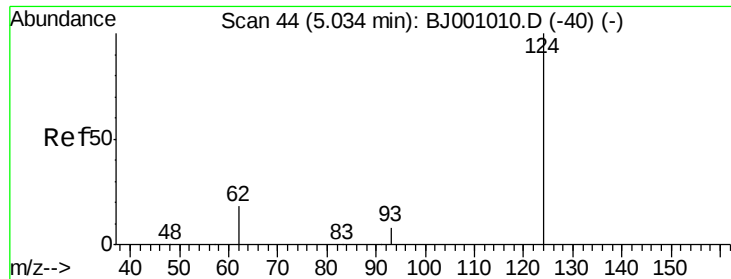

#3

White Phosphorus

Concen: 0.12 ug/ml

RT: 5.04 min Scan# 45

Delta R.T. 0.01 min

Lab File: BJ001013.D

Acq: 18 Jul 2012 13:00

Instrument :

BNA_J

ClientSampleId :

P4-1



Tgt Ion:124 Resp: 45524

Ion Ratio Lower Upper

124 100

93 6.7 0.0 27.8


62 20.1 0.0 39.0

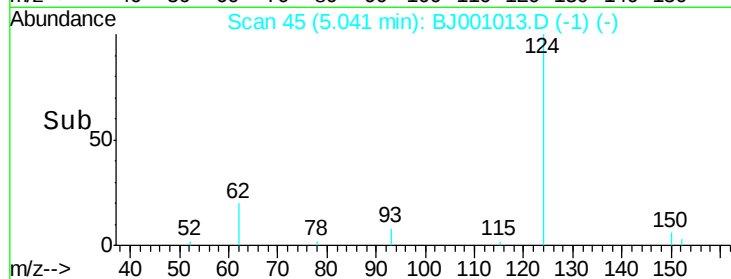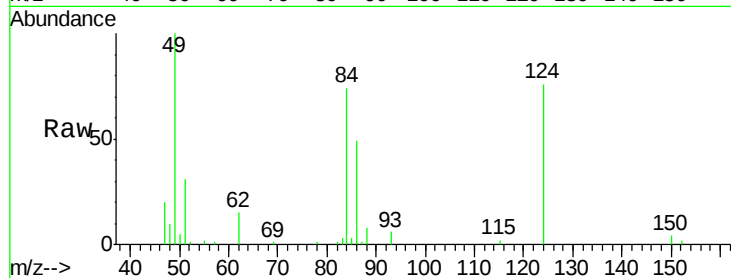

Abundance Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

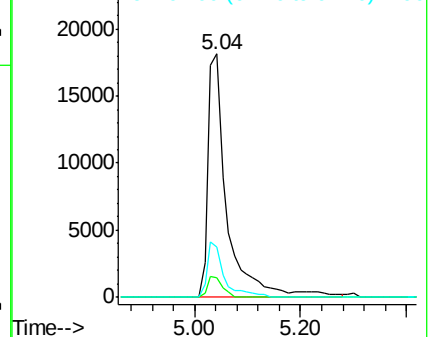

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ071812\
Data File : BJ001013.D
Acq On : 18 Jul 2012 13:00
Operator : HLM
Sample : P4-1
Misc : 0.10ug/mL BNA_J HLM
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
P4-1

Quant Time: Jul 19 04:22:46 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Jul 18 14:01:29 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.65	150	542960	2.50	ug/ml	0.00

System Monitoring Compounds

2) Tripropylphosphate	6.72	99	48608	0.16	ug/ml	0.00
Spiked Amount	2.500	Range	20 - 150	Recovery	=	6.40%#

Target Compounds					Qvalue
3) White Phosphorus	5.04	124	45524	0.12	ug/ml 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed